
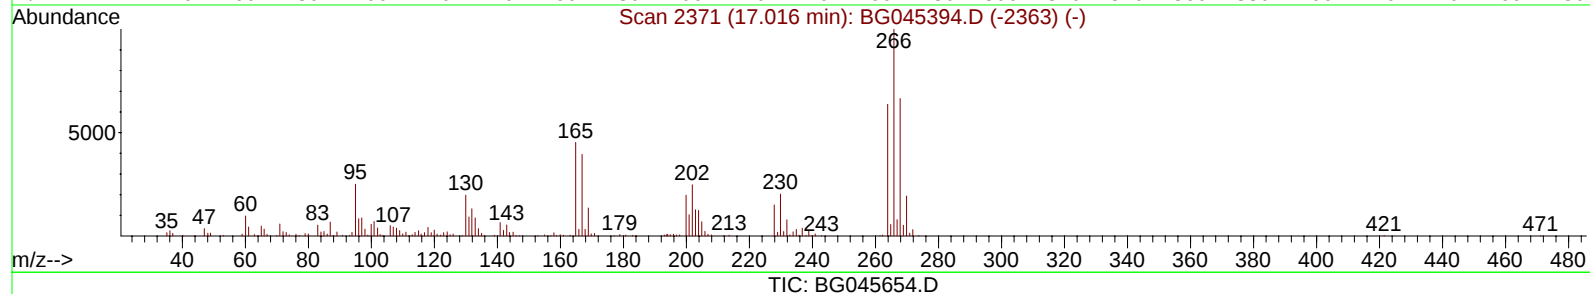
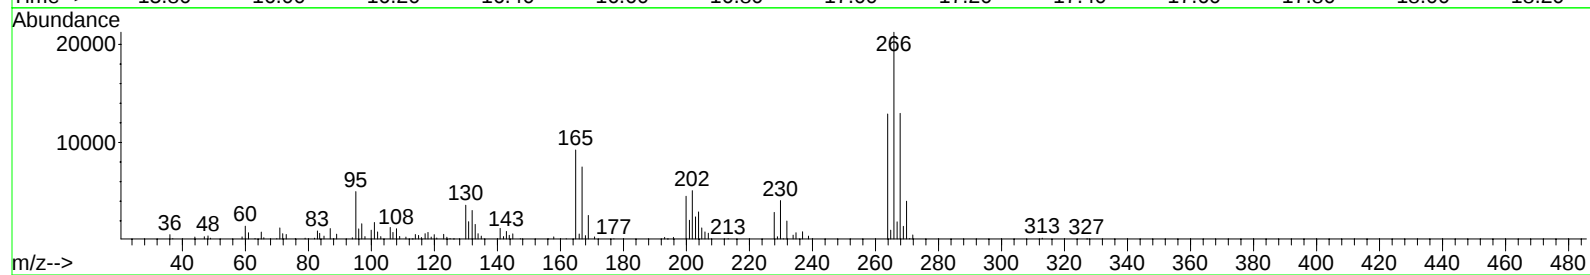


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060920\
Data File : BG045654.D
Acq On : 9 Jun 2020 8:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 16:42:02 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 01 15:07:00 2020
Response via : Initial Calibration

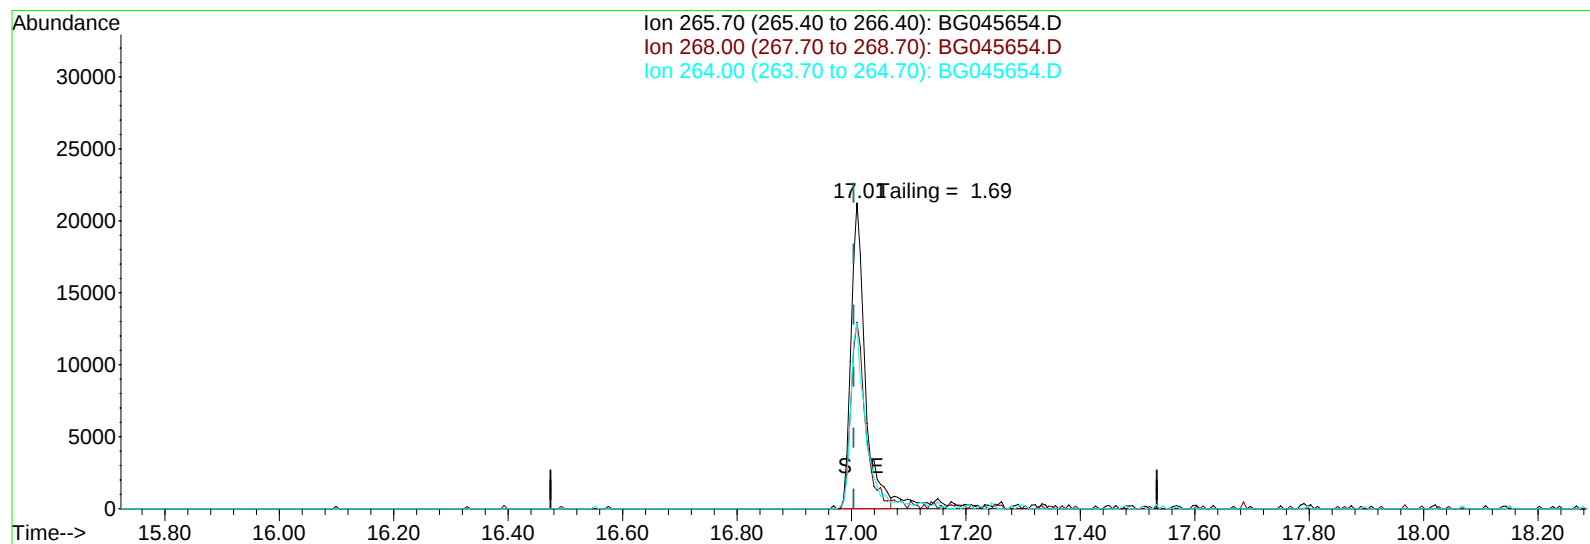

(70) Pentachlorophenol (C)




17.010min (+0.006) 10204.26ng

response 37145

Ion	Exp%	Act%
265.70	100	100
268.00	66.50	61.02
264.00	63.70	60.70
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060920\
Data File : BG045654.D
Acq On : 9 Jun 2020 8:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 16:42:02 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 01 15:07:00 2020
Response via : Initial Calibration

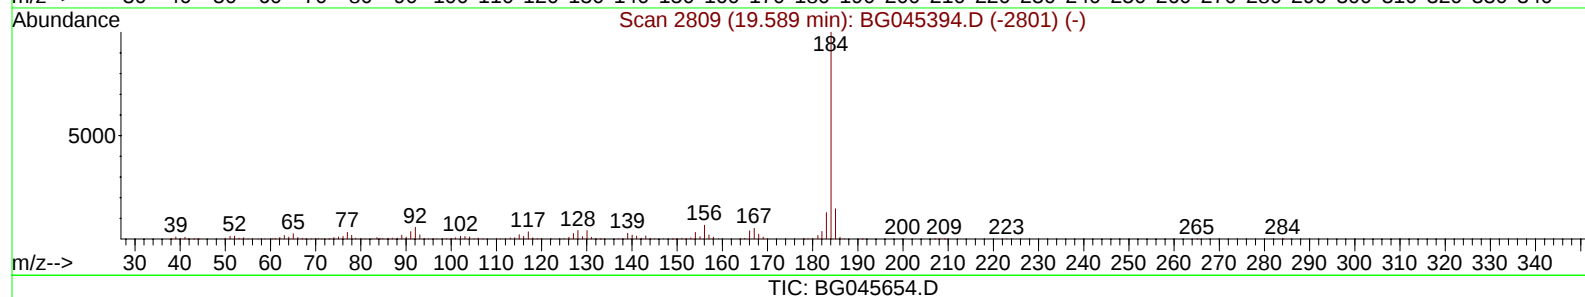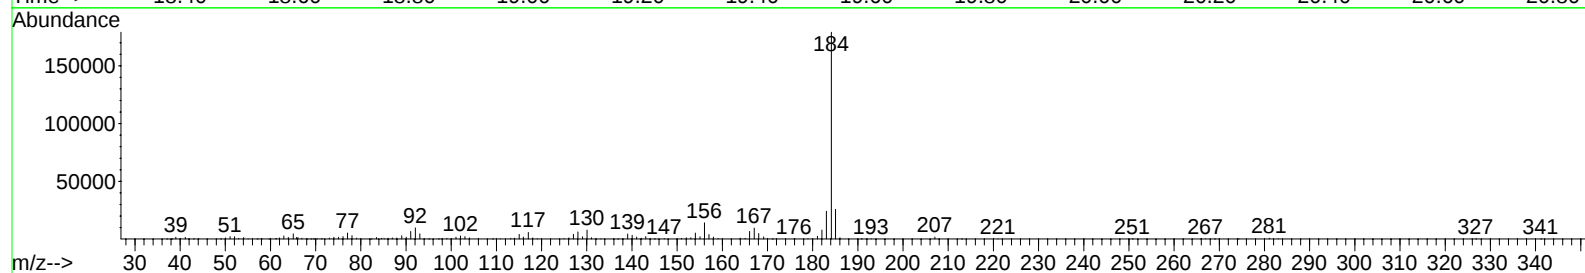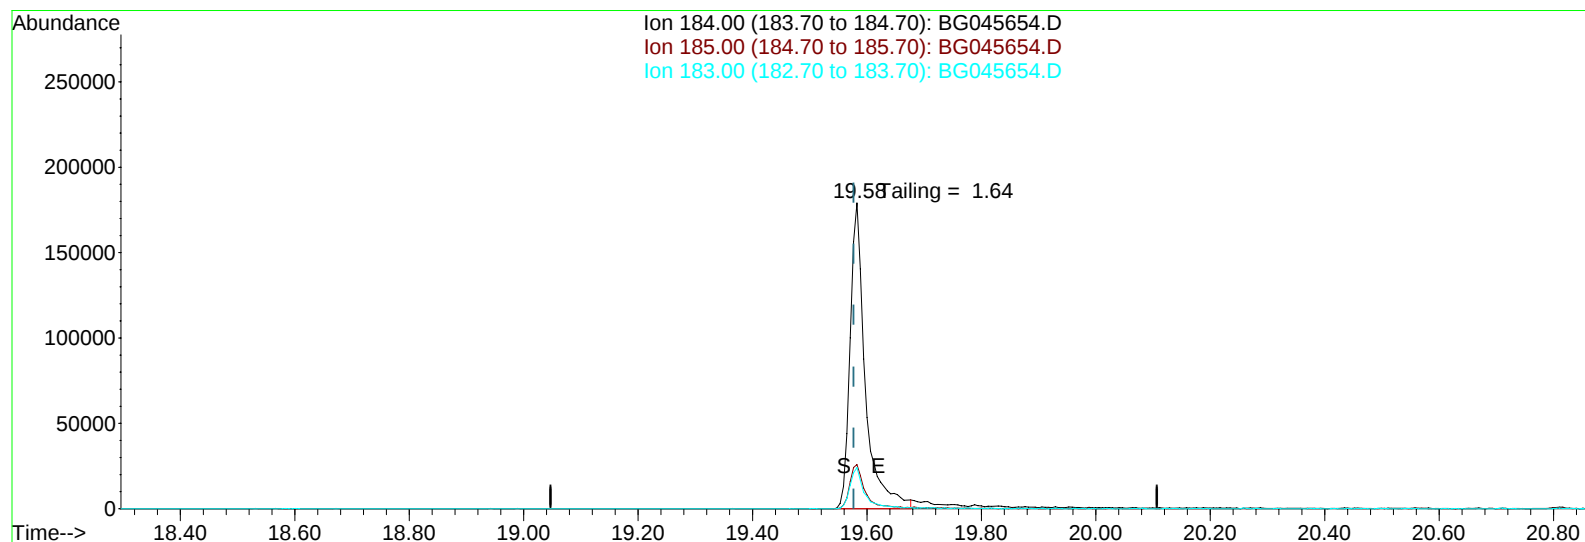

(77) Benzidine

19.583min (+0.006) 10716.41ng

response 345520

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	14.42
183.00	12.80	13.47
0.00	0.00	0.00