
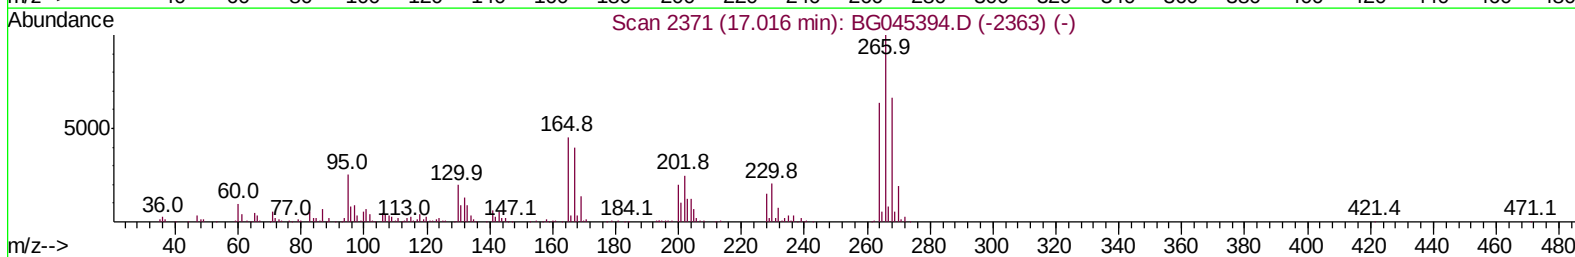
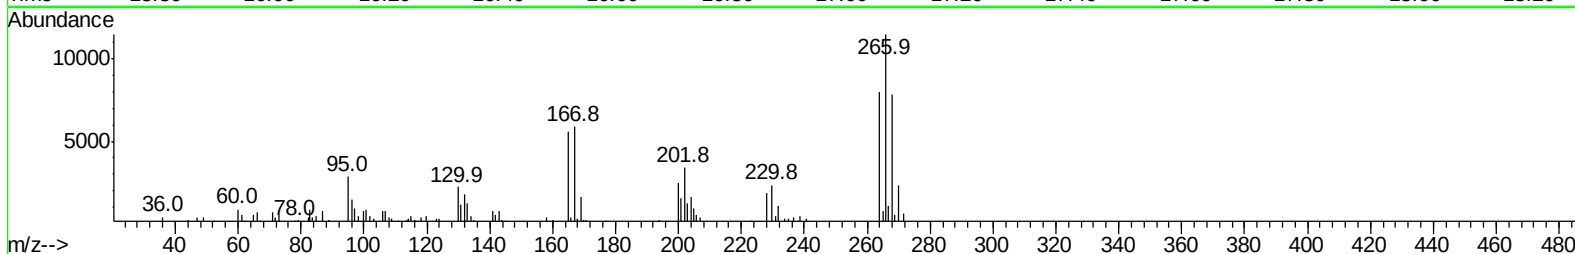


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG060920\
Data File : BG045671.D
Acq On : 9 Jun 2020 21:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 22:36:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 01 15:07:00 2020
Response via : Initial Calibration

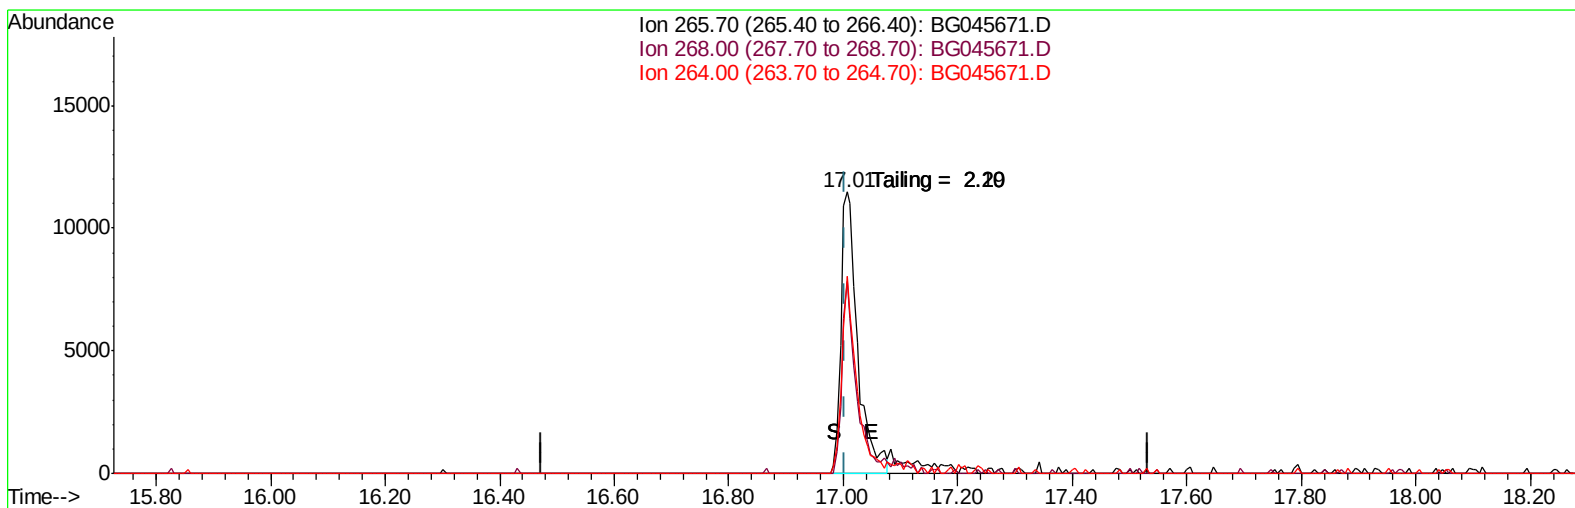

TIC: BG045671.D

(70) Pentachlorophenol (C)




17.007min (+0.003) 72453.33ng

response 22582

Ion	Exp%	Act%
265.70	100	100
268.00	66.50	68.18
264.00	63.70	69.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG060920\
 Data File : BG045671.D
 Acq On : 9 Jun 2020 21:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 22:36:50 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 01 15:07:00 2020
 Response via : Initial Calibration

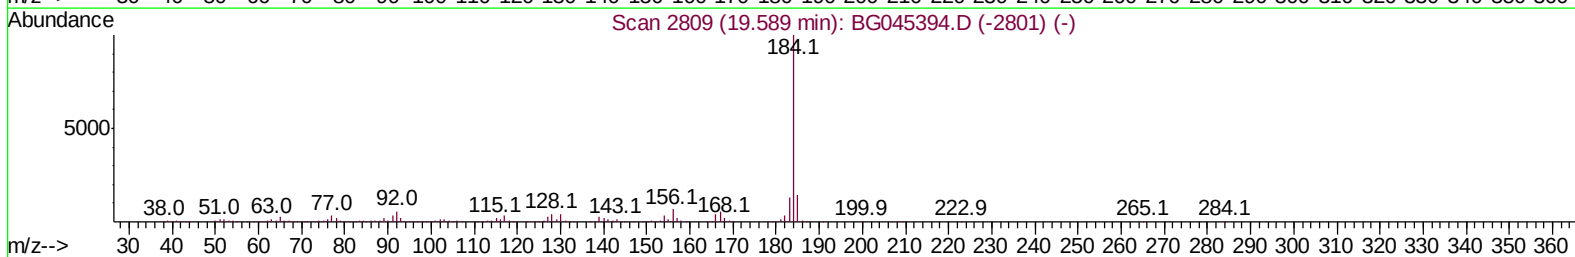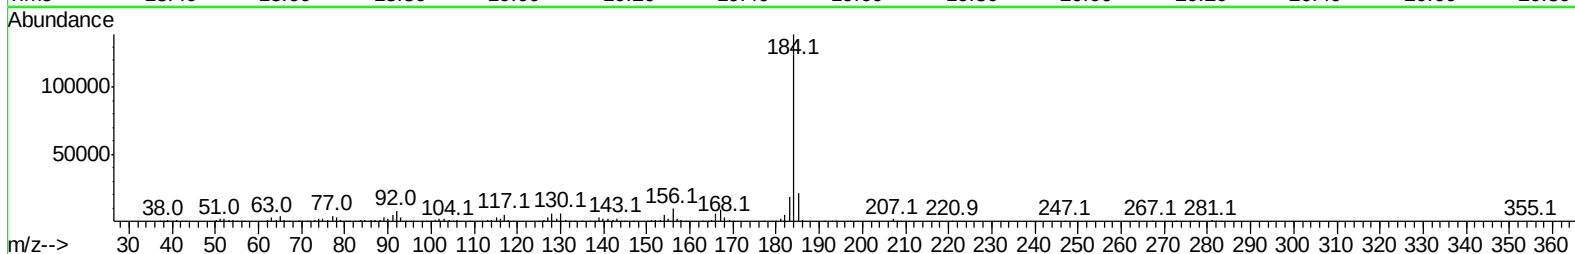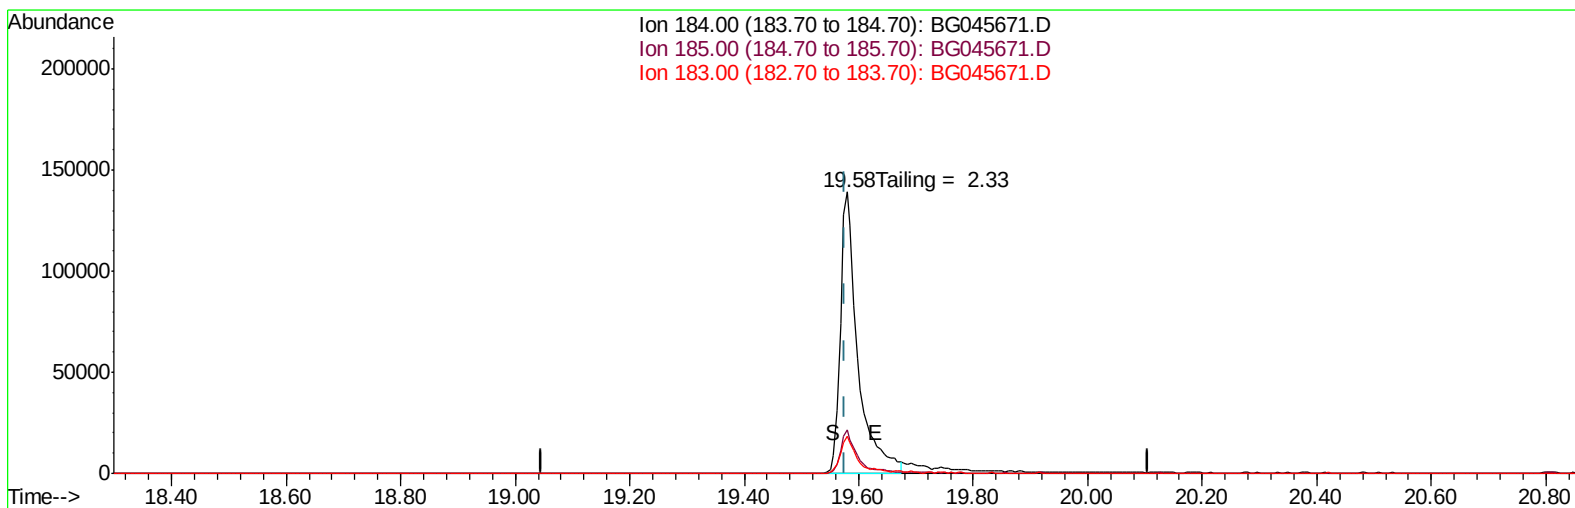

TIC: BG045671.D

(77) Benzidine

19.580min (+0.003) 142904.17ng

response 301015

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	15.39
183.00	12.80	13.22
0.00	0.00	0.00