


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060920\
 Data File : BG045654.D
 Acq On : 9 Jun 2020 8:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG051520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 01 15:07:00 2020

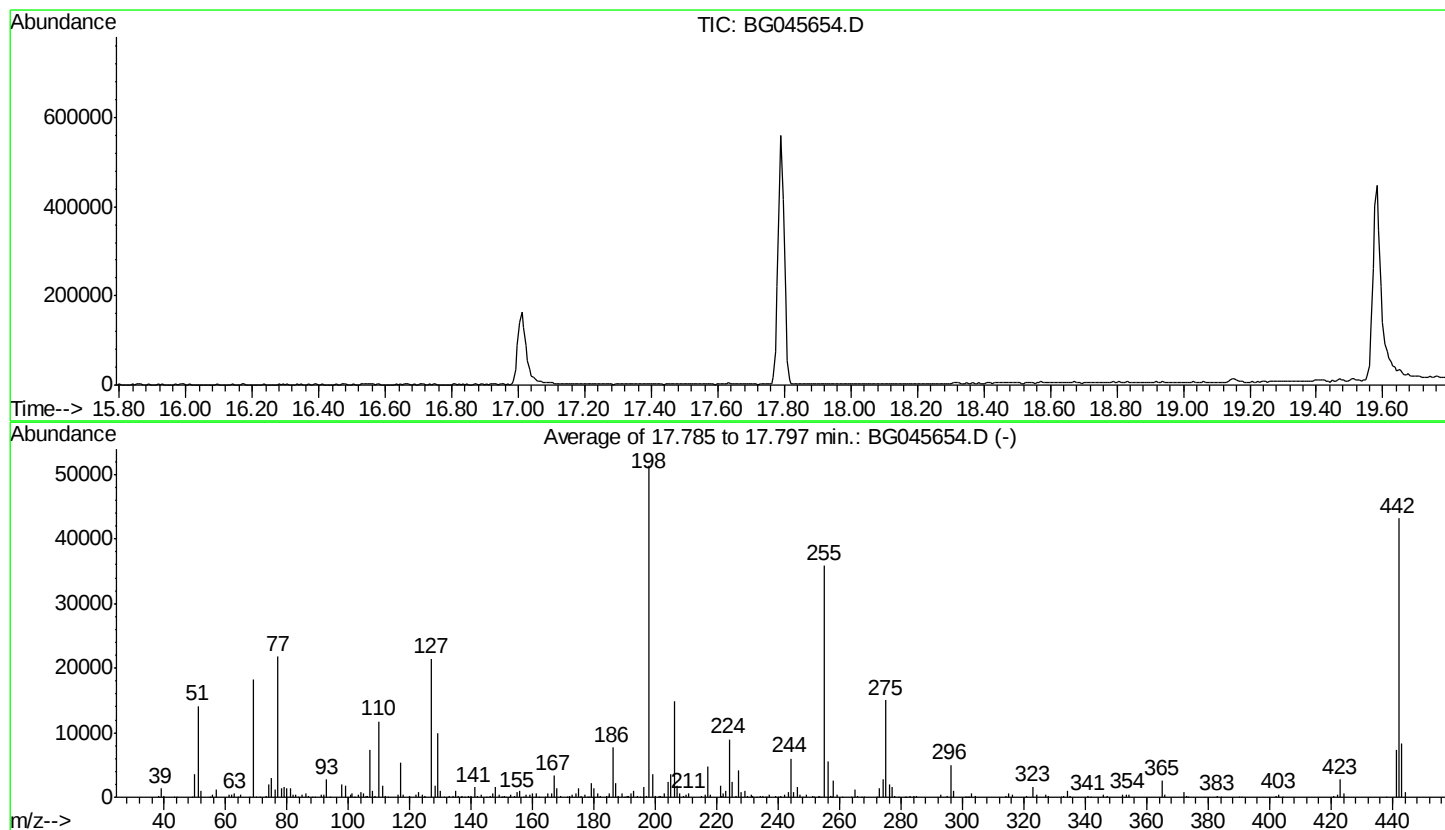

AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.5	14110	PASS
68	69	0.00	2	0.4	74	PASS
69	198	0.00	100	35.7	18316	PASS
70	69	0.00	2	0.3	52	PASS
127	198	10	80	41.8	21485	PASS
197	198	0.00	2	0.5	243	PASS
198	198	100	100	100.0	51370	PASS
199	198	5	9	7.0	3609	PASS
275	198	10	60	29.3	15064	PASS
365	198	1	100	4.9	2538	PASS
441	198	0.01	100	14.4	7377	PASS
442	198	50	100	84.1	43208	PASS
443	442	15	24	19.2	8308	PASS