
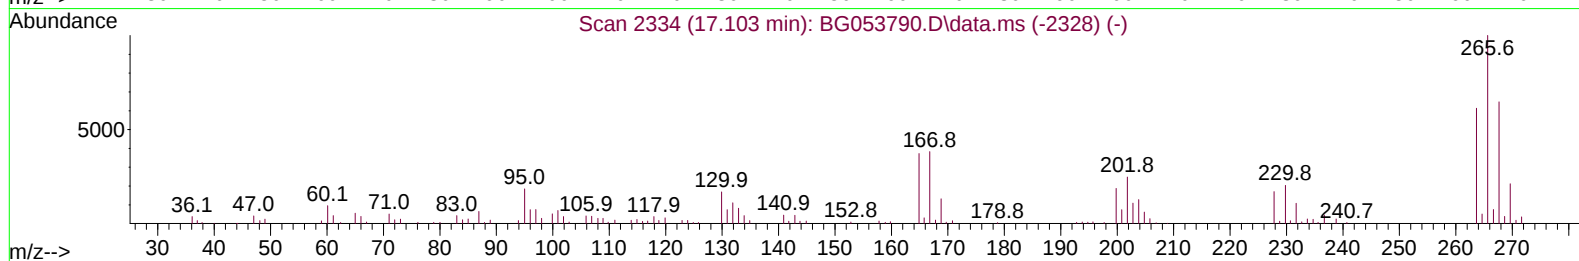
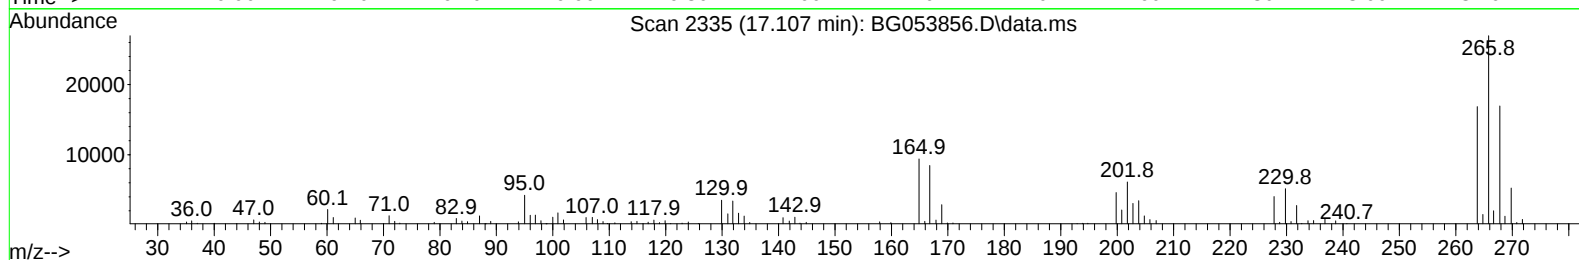


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060922\
Data File : BG053856.D
Acq On : 9 Jun 2022 10:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 14:54:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 23:22:27 2022
Response via : Initial Calibration

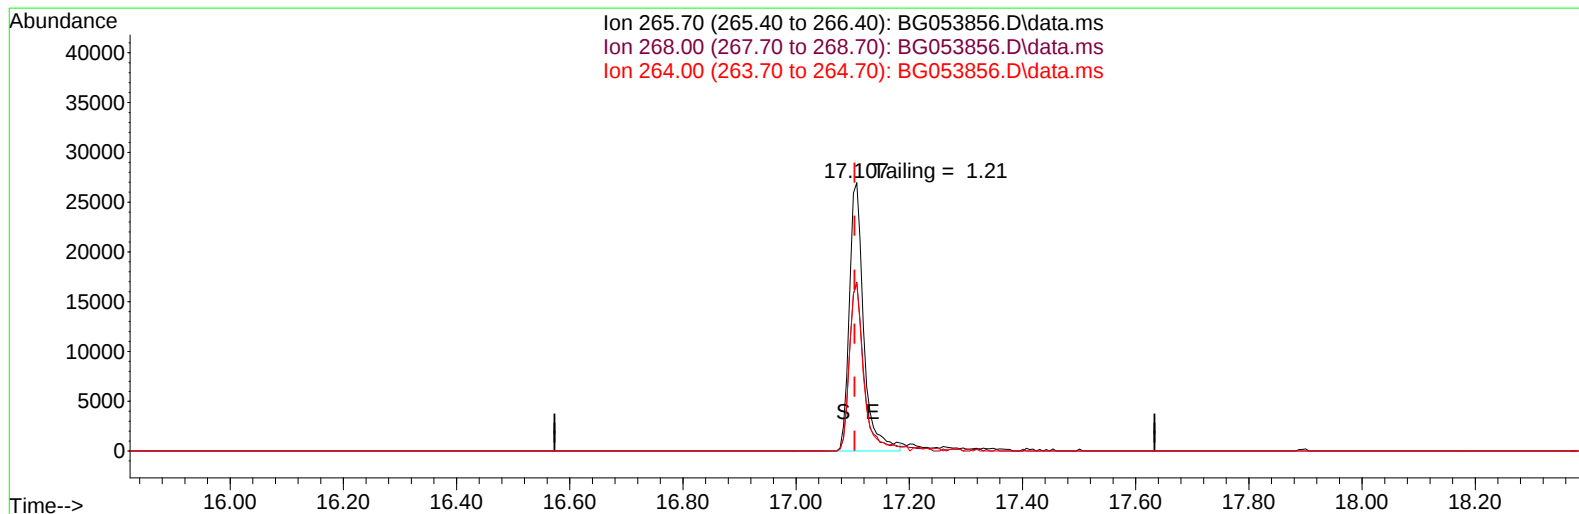

TIC: BG053856.D\data.ms

(70) Pentachlorophenol (C)




17.107min (+ 0.004) 35740.44 ng

response 47157

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	67.42
264.00	66.20	62.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060922\
 Data File : BG053856.D
 Acq On : 9 Jun 2022 10:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 14:54:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 02 23:22:27 2022
 Response via : Initial Calibration

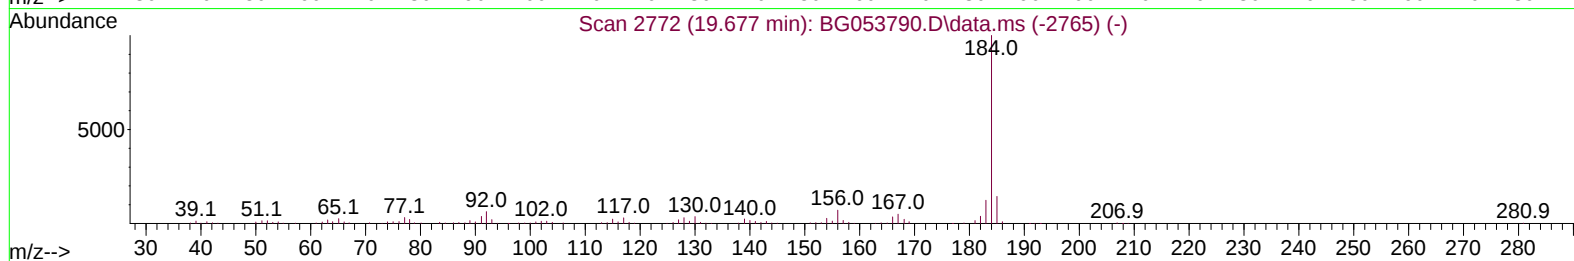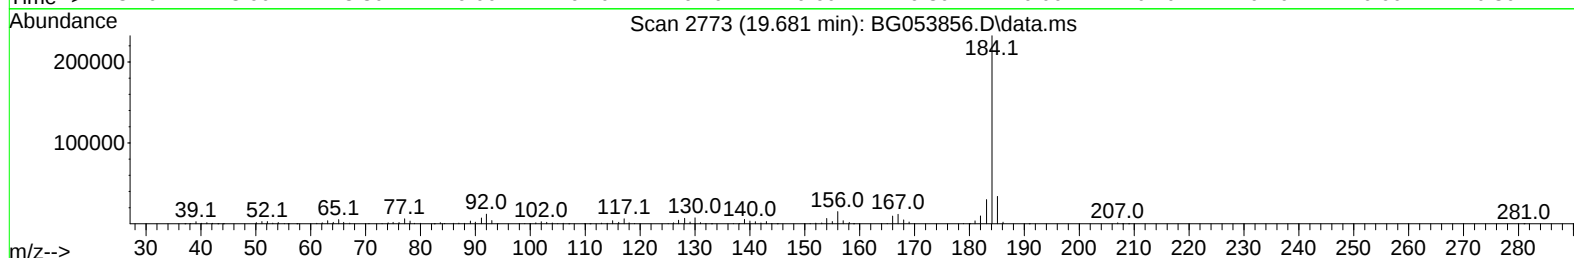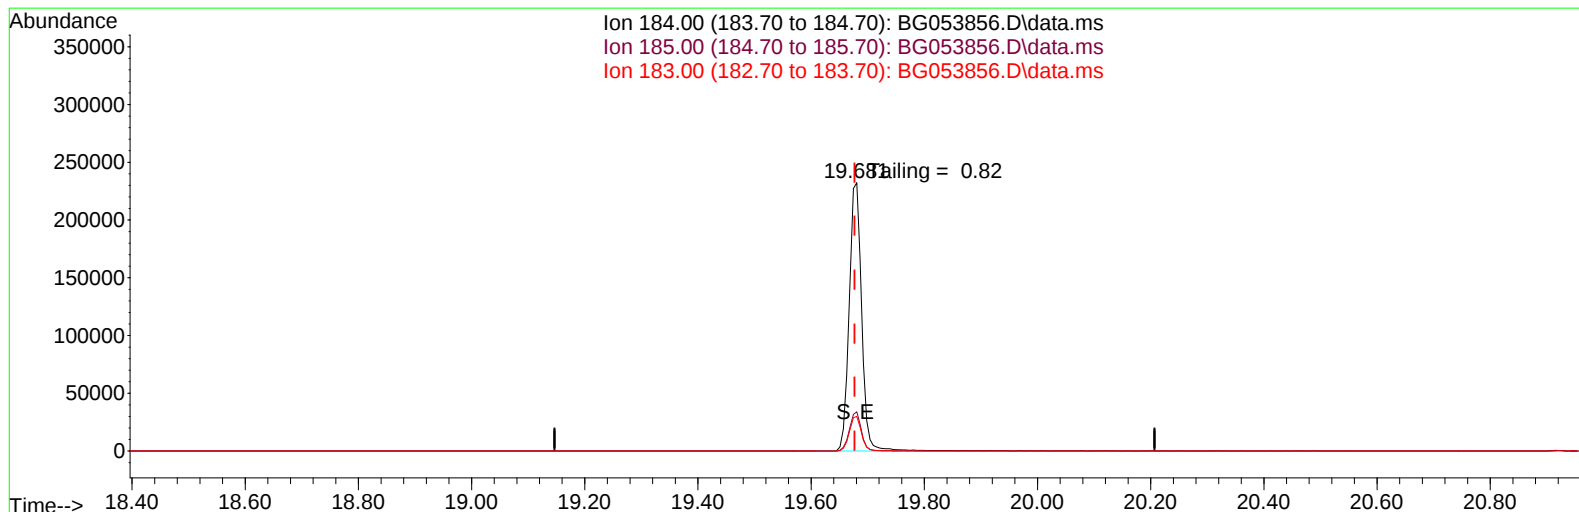

TIC: BG053856.D\data.ms

(77) Benzidine

19.681min (+ 0.004) 0.00 ng

response 352678

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.64
183.00	11.10	12.92
0.00	0.00	0.00