


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060922\
 Data File : BG053856.D
 Acq On : 9 Jun 2022 10:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 02 23:22:27 2022

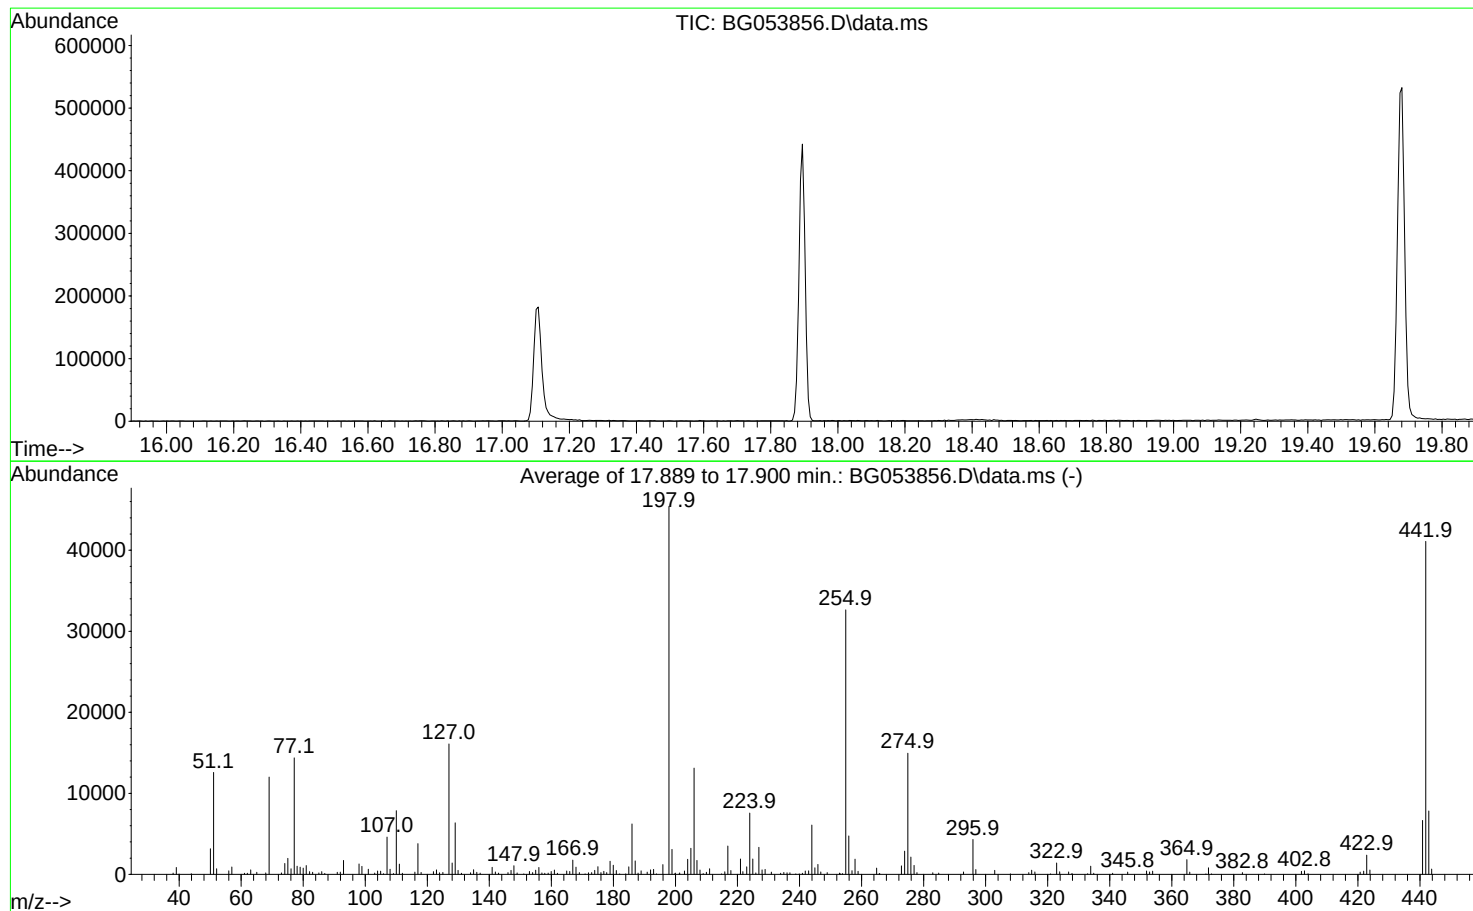




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.7	12572	PASS
68	69	0.00	2	1.5	186	PASS
69	198	0.00	100	26.5	12008	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	35.5	16096	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45395	PASS
199	198	5	9	6.8	3086	PASS
275	198	10	60	32.9	14943	PASS
365	198	1	100	4.0	1826	PASS
441	198	0.01	100	14.6	6650	PASS
442	442	50	100	100.0	41083	PASS
443	442	15	24	19.1	7829	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060922\
Data File : BG053856.D
Acq On : 9 Jun 2022 10:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 09 14:54:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 23:22:27 2022
Response via : Initial Calibration

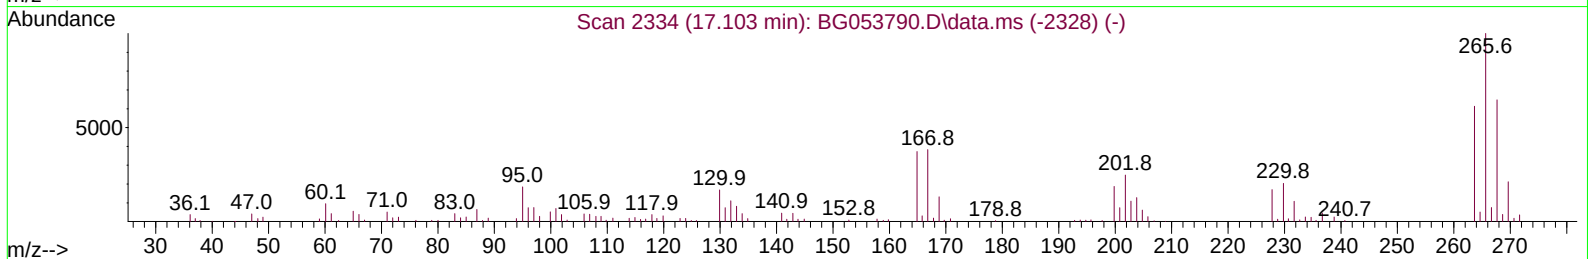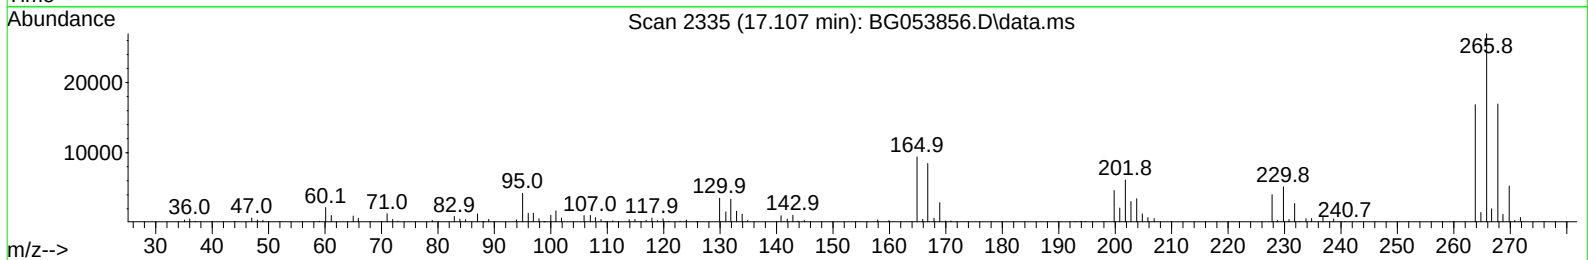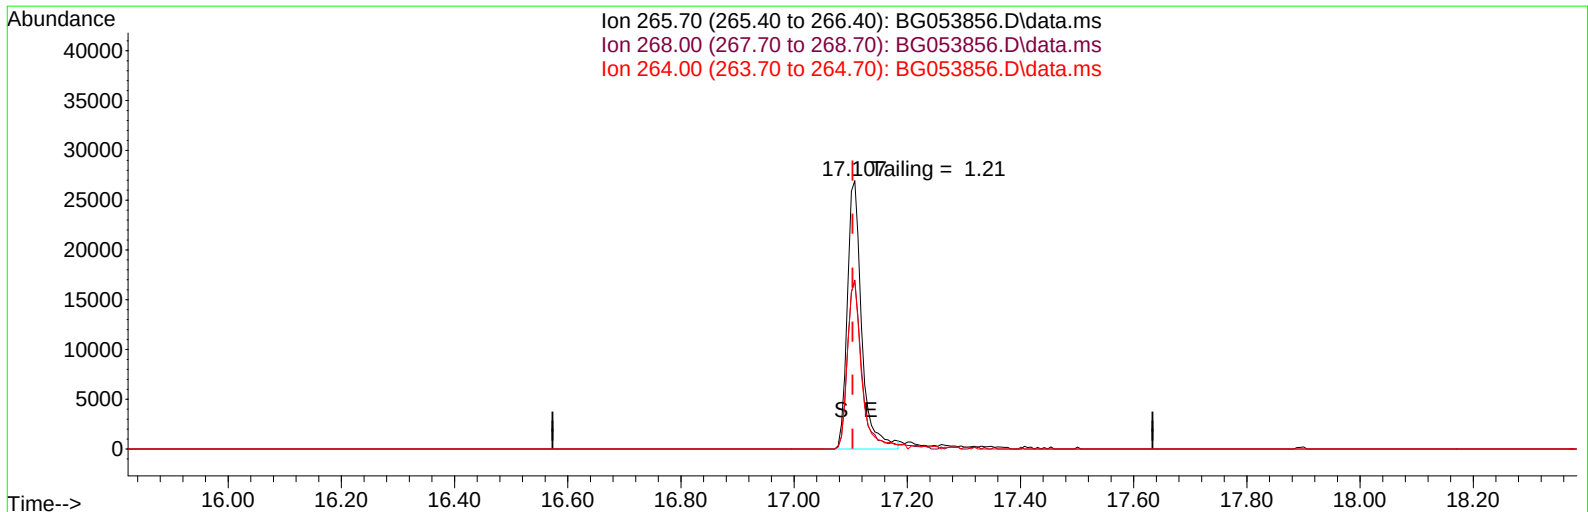

TIC: BG053856.D\data.ms

(70) Pentachlorophenol (C)

17.107min (+ 0.004) 35740.44 ng




response 47157

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	67.42
264.00	66.20	62.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060922\
Data File : BG053856.D
Acq On : 9 Jun 2022 10:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 09 14:54:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 23:22:27 2022
Response via : Initial Calibration

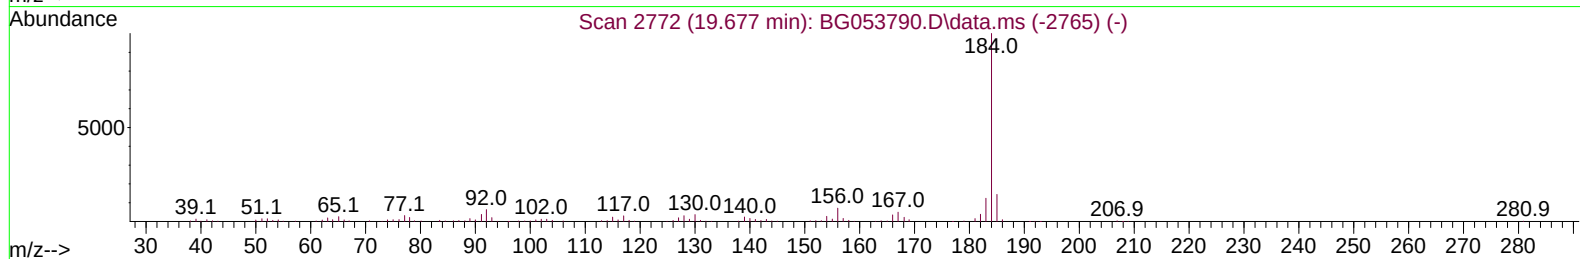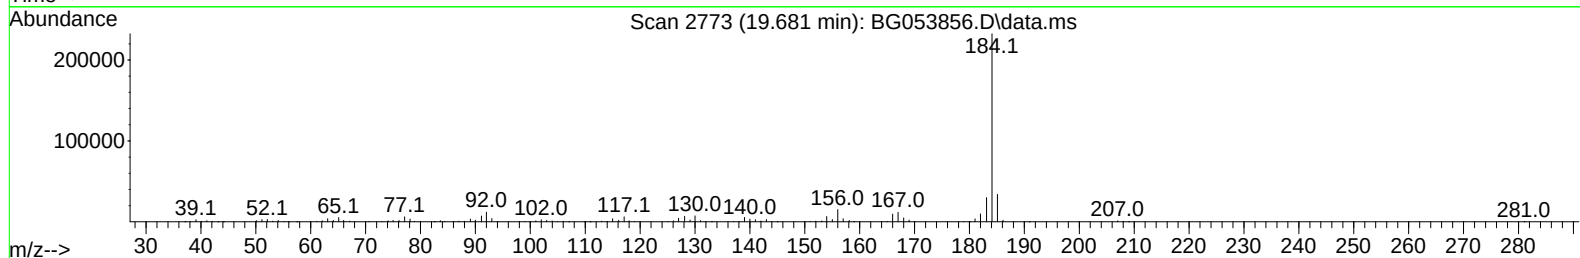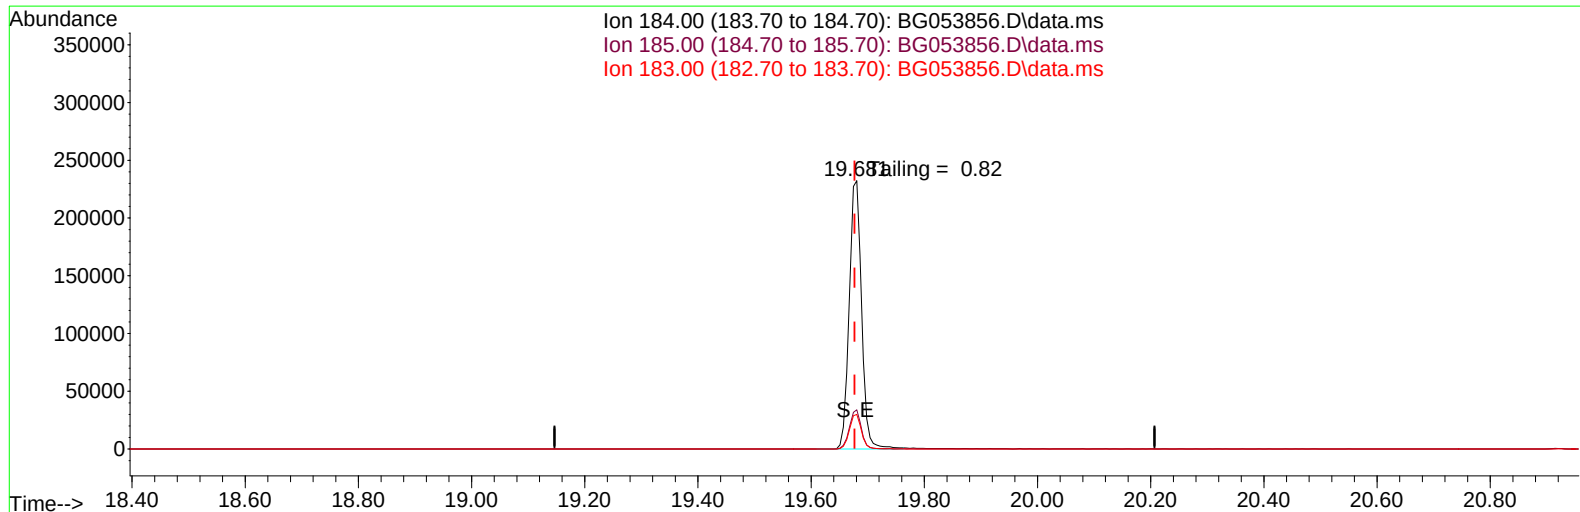

TIC: BG053856.D\data.ms

(77) Benzidine

19.681min (+ 0.004) 0.00 ng

response 352678

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.64
183.00	11.10	12.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/9/2022	BNA_G	<u>BG053856.D</u>
Compound Name	Response	Retention Time
DDT	180761	20.92
DDD	1278	20.47
DDE	59	19.97
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1337	182098	0.73

Instrument :
BNA_G
ClientSampleId :
DFTPP