


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061015\
Data File : BG017600.D
Acq On : 10 Jun 2015 11:15
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 09 15:11:40 2015

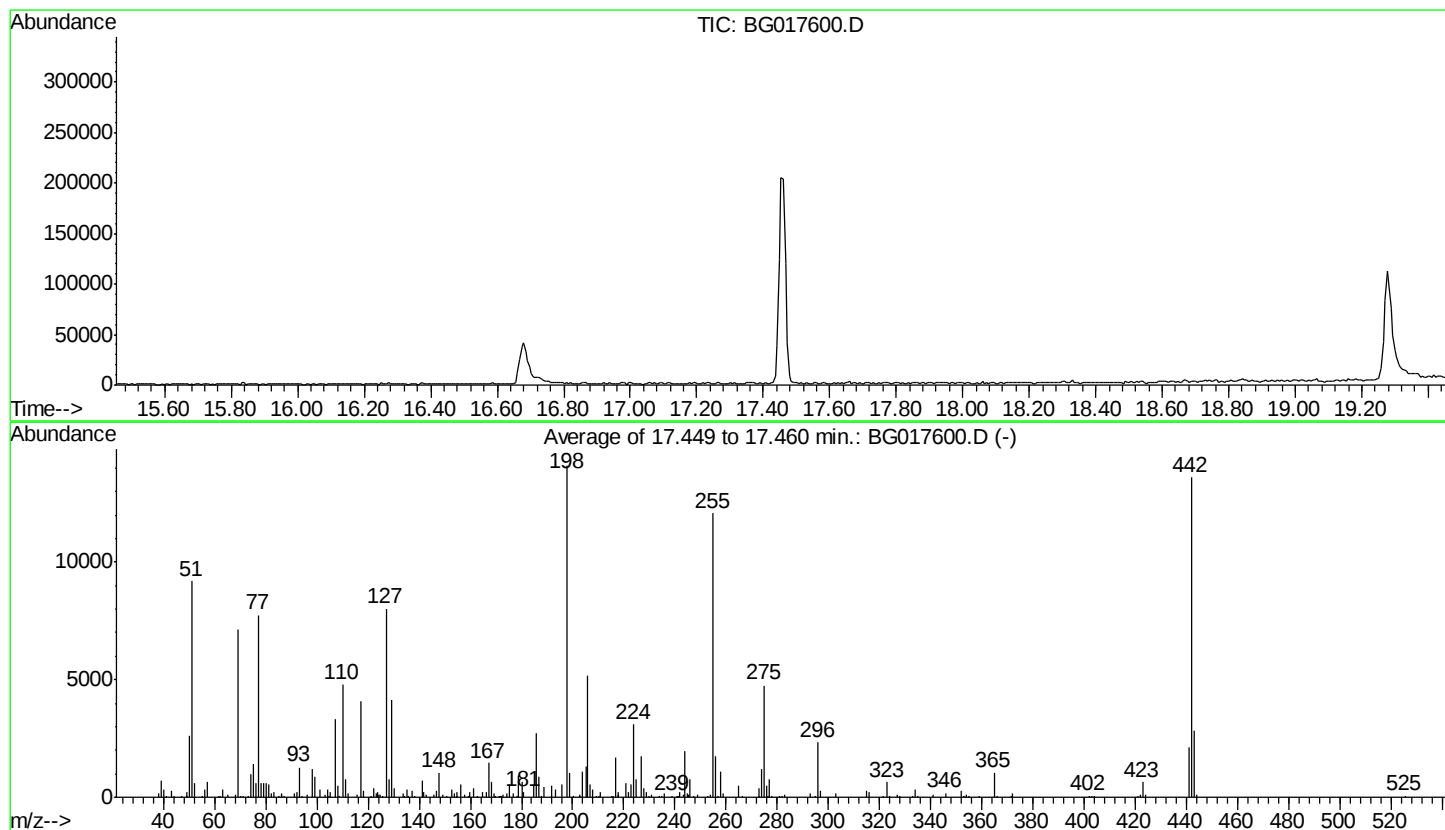

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	65.1	9187	PASS
68	69	0.00	2	1.6	111	PASS
69	198	0.00	100	50.7	7154	PASS
70	69	0.00	2	0.8	57	PASS
127	198	10	80	56.9	8033	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14106	PASS
199	198	5	9	7.5	1063	PASS
275	198	10	60	33.6	4739	PASS
365	198	1	100	7.4	1049	PASS
441	442	0.01	24	15.7	2133	PASS
442	198	50	100	96.4	13599	PASS
443	442	15	24	20.9	2845	PASS