
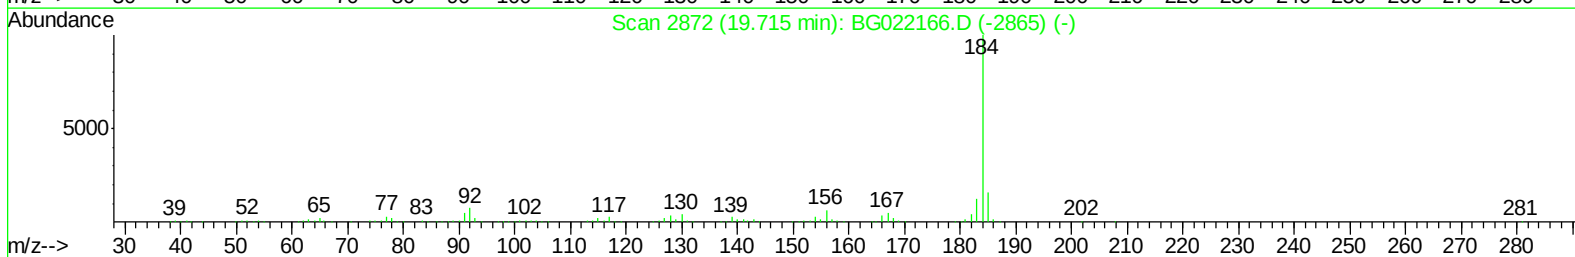
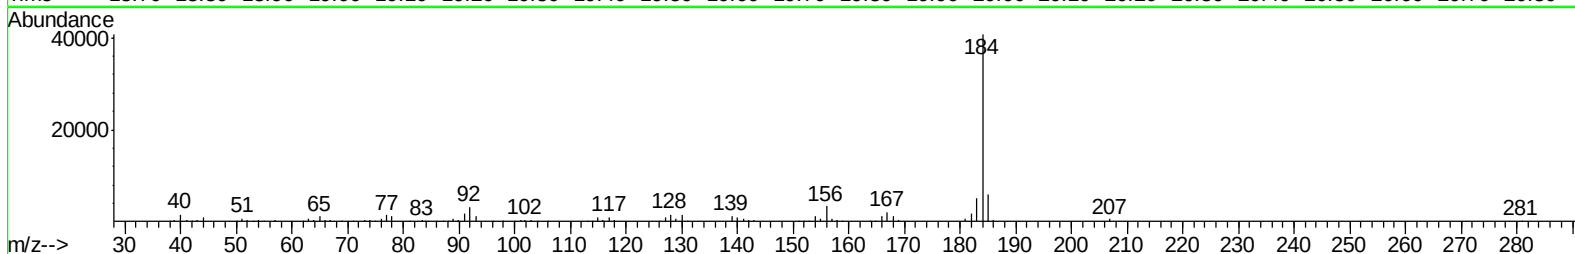


Data Path : Z:\HPCHEM1\BNA_G\Data\BG061016\
Data File : BG022286.D
Acq On : 10 Jun 2016 13:43
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 07:31:30 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 06 16:12:45 2016
Response via : Initial Calibration

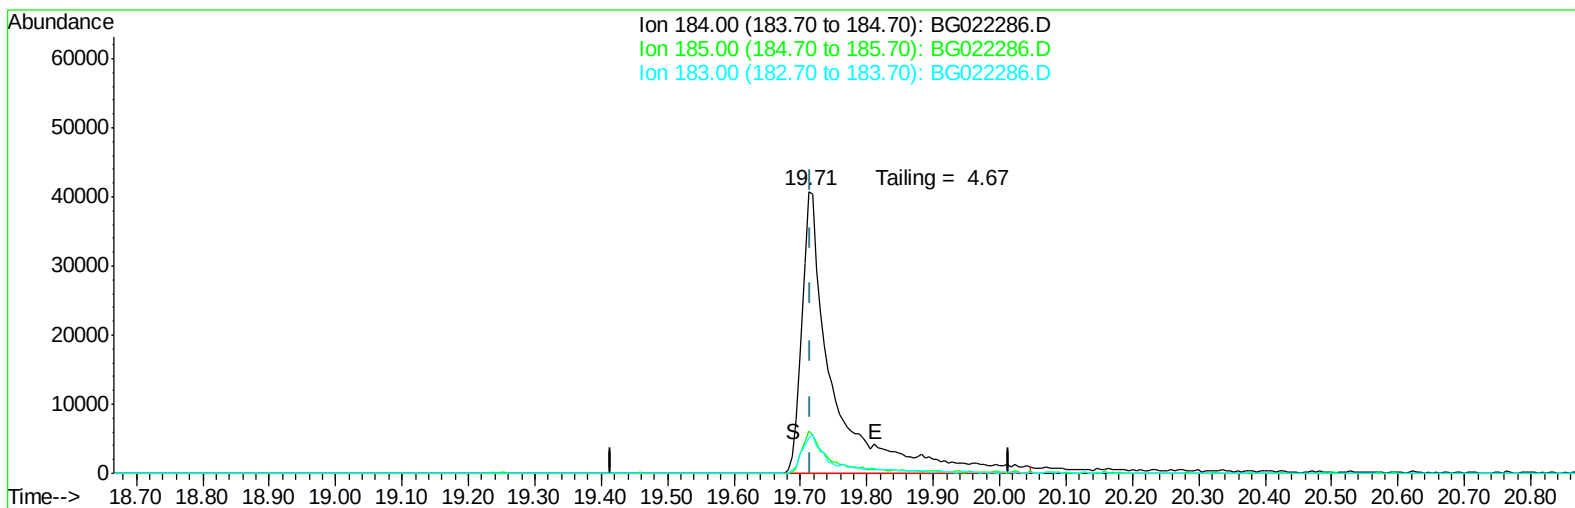

TIC: BG022286.D

(76) Benzidine




19.712min (-0.003) 0.00ng

response 118454

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.99
183.00	12.80	12.84
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG061016\
Data File : BG022286.D
Acq On : 10 Jun 2016 13:43
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 07:31:30 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 06 16:12:45 2016
Response via : Initial Calibration

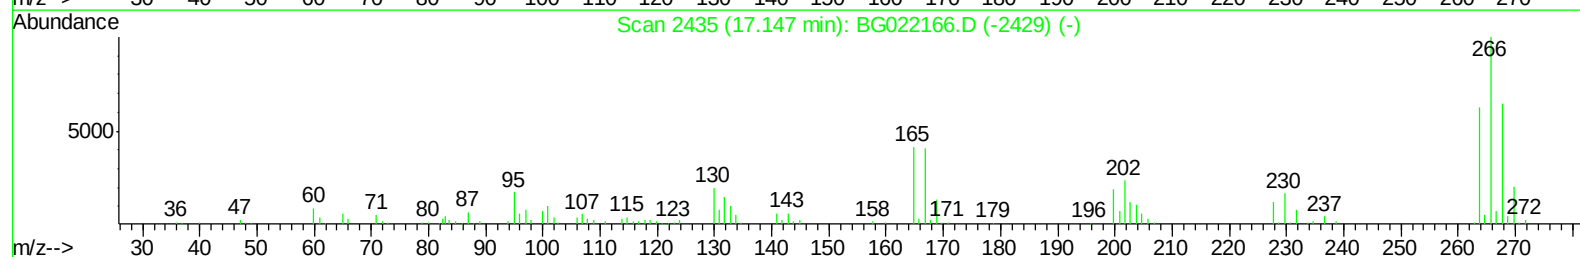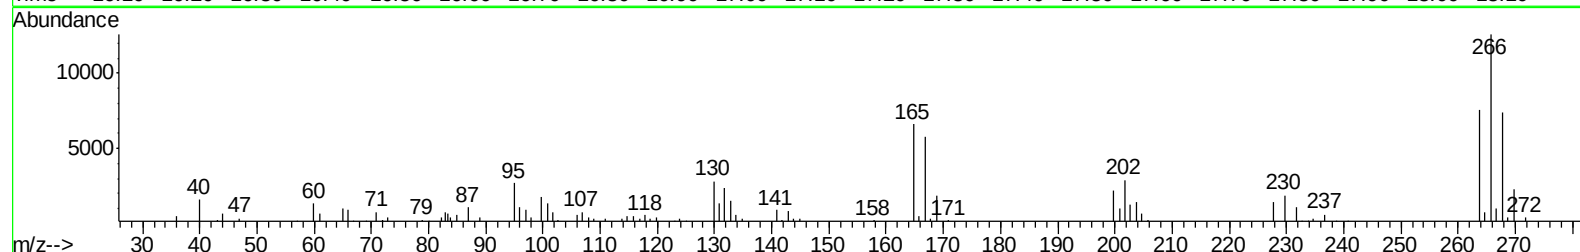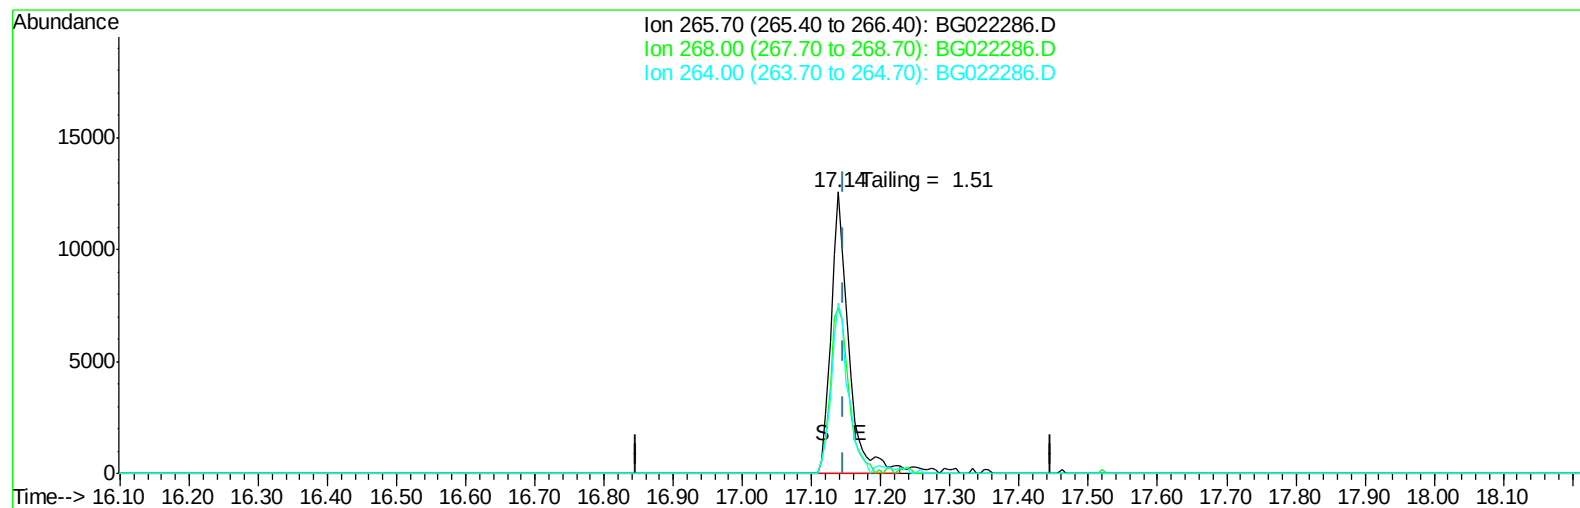

TIC: BG022286.D

(69) Pentachlorophenol (C)

17.138min (-0.009) 0.00ng

response 21918

Ion	Exp%	Act%
265.70	100	100
268.00	68.10	61.97
264.00	67.20	66.09
0.00	0.00	0.00