
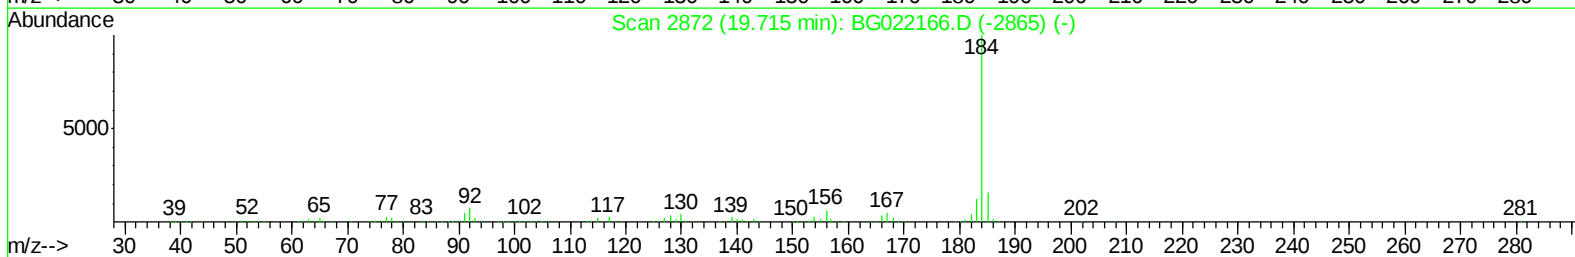
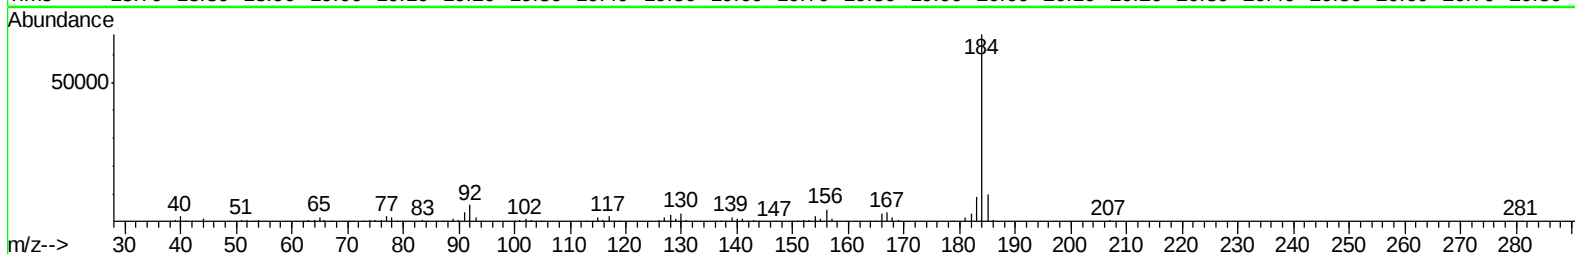


Data Path : Z:\HPCHEM1\BNA_G\Data\BG061016\
Data File : BG022303.D
Acq On : 11 Jun 2016 1:47
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 07:32:44 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 06 16:12:45 2016
Response via : Initial Calibration

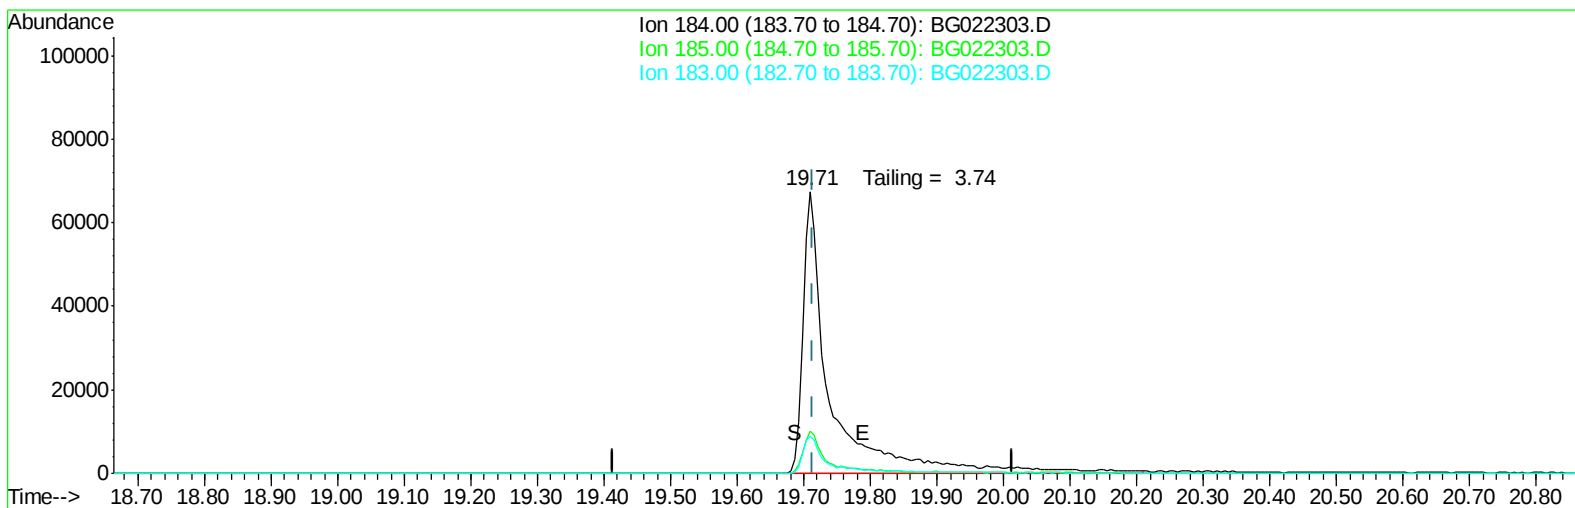

TIC: BG022303.D

(76) Benzidine




19.709min (-0.005) 107886.19ng

response 169275

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.91
183.00	12.80	13.07
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG061016\
Data File : BG022303.D
Acq On : 11 Jun 2016 1:47
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 07:32:44 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 06 16:12:45 2016
Response via : Initial Calibration

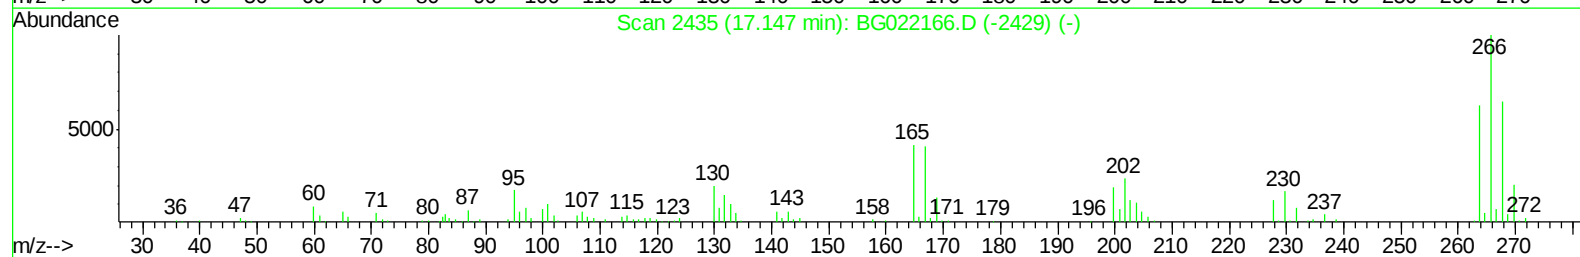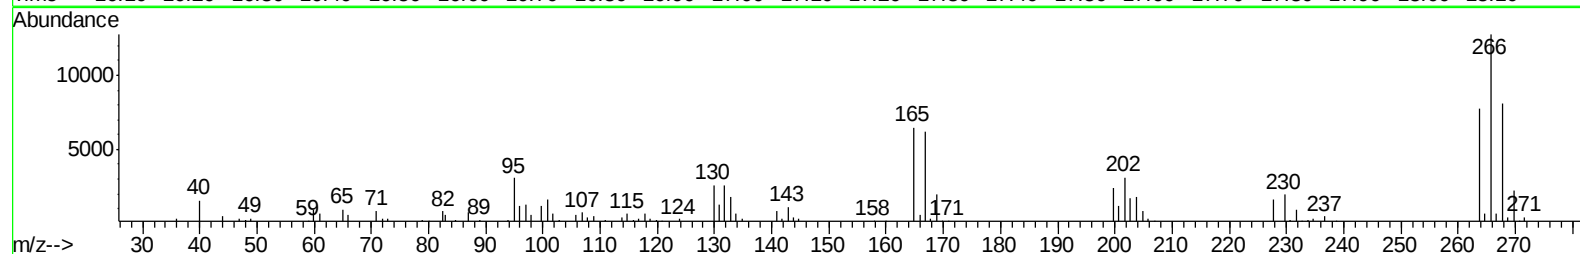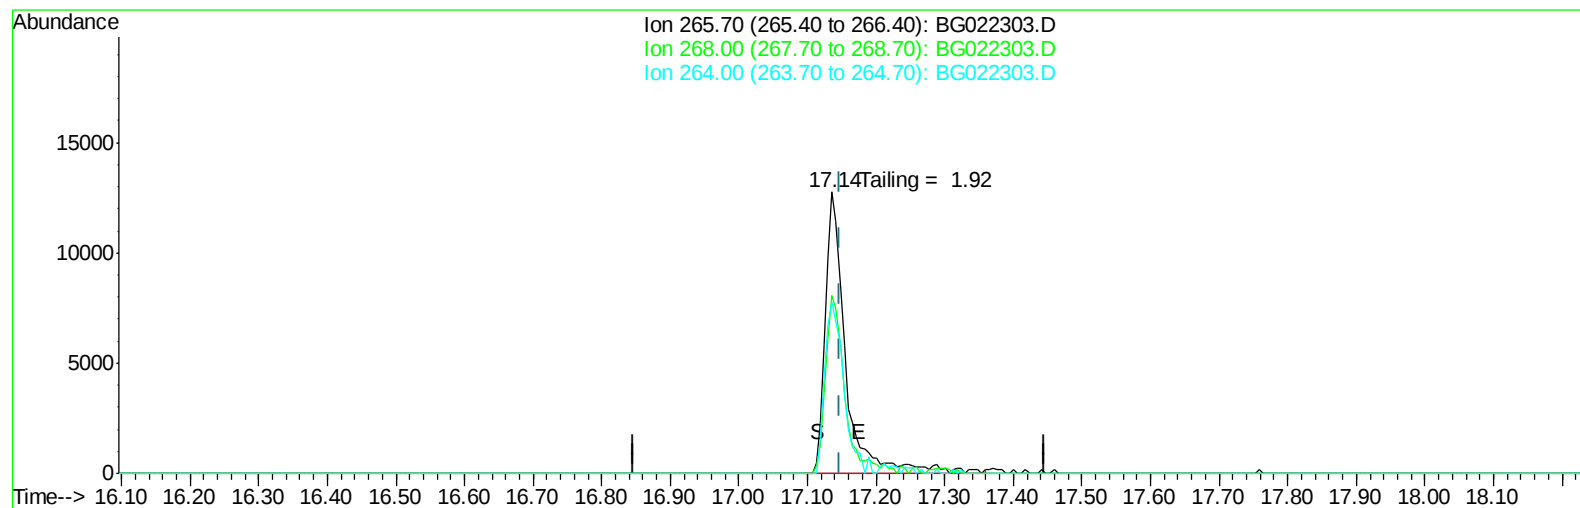

TIC: BG022303.D

(69) Pentachlorophenol (C)

17.136min (-0.011) 0.00ng

response 24824

Ion	Exp%	Act%
265.70	100	100
268.00	68.10	66.80
264.00	67.20	65.75
0.00	0.00	0.00