


Data Path : Z:\HPCHEM1\BNA_G\Data\BG061016\
 Data File : BG022286.D
 Acq On : 10 Jun 2016 13:43
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 13 17:40:23 2016

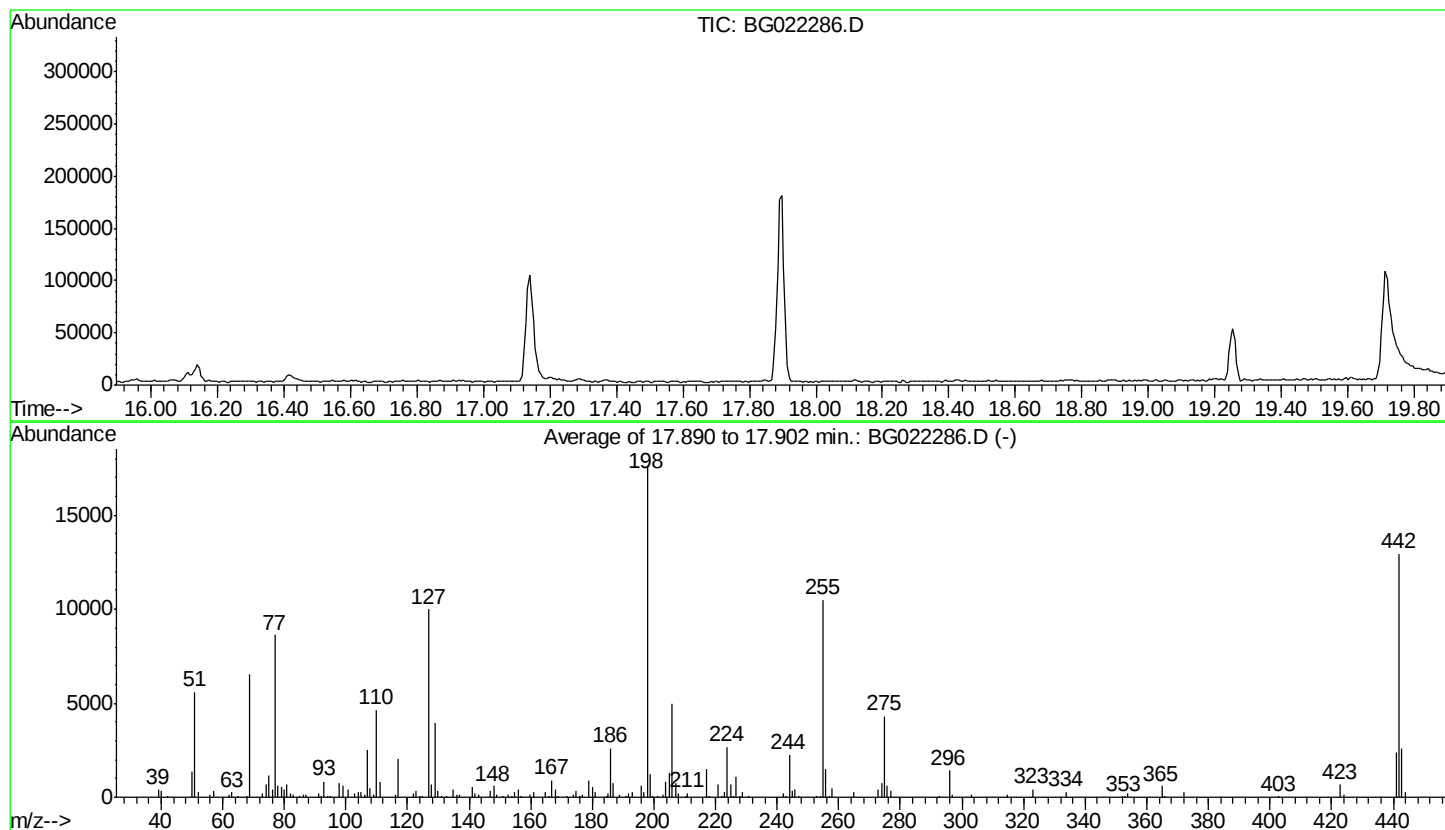

AutoFind: Scans 2562, 2563, 2564; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	5601	PASS
68	69	0.00	2	1.2	80	PASS
69	198	0.00	100	37.3	6569	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.7	9998	PASS
197	198	0.00	2	1.4	255	PASS
198	198	100	100	100.0	17634	PASS
199	198	5	9	6.9	1225	PASS
275	198	10	60	24.5	4319	PASS
365	198	1	100	3.4	599	PASS
441	442	0.01	24	18.2	2362	PASS
442	198	50	100	73.5	12967	PASS
443	442	15	24	20.0	2596	PASS