


Data Path : Z:\HPCHEM1\BNA_G\Data\BG061016\
 Data File : BG022303.D
 Acq On : 11 Jun 2016 1:47
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 13 17:40:23 2016

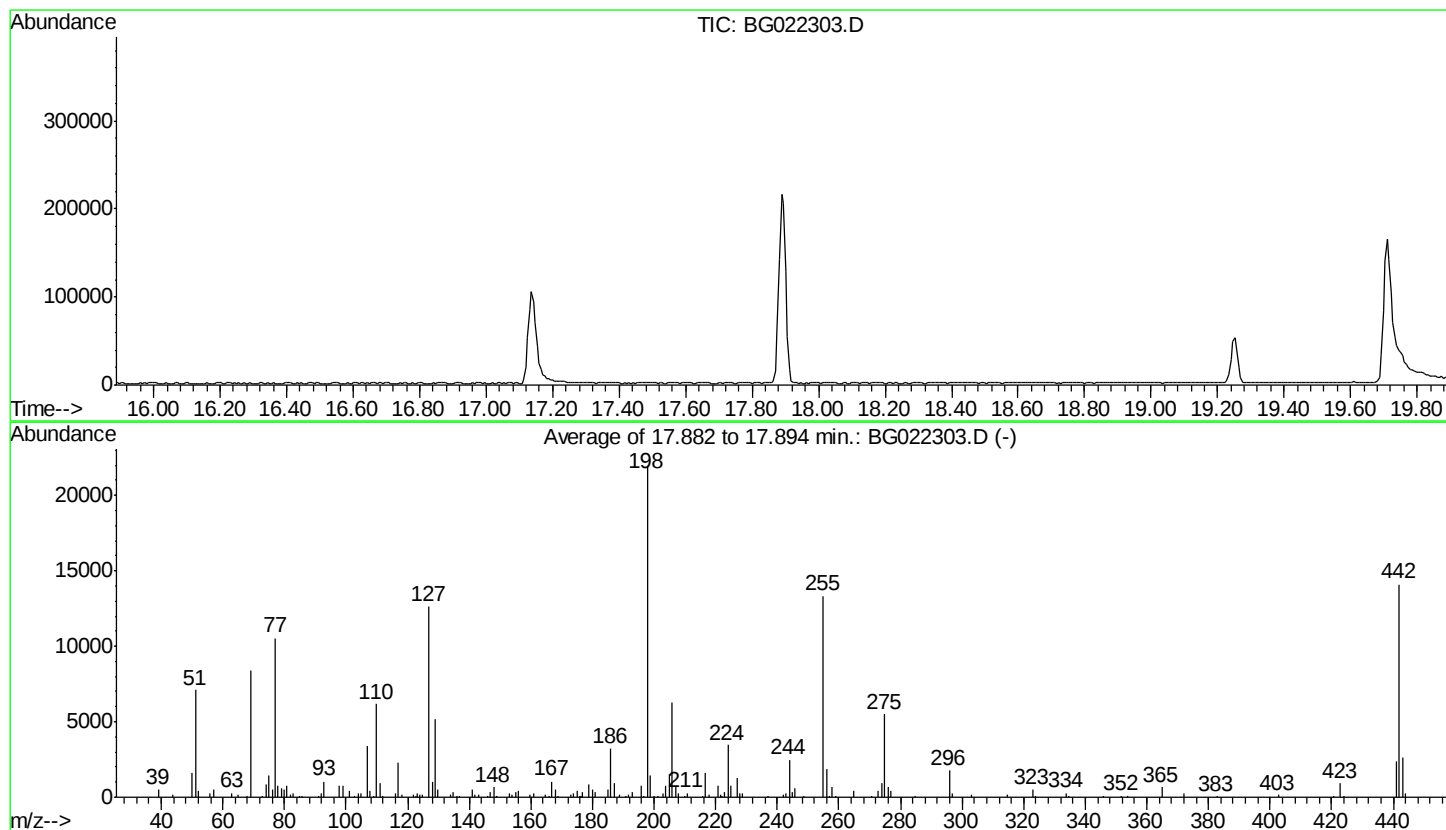

AutoFind: Scans 2560, 2561, 2562; Background Corrected with Scan 2554

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	7103	PASS
68	69	0.00	2	1.0	86	PASS
69	198	0.00	100	38.1	8377	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	57.5	12620	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	21965	PASS
199	198	5	9	6.8	1485	PASS
275	198	10	60	25.0	5489	PASS
365	198	1	100	3.0	658	PASS
441	442	0.01	24	16.8	2368	PASS
442	198	50	100	64.1	14083	PASS
443	442	15	24	18.9	2667	PASS