


Data Path : Z:\HPCHEM1\BNA_G\Data\BG061017\
 Data File : BG027367.D
 Acq On : 10 Jun 2017 11:52
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 05 16:00:35 2017

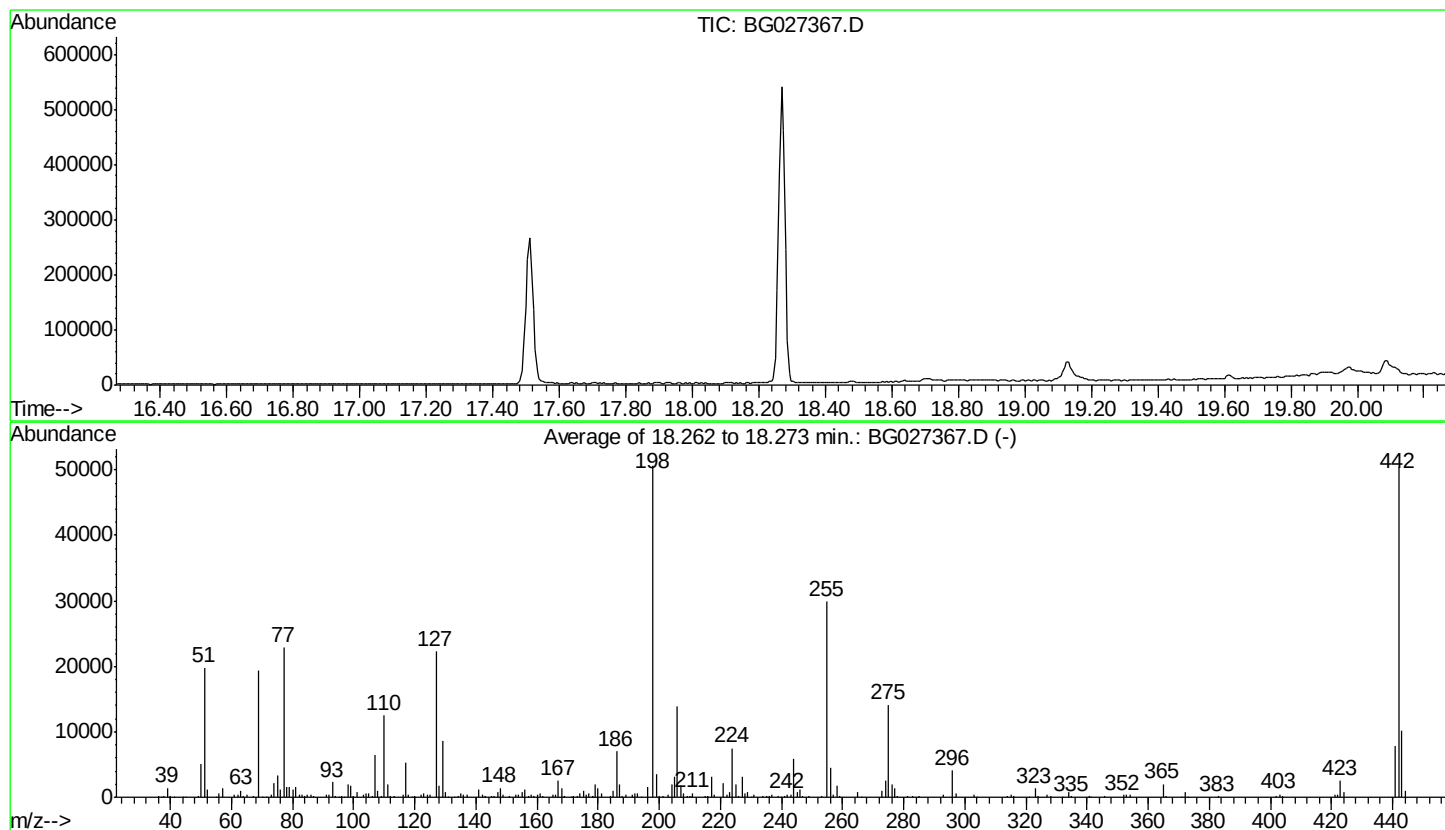

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	19784	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.1	19312	PASS
70	69	0.00	2	0.2	45	PASS
127	198	10	80	44.0	22288	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50648	PASS
199	198	5	9	6.8	3455	PASS
275	198	10	60	27.9	14137	PASS
365	198	1	100	3.9	1980	PASS
441	442	0.01	24	15.7	7910	PASS
442	198	50	100	99.5	50405	PASS
443	442	15	24	20.0	10089	PASS