
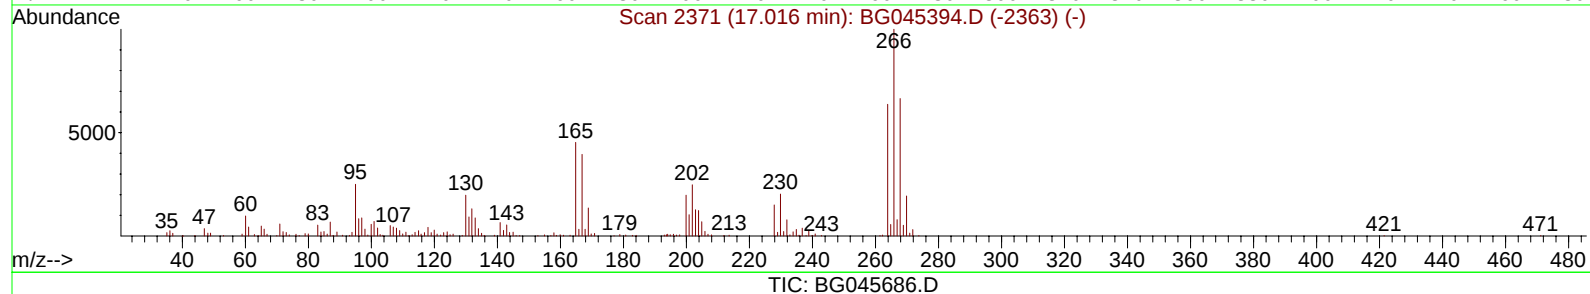
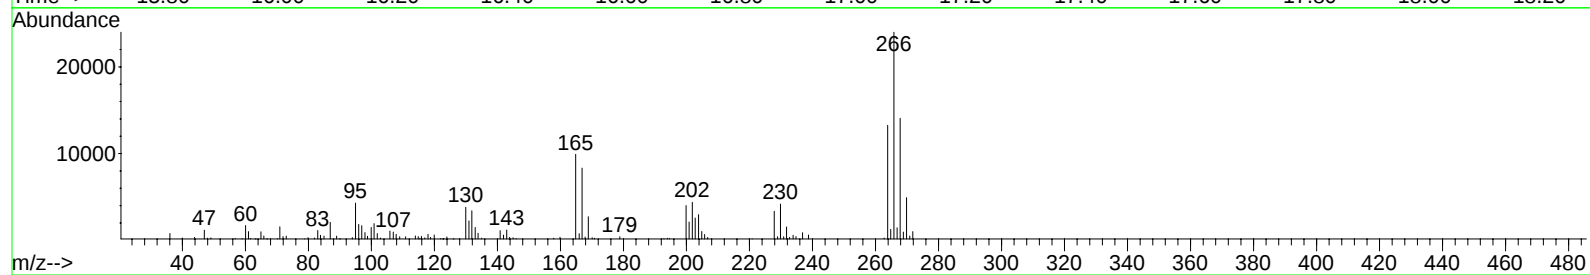


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061020\
Data File : BG045686.D
Acq On : 10 Jun 2020 11:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 19:03:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 01 15:07:00 2020
Response via : Initial Calibration

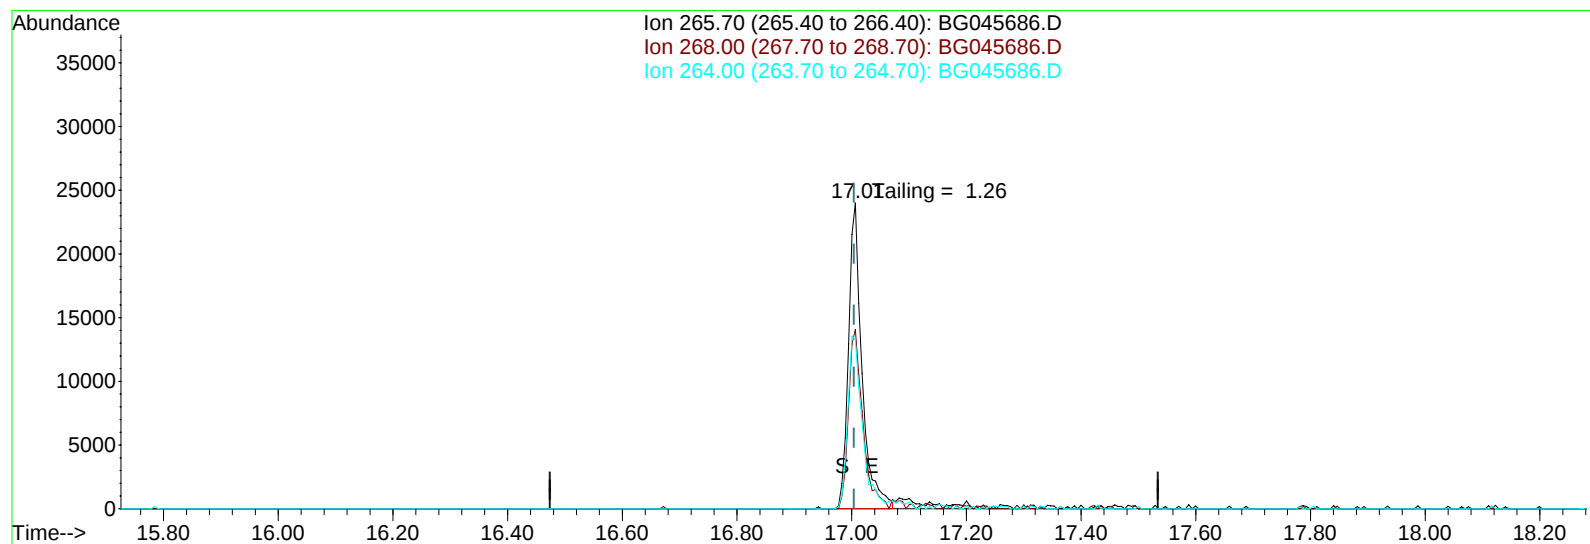

(70) Pentachlorophenol (C)




17.006min (+0.003) 81905.12ng

response 39496

Ion	Exp%	Act%
265.70	100	100
268.00	66.50	58.62
264.00	63.70	55.24
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061020\
Data File : BG045686.D
Acq On : 10 Jun 2020 11:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 19:03:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 01 15:07:00 2020
Response via : Initial Calibration

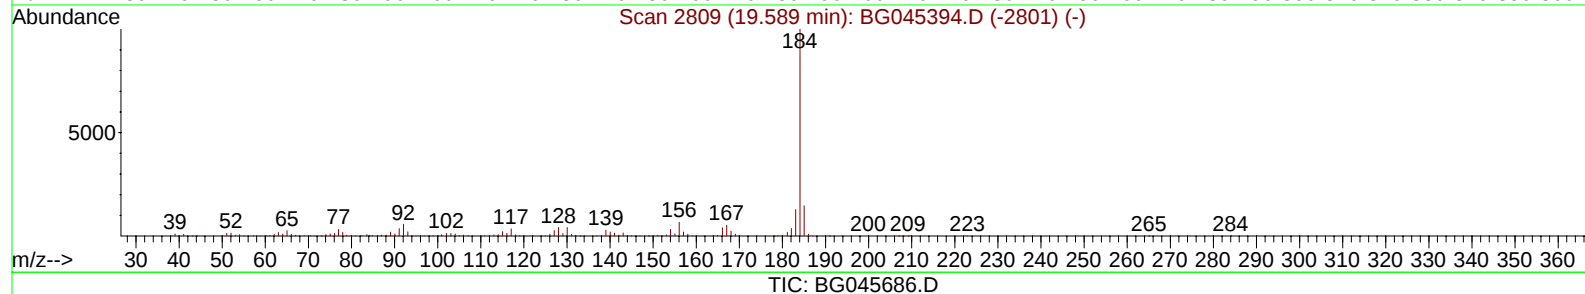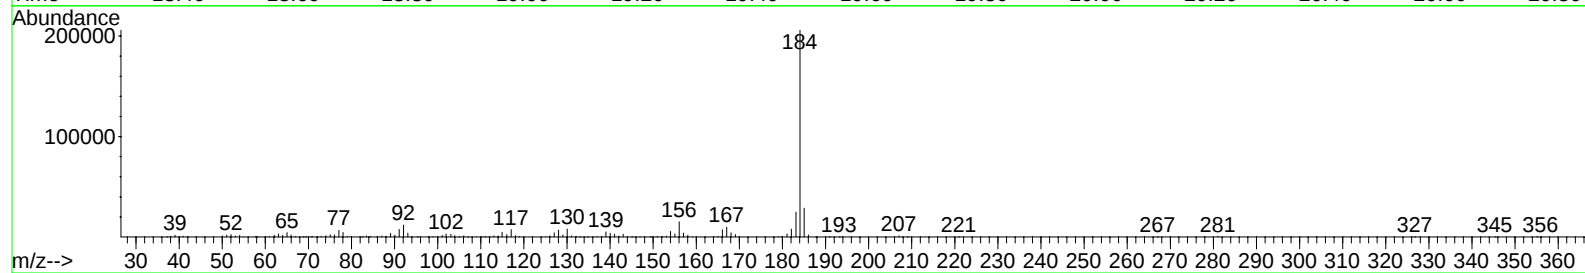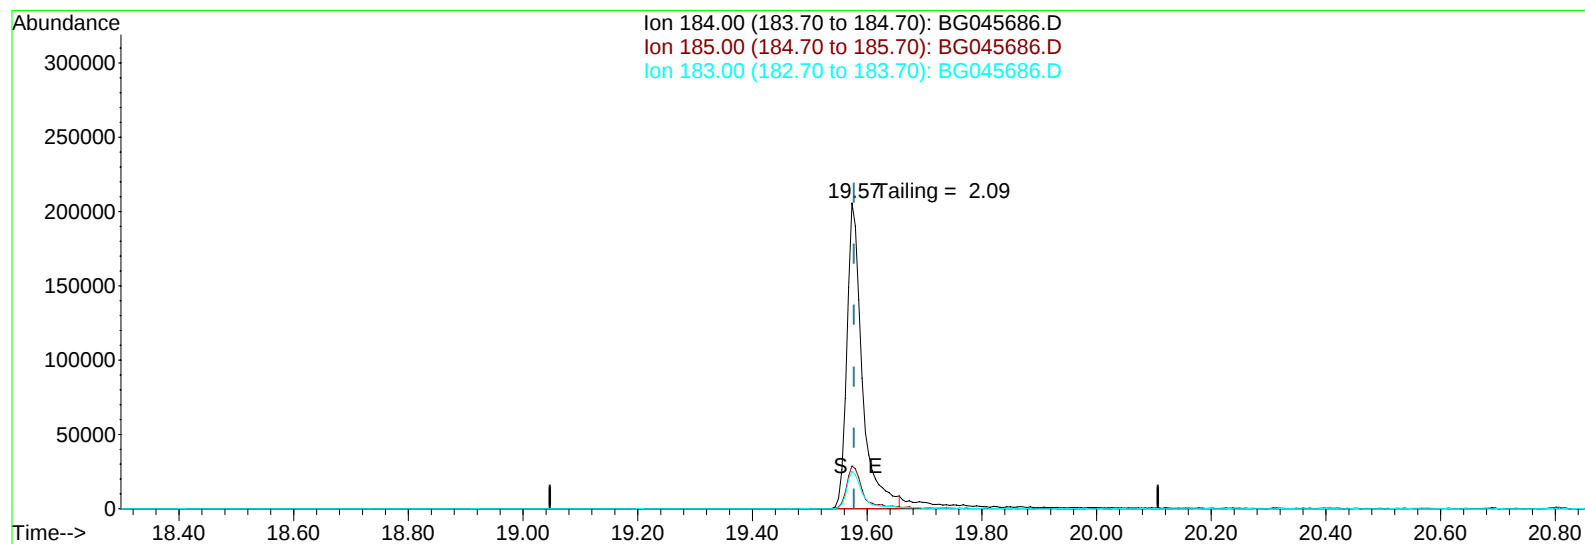

TIC: BG045686.D

(77) Benzidine

19.573min (-0.003) 246243.80ng

response 394205

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	14.01
183.00	12.80	12.18
0.00	0.00	0.00