
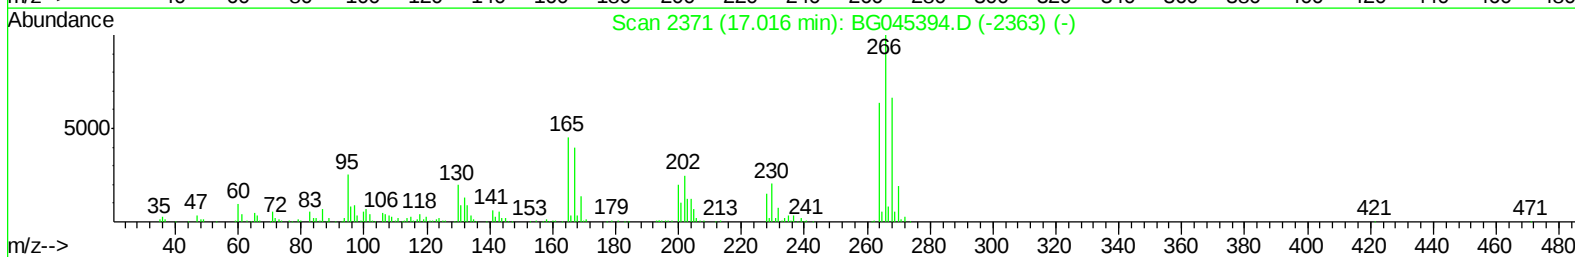
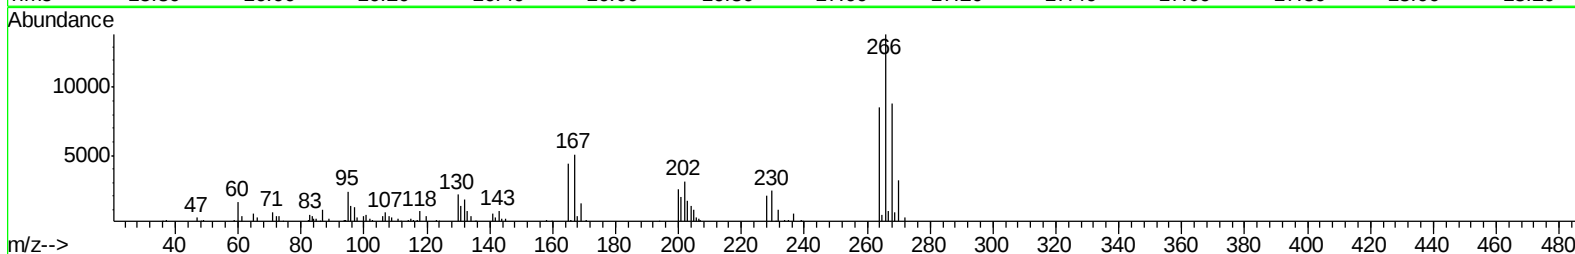


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061020\
Data File : BG045705.D
Acq On : 11 Jun 2020 2:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 02:44:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 01 15:07:00 2020
Response via : Initial Calibration

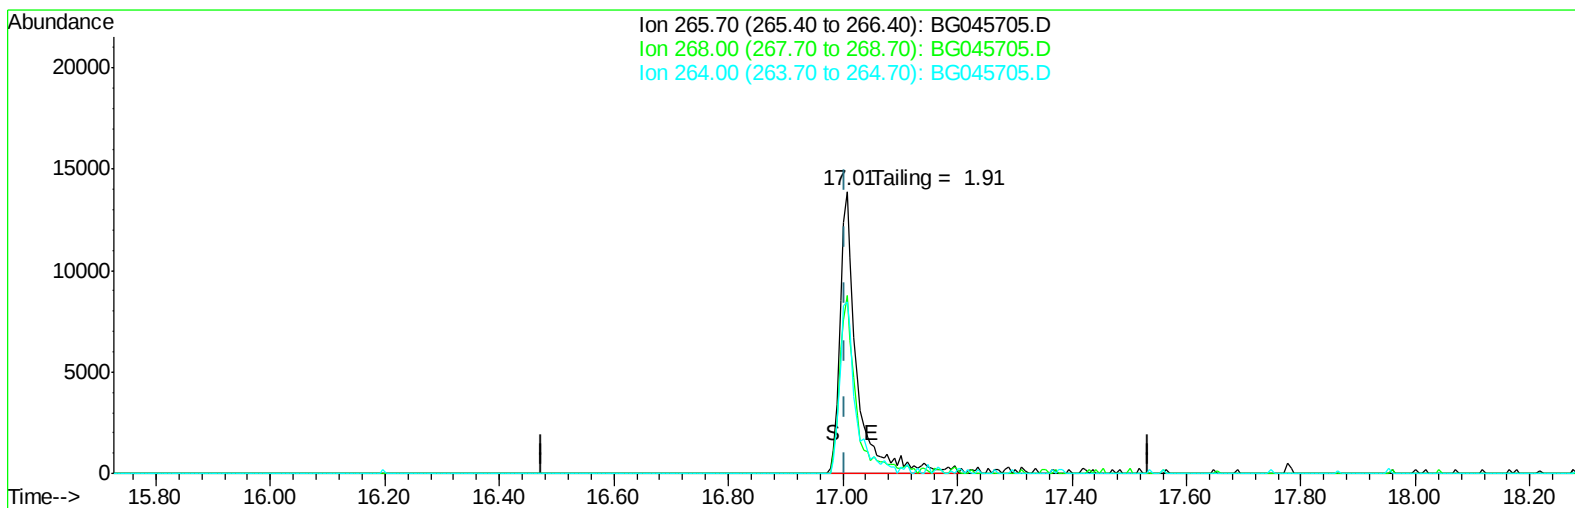

TIC: BG045705.D

(70) Pentachlorophenol (C)




17.007min (+0.003) 62081.35ng

response 27016

Ion	Exp%	Act%
265.70	100	100
268.00	66.50	63.29
264.00	63.70	61.12
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061020\
Data File : BG045705.D
Acq On : 11 Jun 2020 2:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 02:44:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 01 15:07:00 2020
Response via : Initial Calibration

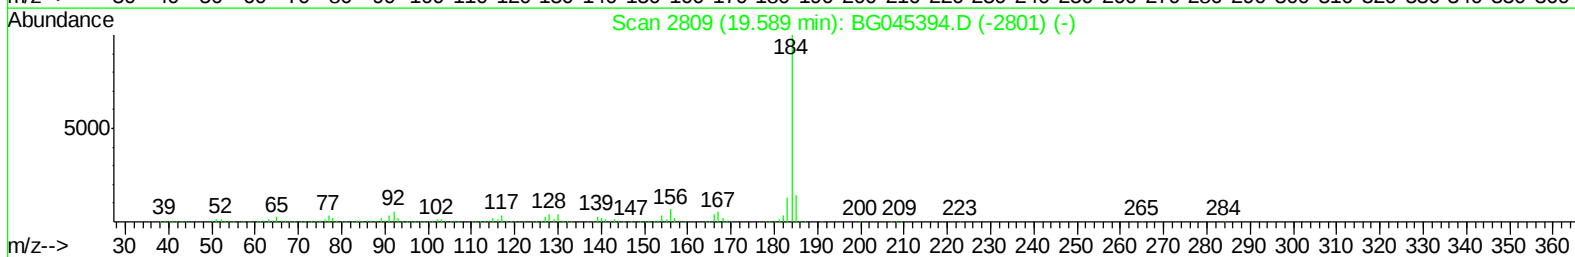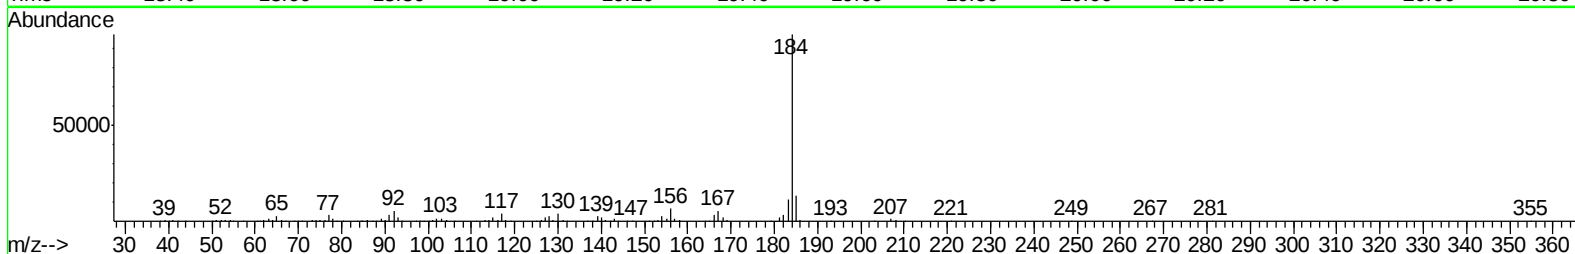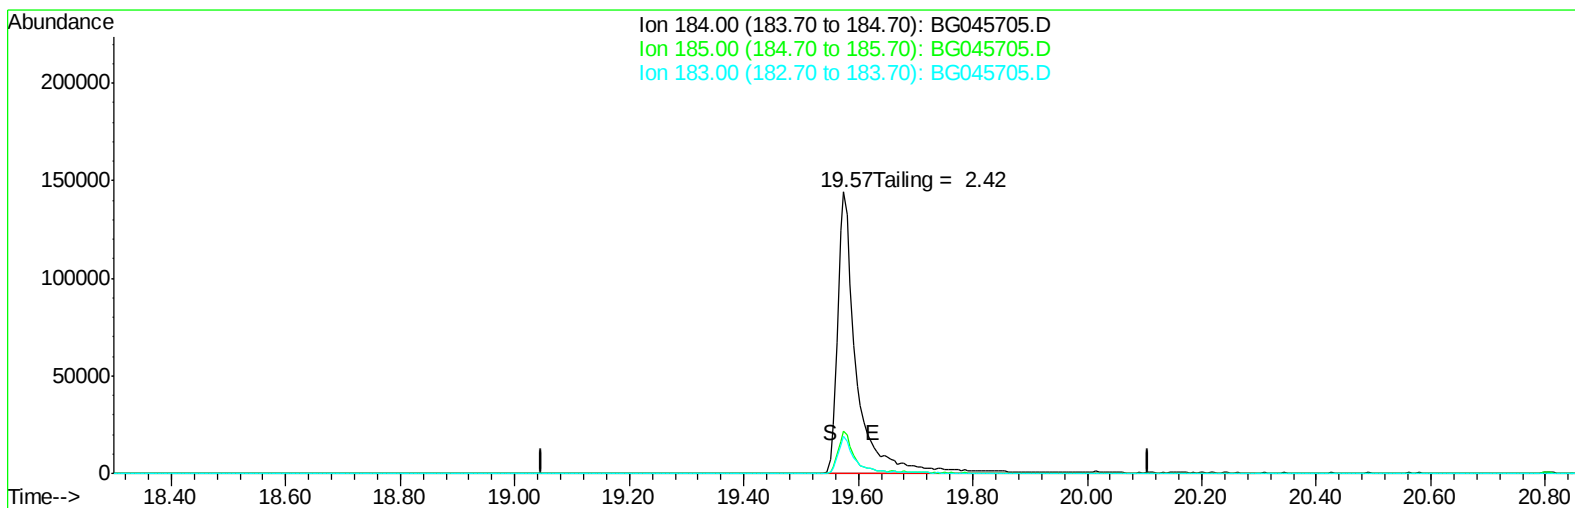

TIC: BG045705.D

(77) Benzidine

19.577min (-19.577) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	14.60	0.00#
183.00	12.80	0.00#
0.00	0.00	0.00