
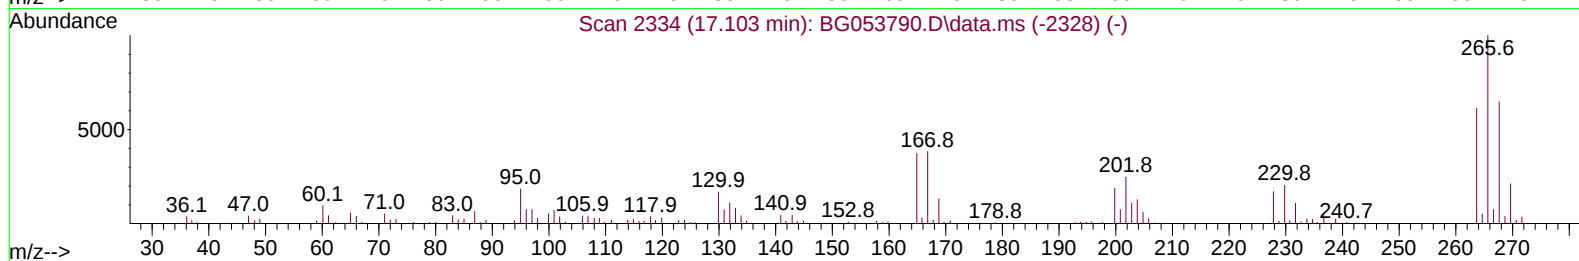
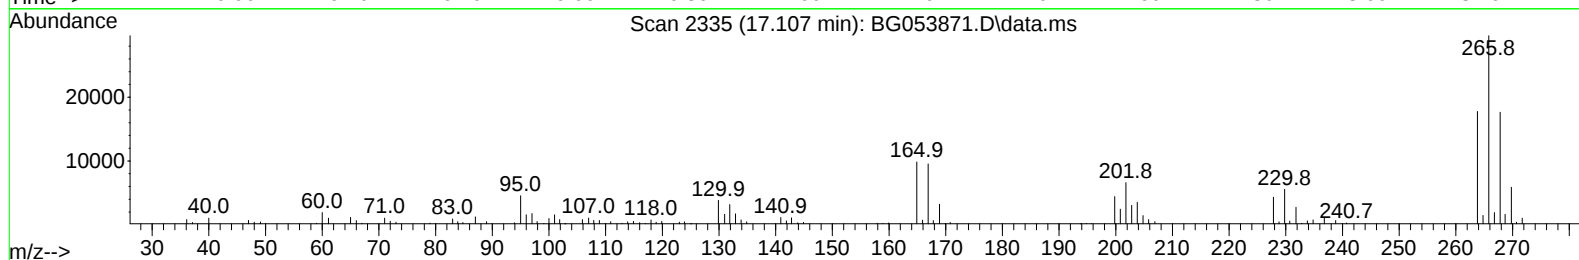


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061022\
Data File : BG053871.D
Acq On : 10 Jun 2022 11:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 11:59:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 23:22:27 2022
Response via : Initial Calibration

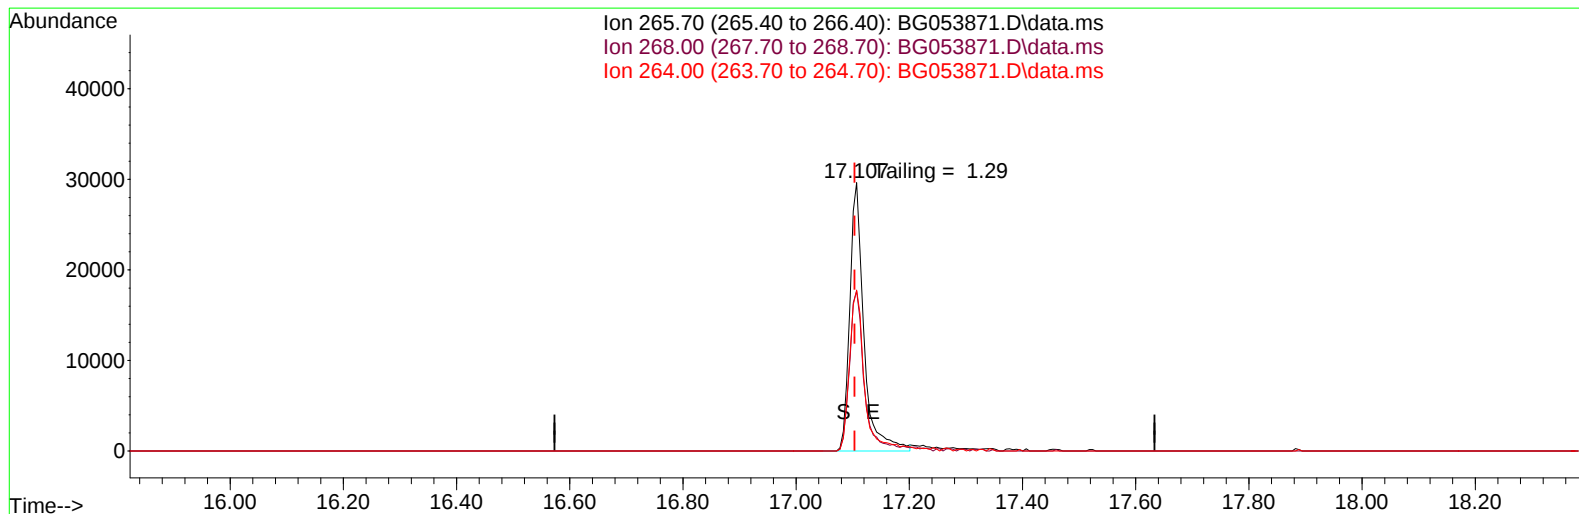

TIC: BG053871.D\data.ms

(70) Pentachlorophenol (C)




17.107min (+ 0.004) 35358.29 ng

response 51289

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	65.07
264.00	66.20	59.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061022\
Data File : BG053871.D
Acq On : 10 Jun 2022 11:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 11:59:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 23:22:27 2022
Response via : Initial Calibration

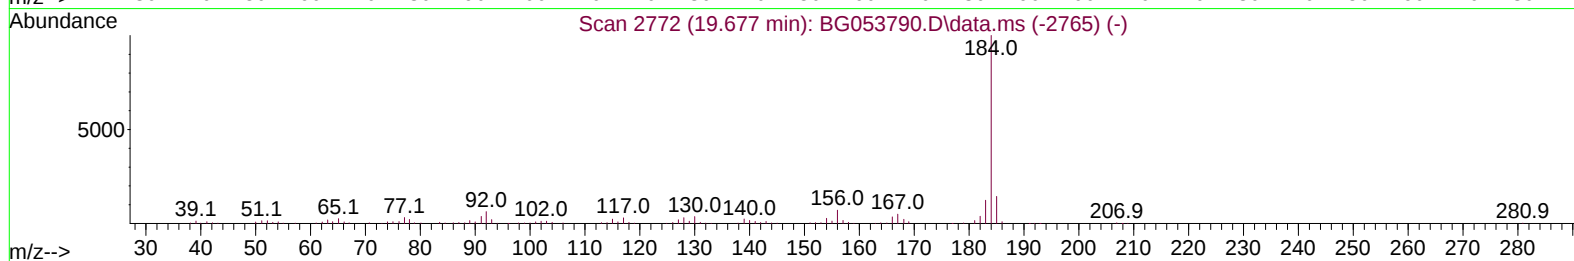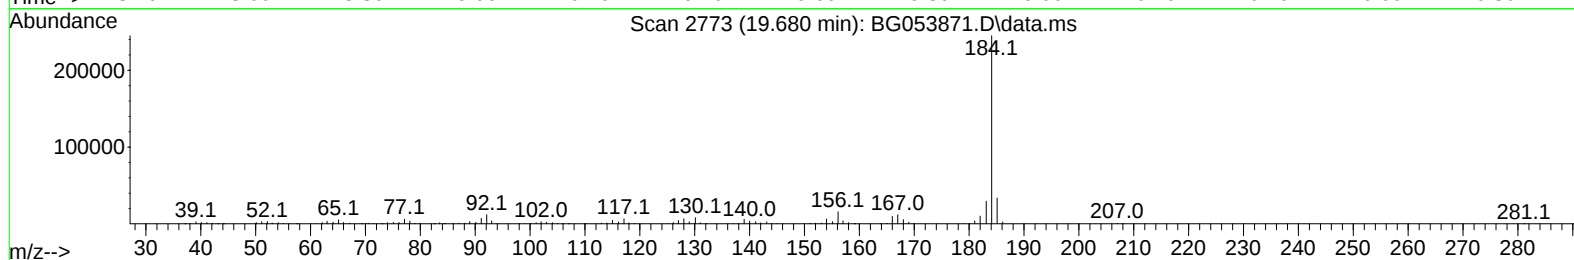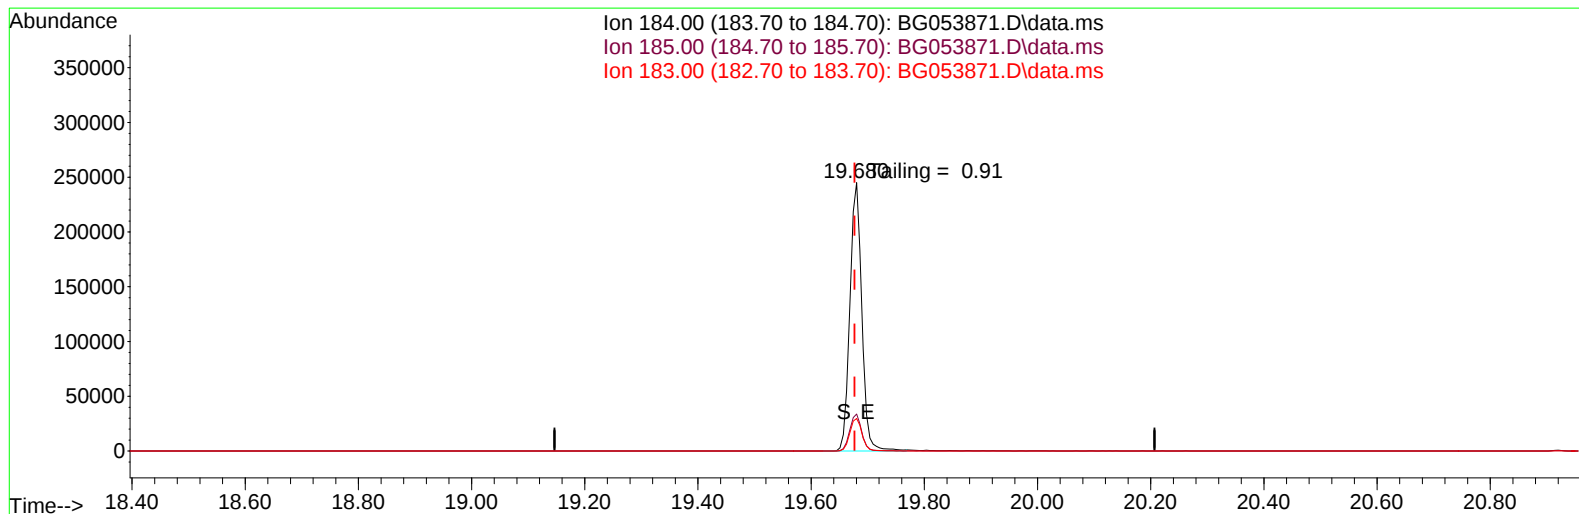

TIC: BG053871.D\data.ms

(77) Benzidine**19.680min (+ 0.004) 0.00 ng****response 358719**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.78
183.00	11.10	12.10
0.00	0.00	0.00