


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061022\
 Data File : BG053871.D
 Acq On : 10 Jun 2022 11:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 02 23:22:27 2022

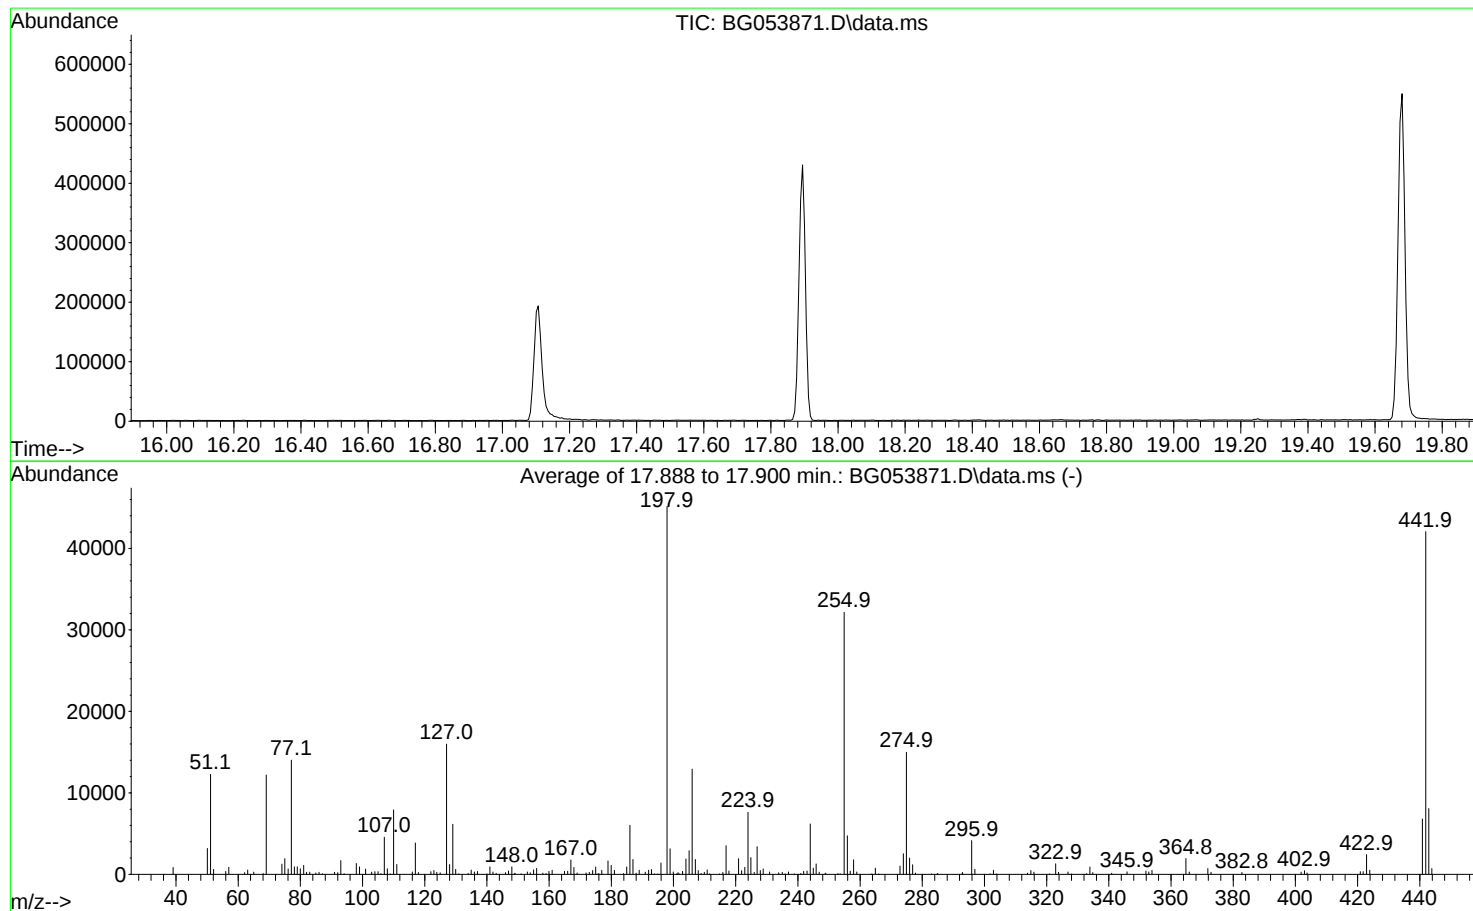

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.2	12280	PASS
68	69	0.00	2	0.7	86	PASS
69	198	0.00	100	27.0	12195	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	35.4	15980	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45139	PASS
199	198	5	9	7.0	3138	PASS
275	198	10	60	33.2	14985	PASS
365	198	1	100	4.3	1946	PASS
441	198	0.01	100	15.1	6803	PASS
442	442	50	100	100.0	42056	PASS
443	442	15	24	19.2	8072	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/10/2022	BNA_G	<u>BG053871.D</u>
Compound Name	Response	Retention Time
DDT	184394	20.91
DDD	1158	20.47
DDE	62	19.97
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1220	185614	0.66

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061022\
Data File : BG053871.D
Acq On : 10 Jun 2022 11:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 10 11:59:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 23:22:27 2022
Response via : Initial Calibration

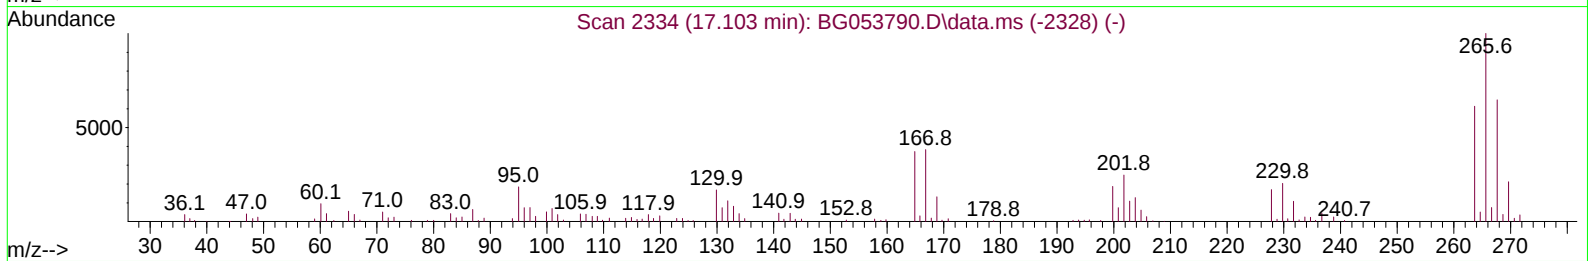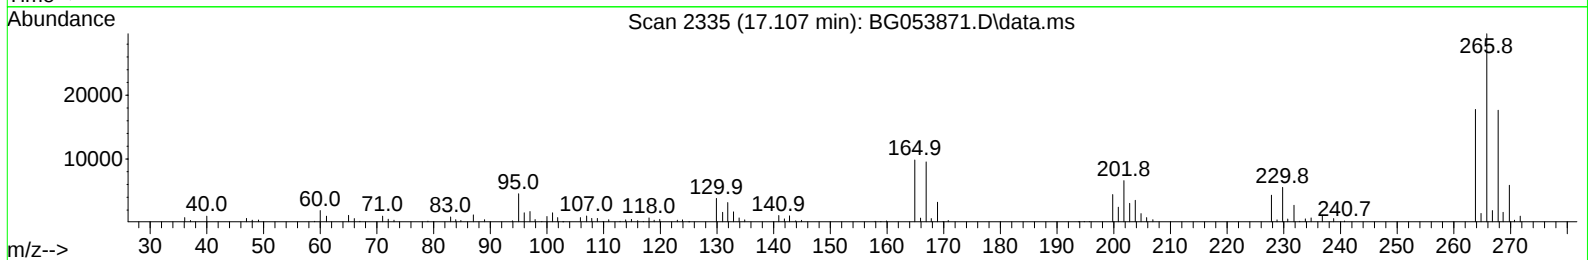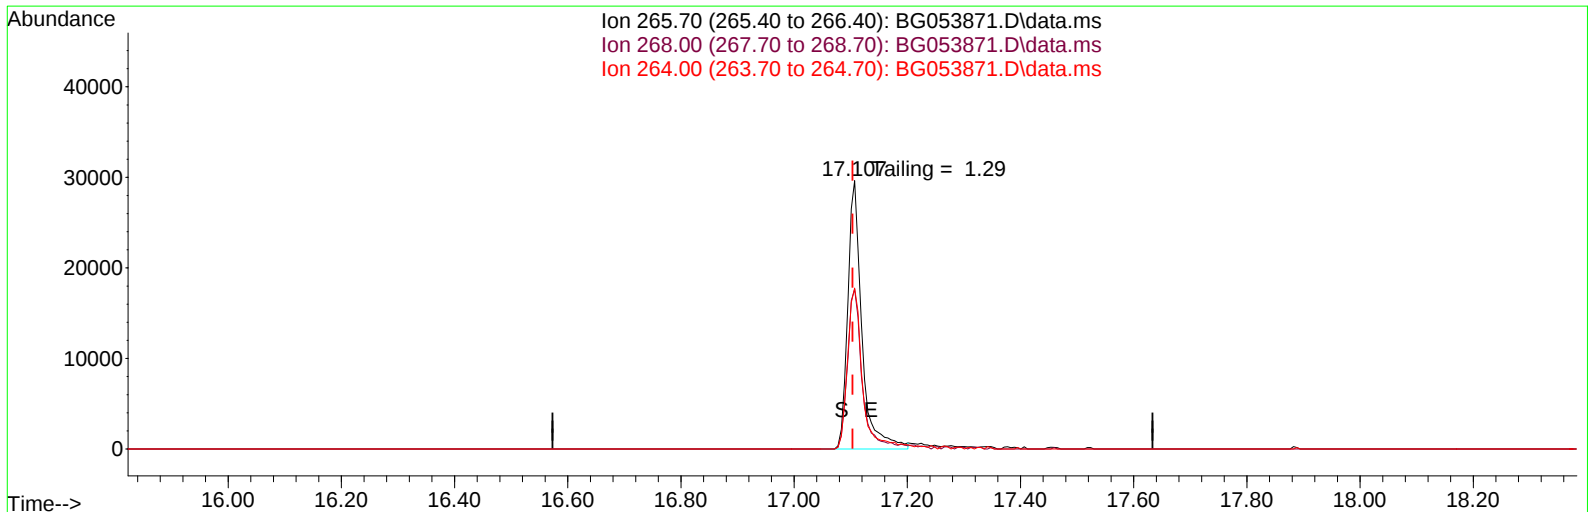

TIC: BG053871.D\data.ms

(70) Pentachlorophenol (C)

17.107min (+ 0.004) 35358.29 ng




response 51289

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	65.07
264.00	66.20	59.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061022\
Data File : BG053871.D
Acq On : 10 Jun 2022 11:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 10 11:59:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 23:22:27 2022
Response via : Initial Calibration

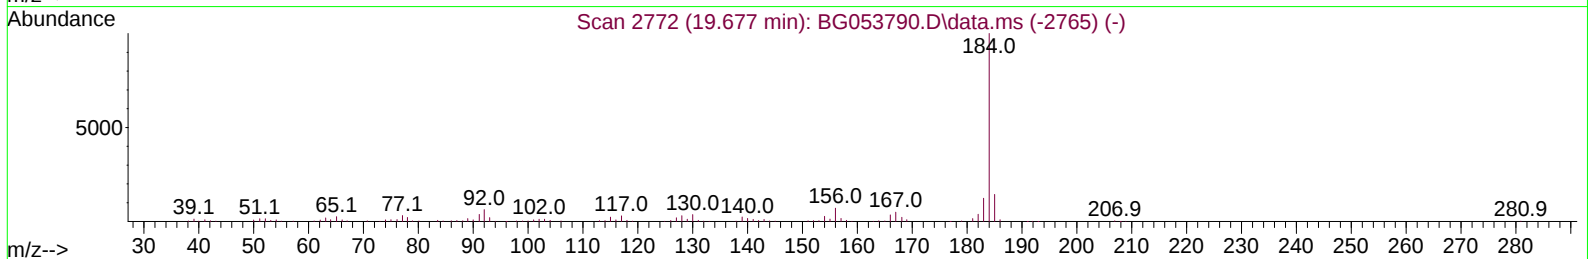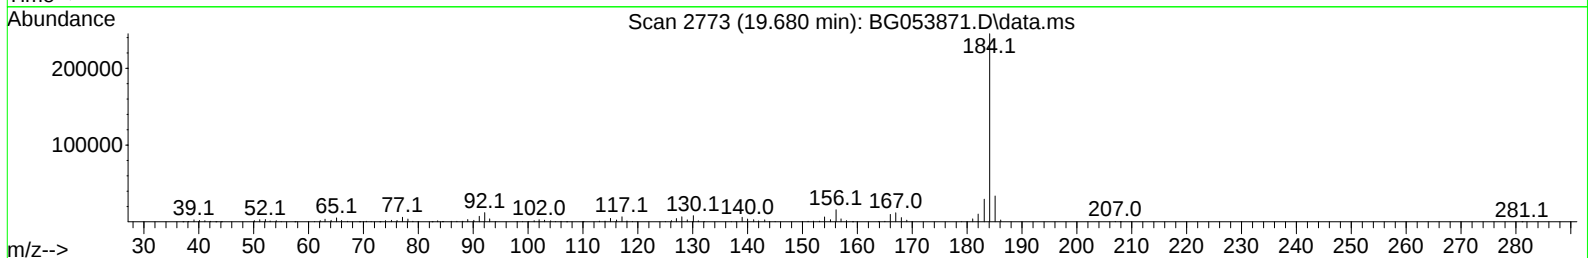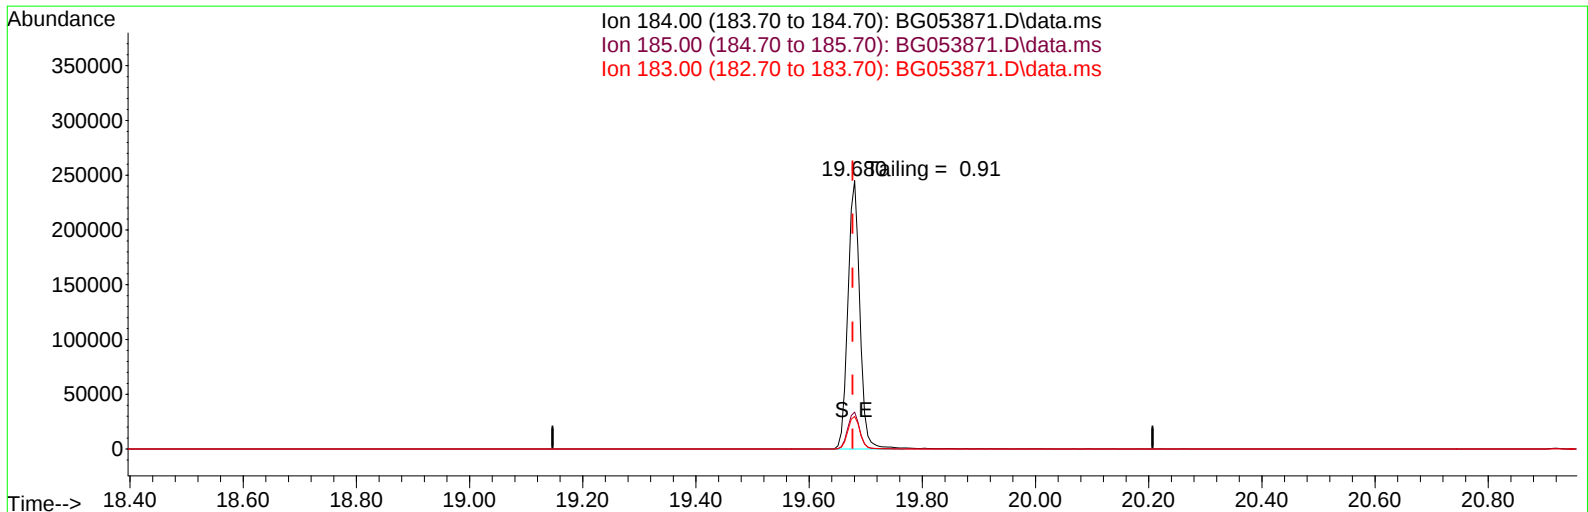

TIC: BG053871.D\data.ms

(77) Benzidine

19.680min (+ 0.004) 0.00 ng

response 358719

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.78
183.00	11.10	12.10
0.00	0.00	0.00