


Data Path : Z:\HPCHEM1\BNA_G\Data\BG061115\
Data File : BG017610.D
Acq On : 11 Jun 2015 14:54
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 08 18:39:50 2015

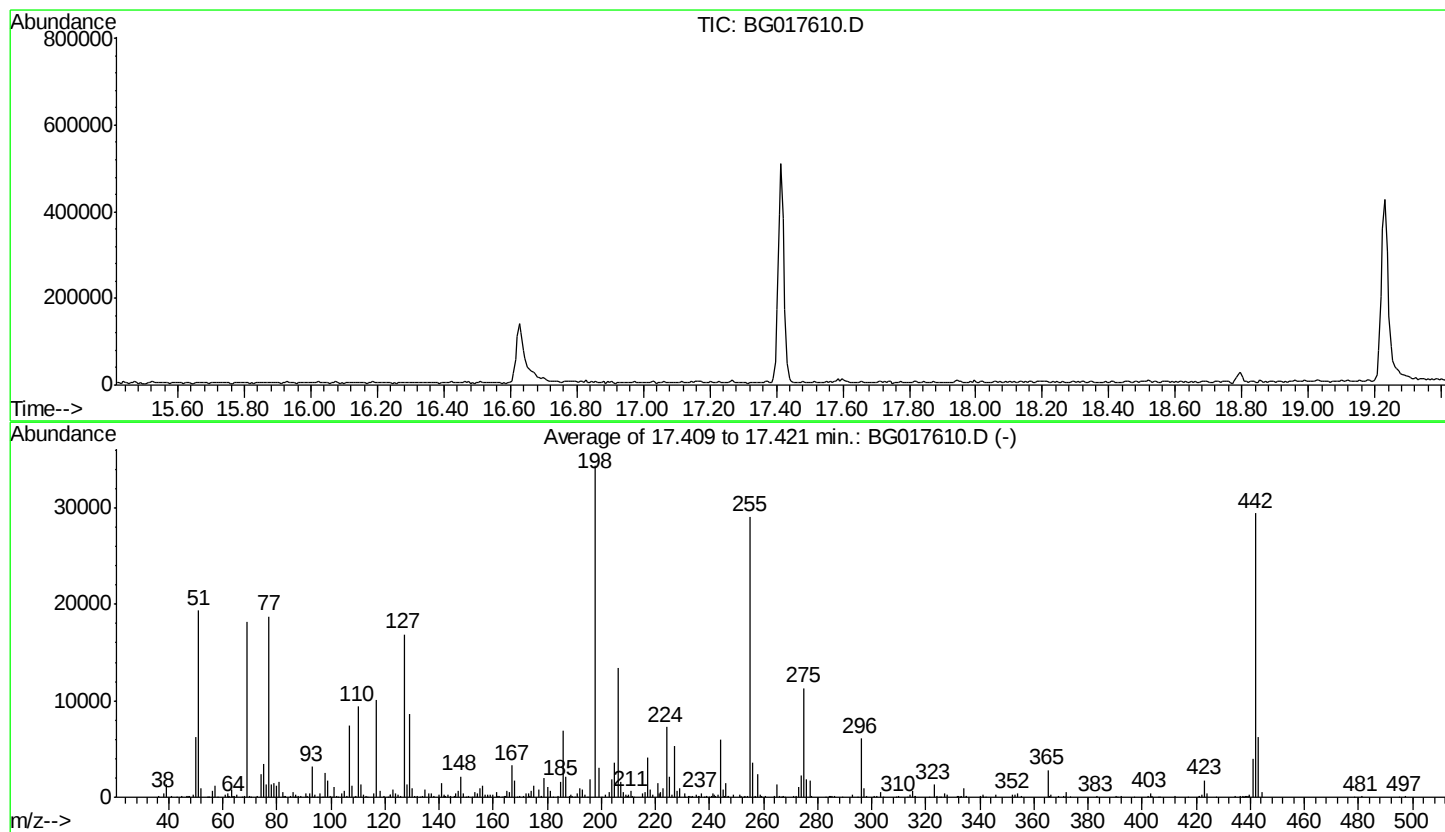

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.2	19327	PASS
68	69	0.00	2	0.6	110	PASS
69	198	0.00	100	52.8	18146	PASS
70	69	0.00	2	0.8	151	PASS
127	198	10	80	49.2	16913	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	34378	PASS
199	198	5	9	9.0	3083	PASS
275	198	10	60	32.8	11293	PASS
365	198	1	100	8.2	2828	PASS
441	442	0.01	24	13.5	3971	PASS
442	198	50	100	85.6	29413	PASS
443	442	15	24	21.0	6191	PASS