


Data Path : Z:\HPCHEM1\BNA_G\Data\BG061115\
 Data File : BG017629.D
 Acq On : 12 Jun 2015 4:38
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 08 18:39:50 2015

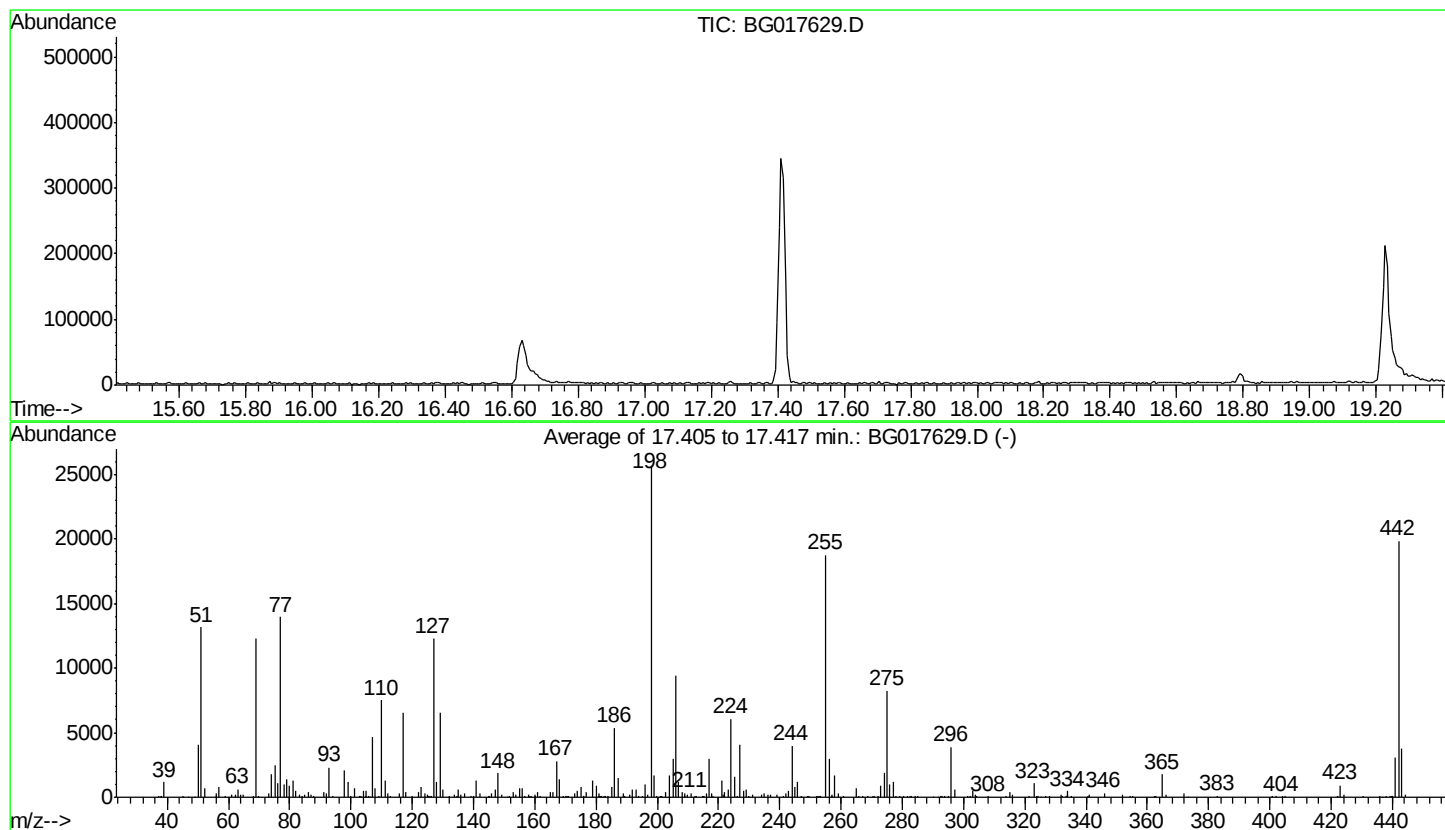

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.3	13165	PASS
68	69	0.00	2	0.7	87	PASS
69	198	0.00	100	47.8	12279	PASS
70	69	0.00	2	1.0	118	PASS
127	198	10	80	47.7	12247	PASS
197	198	0.00	2	0.8	207	PASS
198	198	100	100	100.0	25666	PASS
199	198	5	9	6.6	1703	PASS
275	198	10	60	32.2	8265	PASS
365	198	1	100	6.9	1772	PASS
441	442	0.01	24	15.5	3077	PASS
442	198	50	100	77.4	19858	PASS
443	442	15	24	18.9	3754	PASS