
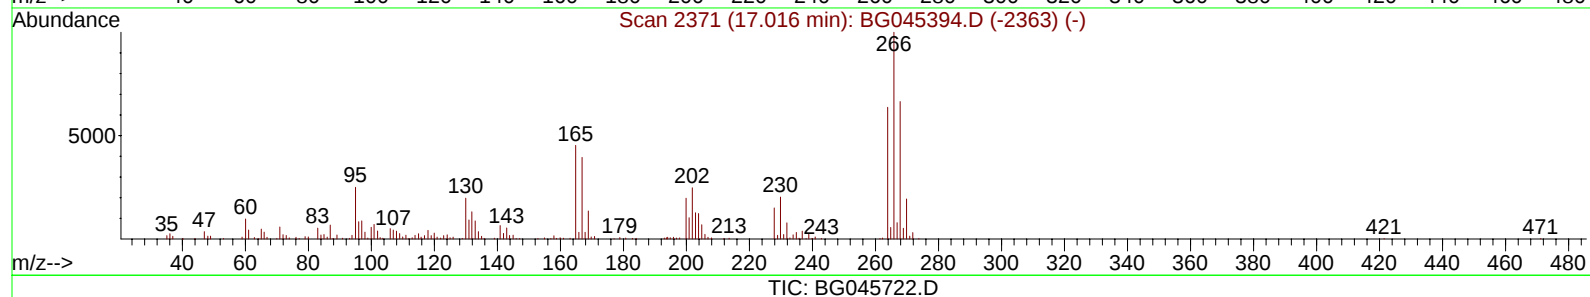
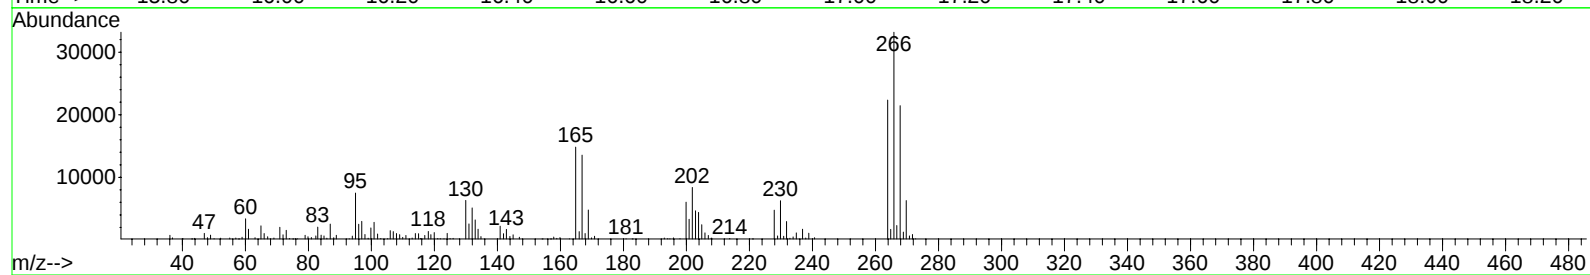


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061120\
Data File : BG045722.D
Acq On : 11 Jun 2020 14:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 18:05:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 01 15:07:00 2020
Response via : Initial Calibration

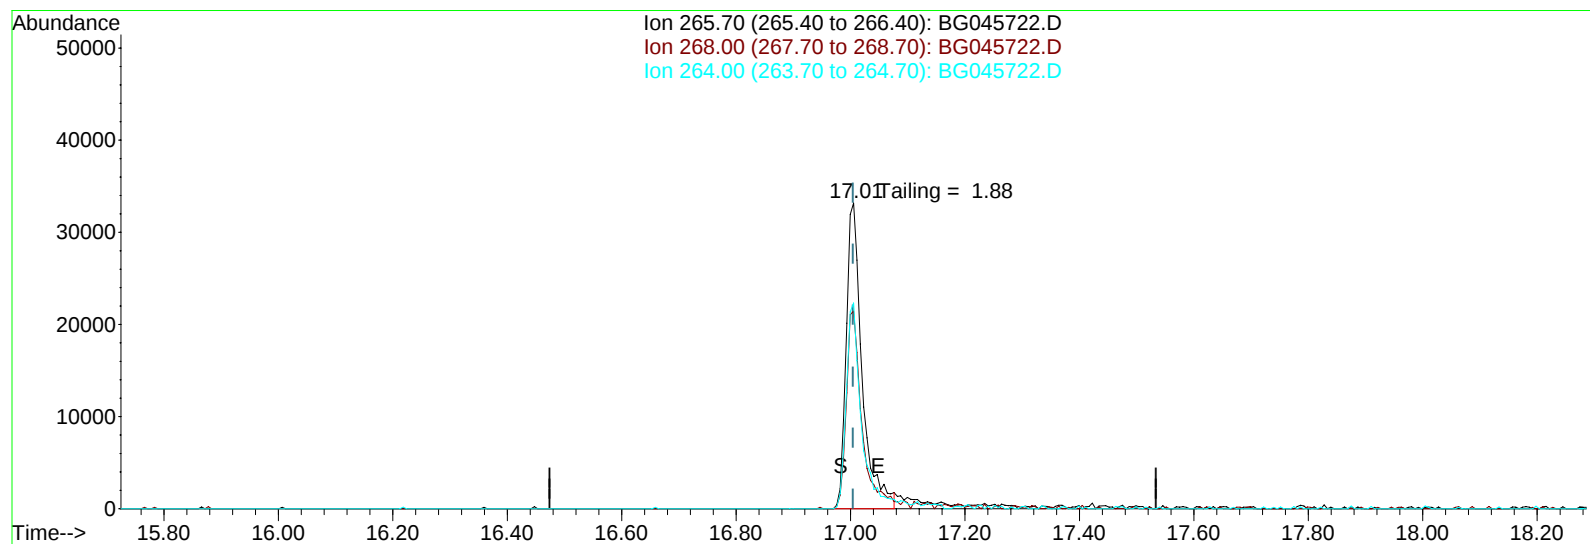

(70) Pentachlorophenol (C)




17.005min (+0.002) 203634.10ng

response 68258

Ion	Exp%	Act%
265.70	100	100
268.00	66.50	64.61
264.00	63.70	67.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061120\
 Data File : BG045722.D
 Acq On : 11 Jun 2020 14:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 18:05:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 01 15:07:00 2020
 Response via : Initial Calibration

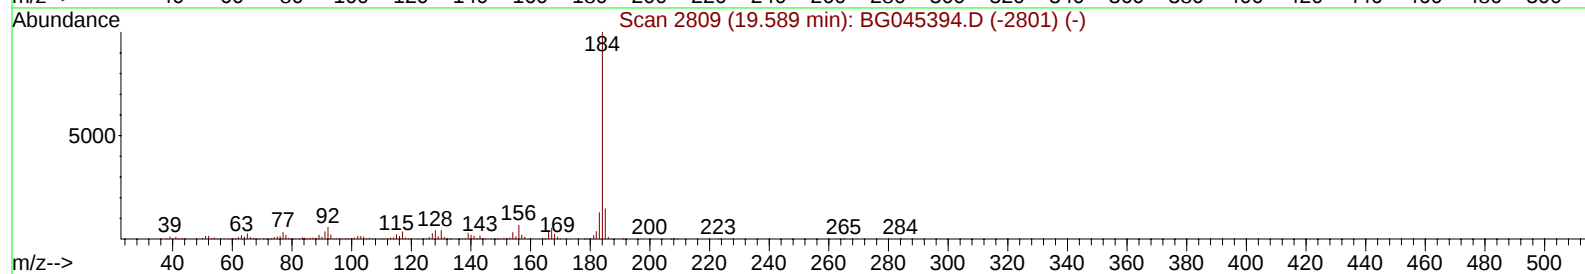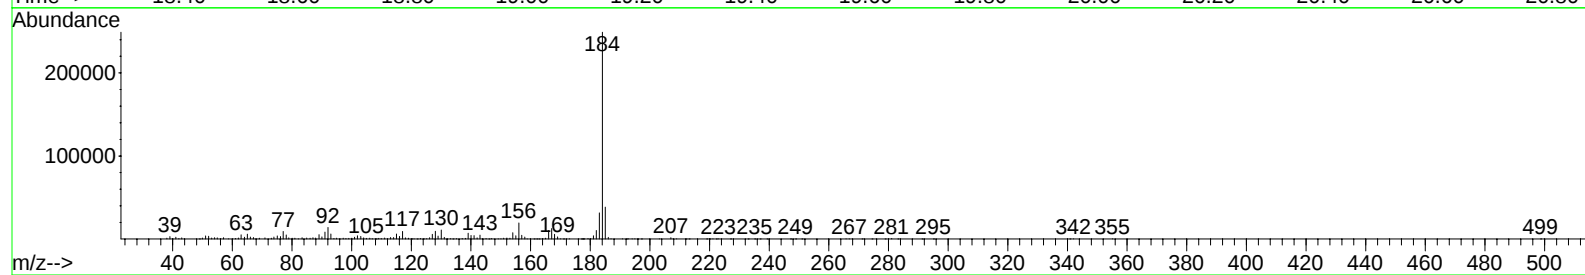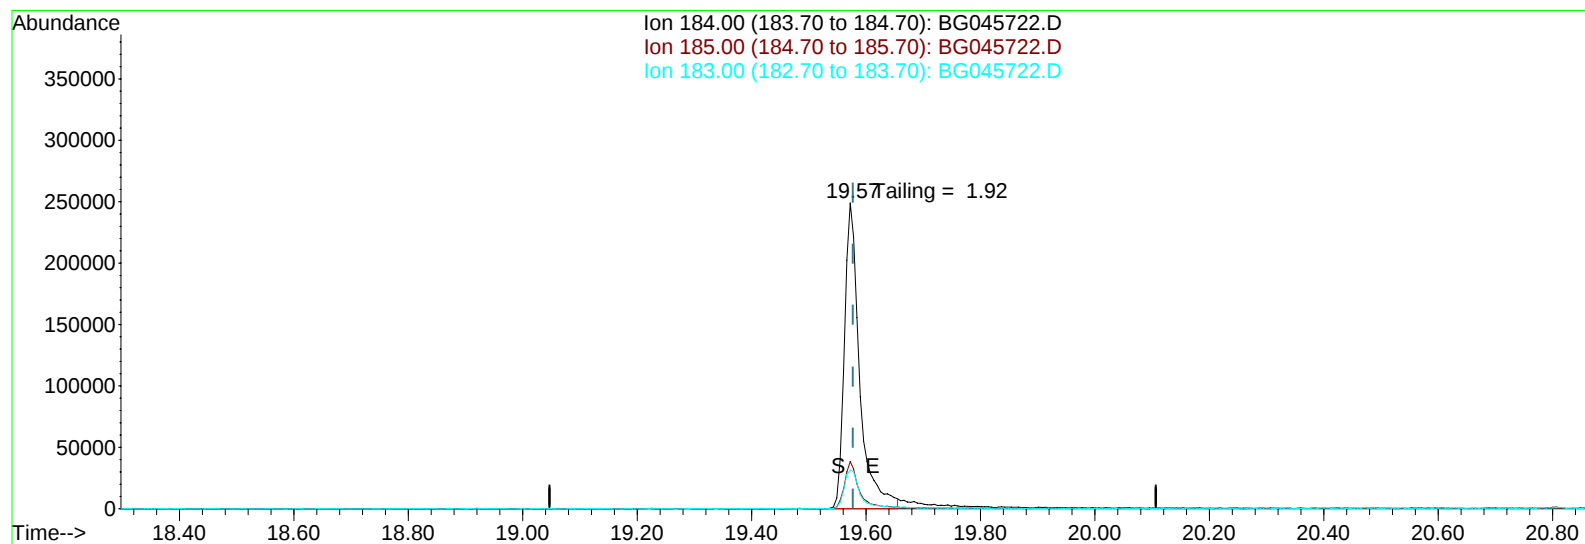

TIC: BG045722.D

(77) Benzidine

19.572min (-0.004) 61484.11ng

response 493868

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	15.46
183.00	12.80	12.66
0.00	0.00	0.00