


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061120\
 Data File : BG045722.D
 Acq On : 11 Jun 2020 14:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG051520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 01 15:07:00 2020

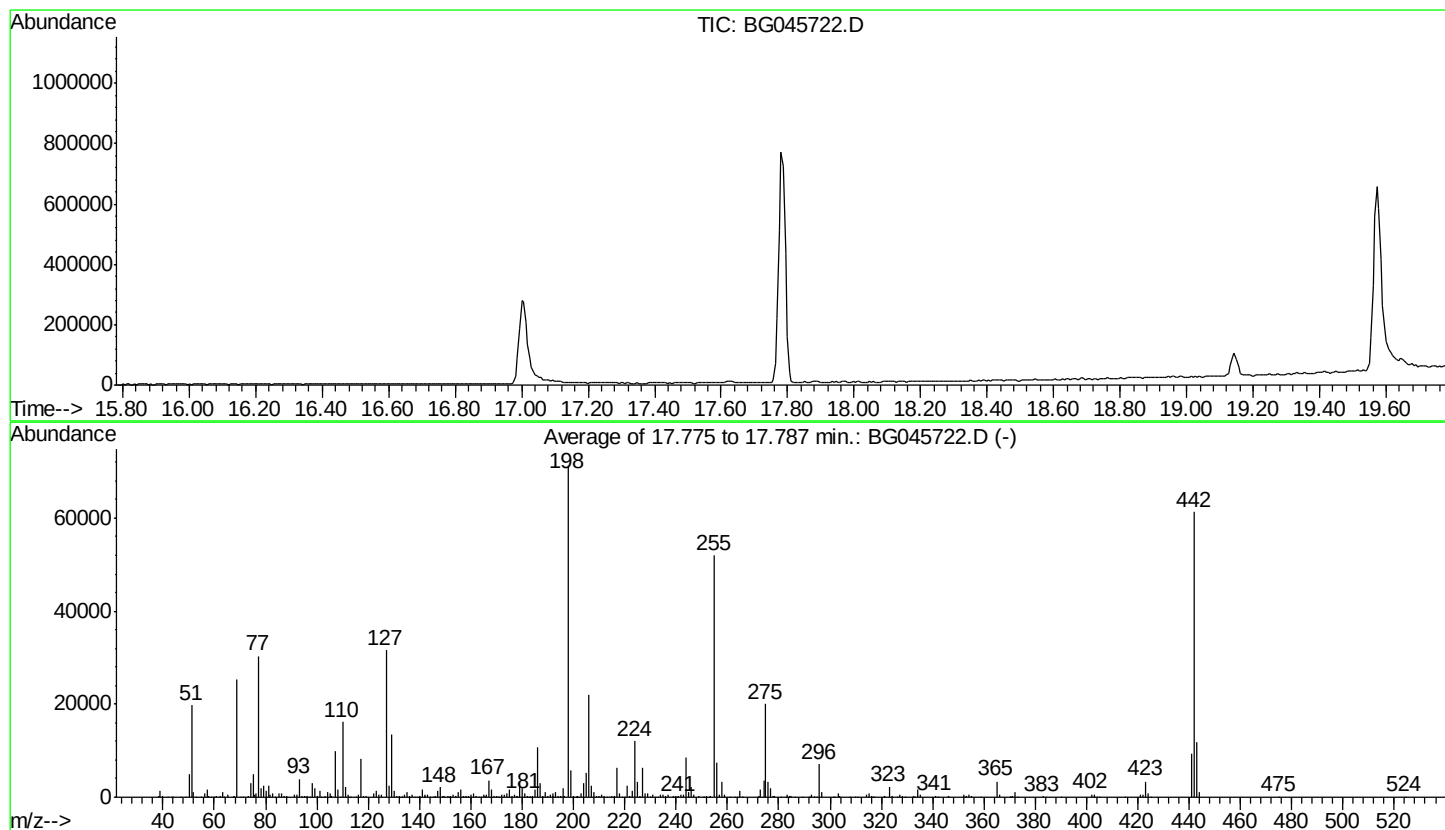

AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.7	19736	PASS
68	69	0.00	2	1.6	396	PASS
69	198	0.00	100	35.7	25404	PASS
70	69	0.00	2	0.2	57	PASS
127	198	10	80	44.3	31541	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	71256	PASS
199	198	5	9	8.2	5826	PASS
275	198	10	60	28.0	19953	PASS
365	198	1	100	4.8	3421	PASS
441	198	0.01	100	13.1	9299	PASS
442	198	50	100	86.0	61245	PASS
443	442	15	24	19.4	11855	PASS