
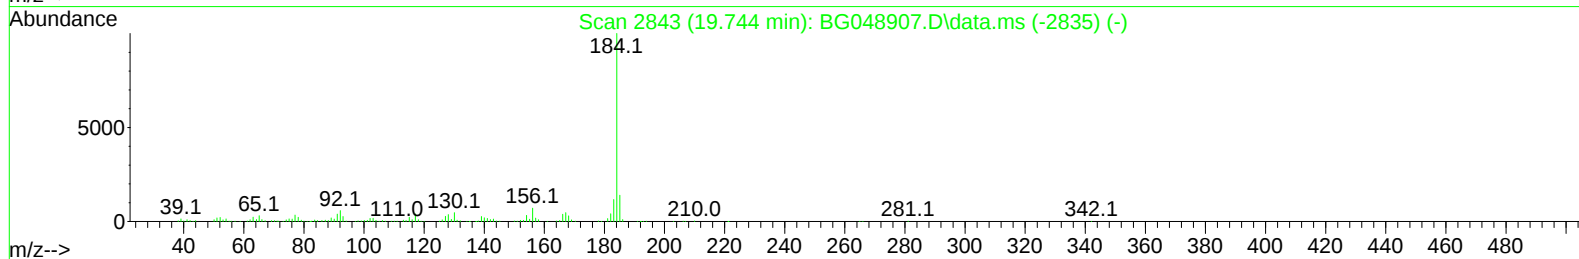
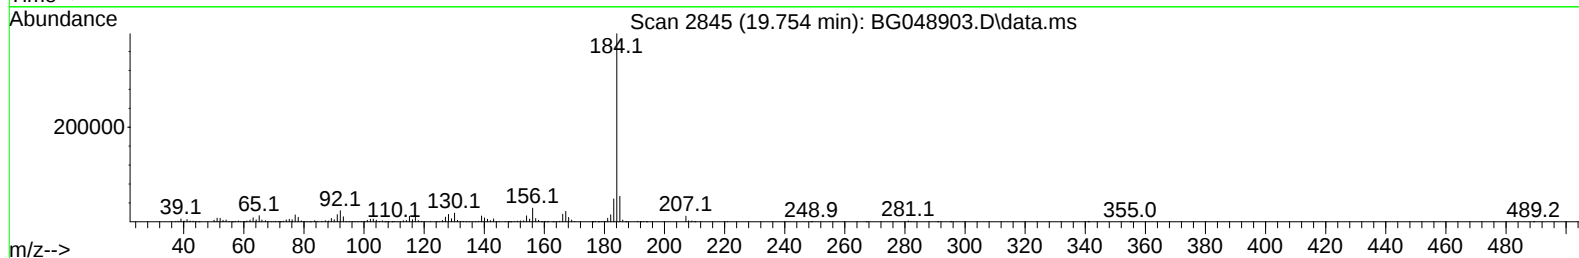


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061121\
Data File : BG048903.D
Acq On : 11 Jun 2021 9:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 14:14:14 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 11 13:47:28 2021
Response via : Initial Calibration

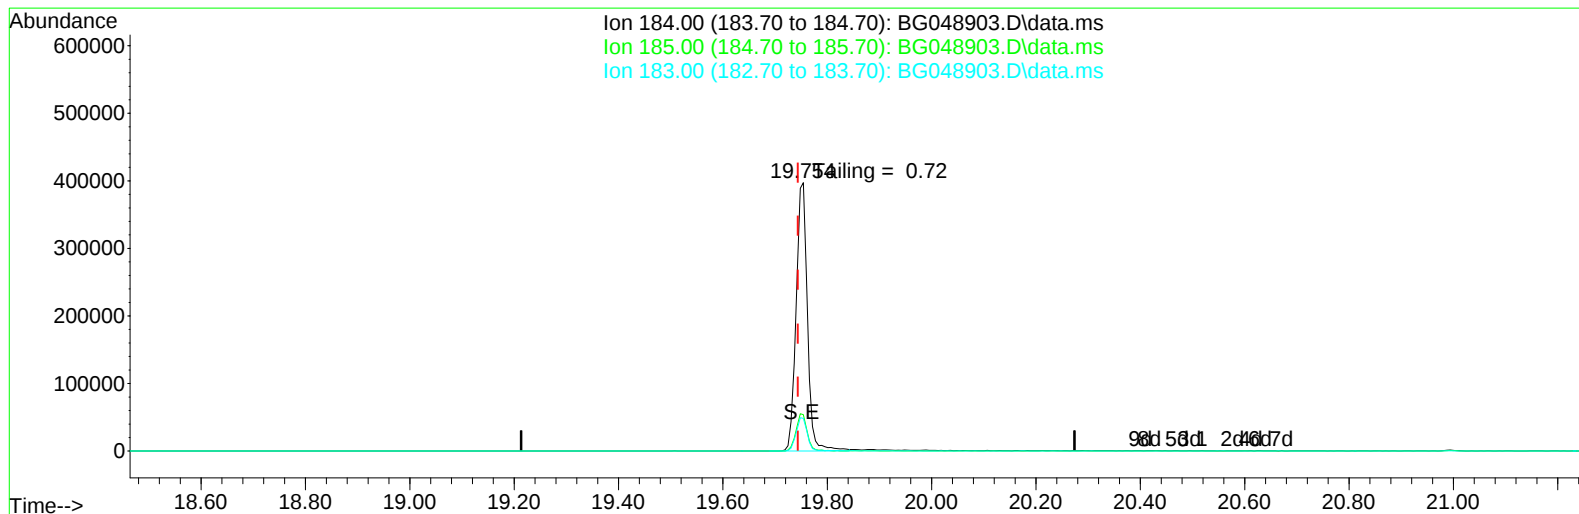

TIC: BG048903.D\data.ms

(77) Benzidine




19.754min (+ 0.010) 418422.30 ng m

response 624954

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.54
183.00	11.70	12.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061121\
 Data File : BG048903.D
 Acq On : 11 Jun 2021 9:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 14:14:14 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 11 13:47:28 2021
 Response via : Initial Calibration

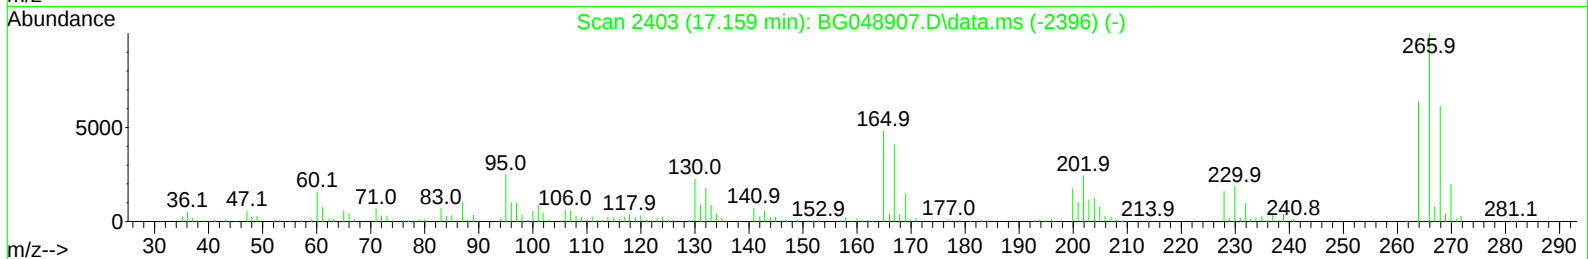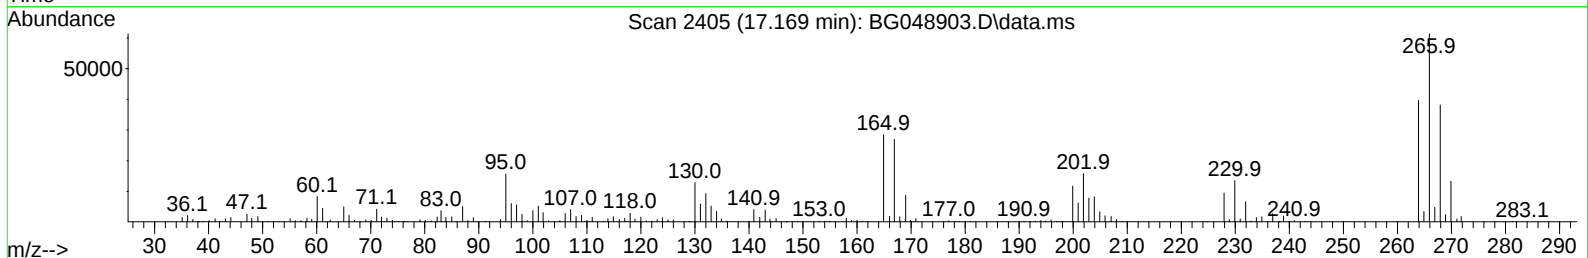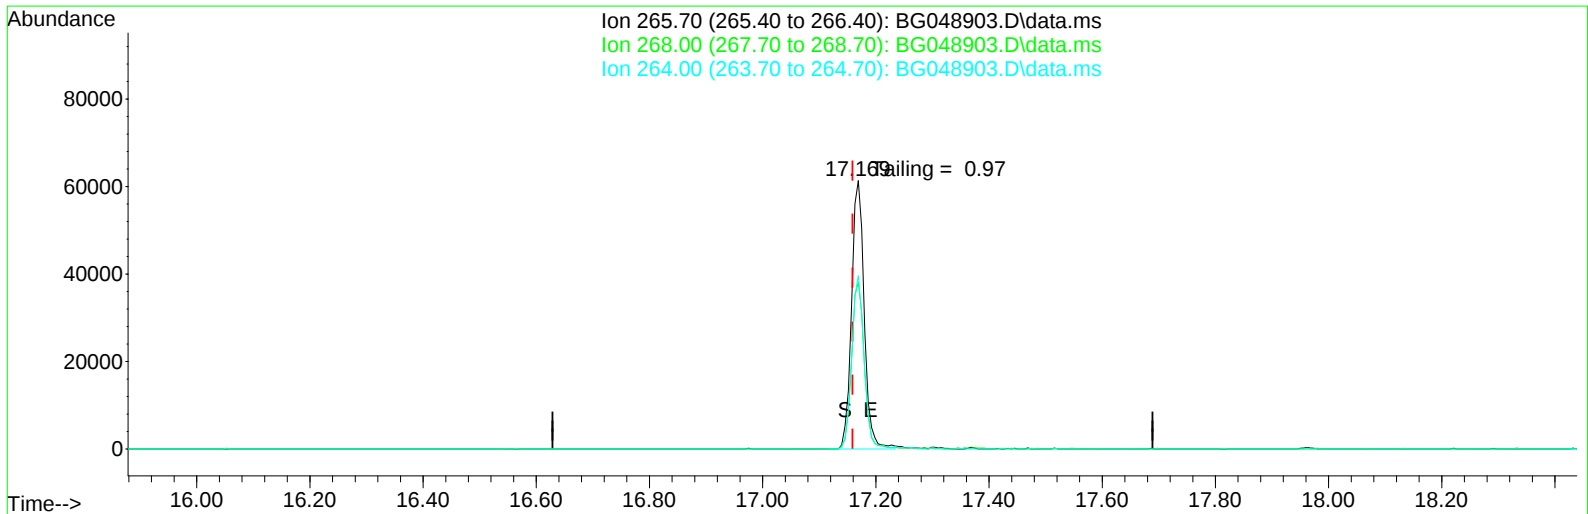

TIC: BG048903.D\data.ms

(70) Pentachlorophenol (C)

17.169min (+ 0.010) 22826.99 ng

response 94727

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.19
264.00	61.30	64.58
0.00	0.00	0.00