


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061121\
 Data File : BG048903.D
 Acq On : 11 Jun 2021 9:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 11 16:03:10 2021

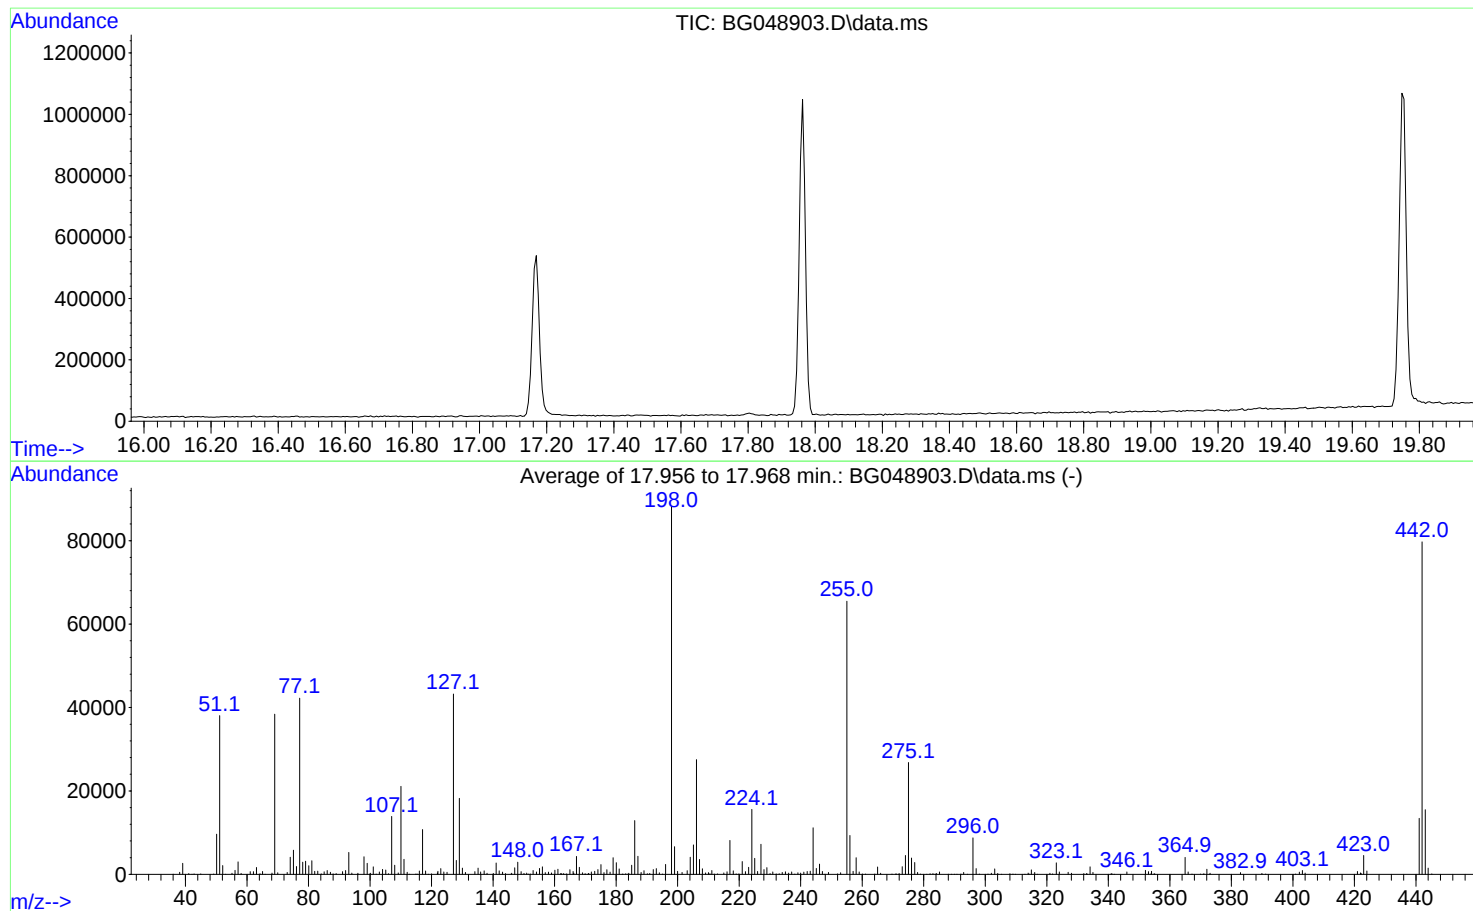




AutoFind: Scans 2539, 2540, 2541; Background Corrected with Scan 2532

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.1	38048	PASS
68	69	0.00	2	0.8	299	PASS
69	198	0.00	100	43.6	38418	PASS
70	69	0.00	2	1.0	398	PASS
127	198	10	80	49.0	43243	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	88192	PASS
199	198	5	9	7.5	6636	PASS
275	198	10	60	30.4	26813	PASS
365	198	1	100	4.6	4081	PASS
441	198	0.01	100	15.2	13447	PASS
442	198	50	100	90.4	79712	PASS
443	442	15	24	19.4	15486	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061121\
Data File : BG048903.D
Acq On : 11 Jun 2021 9:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 11 14:14:14 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 11 13:47:28 2021
Response via : Initial Calibration

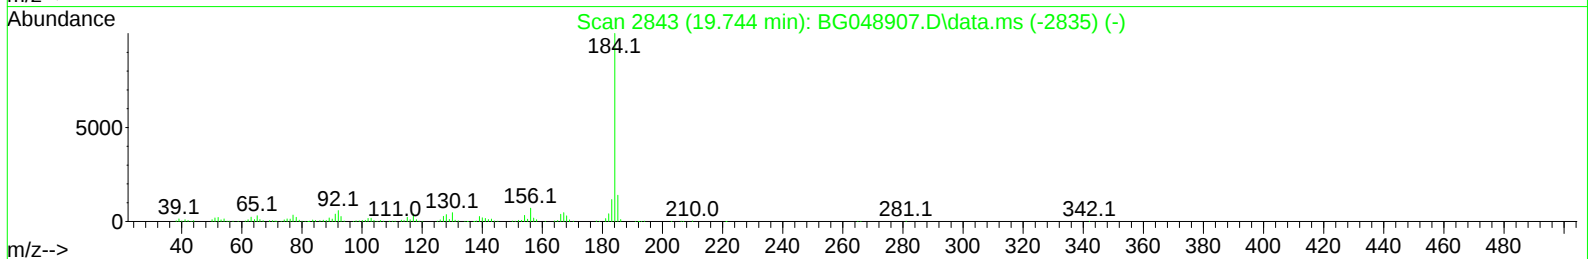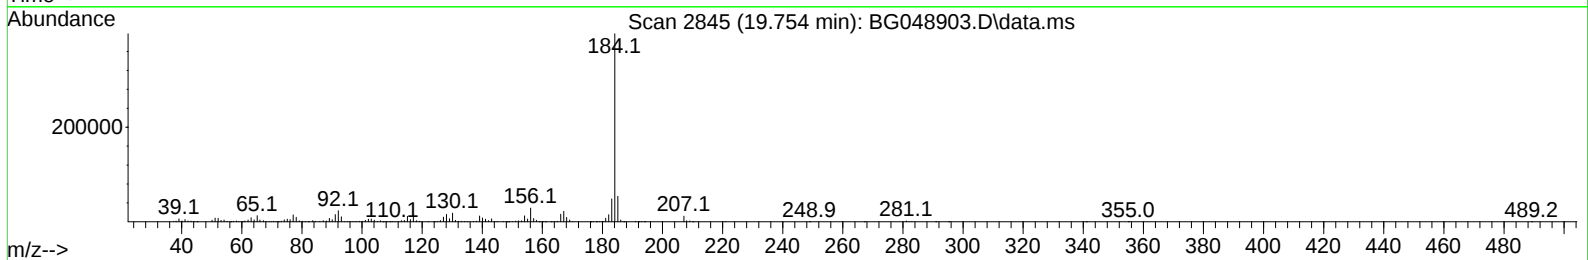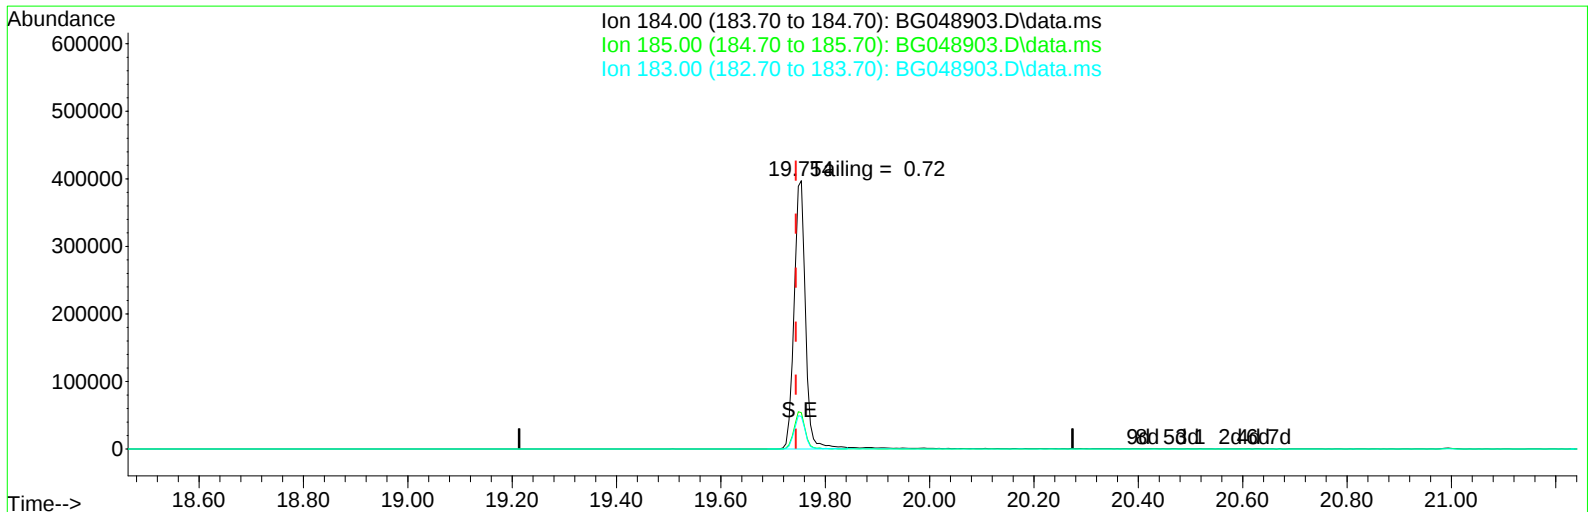

TIC: BG048903.D\data.ms

(77) Benzidine

19.754min (+ 0.010) 418422.30 ng m




response 624954

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.54
183.00	11.70	12.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061121\
 Data File : BG048903.D
 Acq On : 11 Jun 2021 9:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jun 11 14:14:14 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 11 13:47:28 2021
 Response via : Initial Calibration

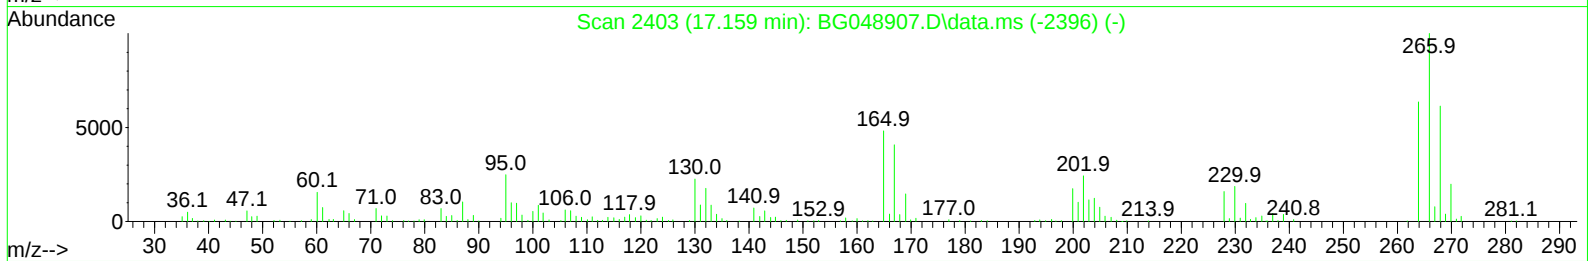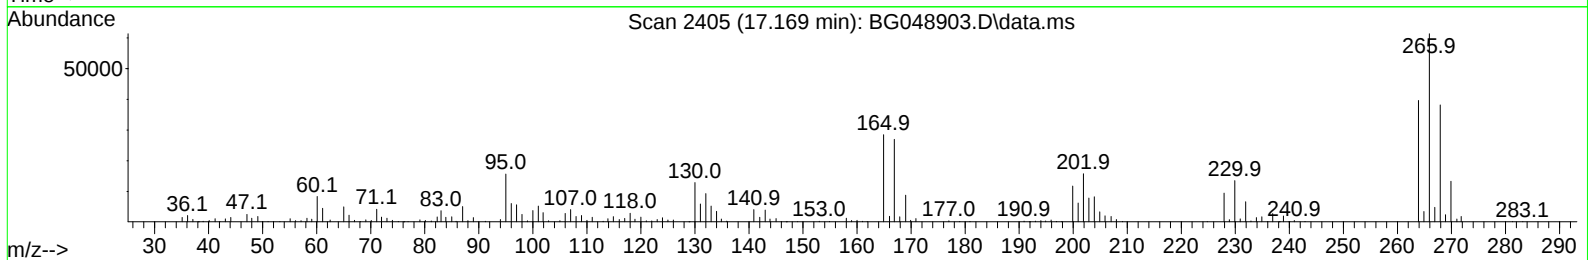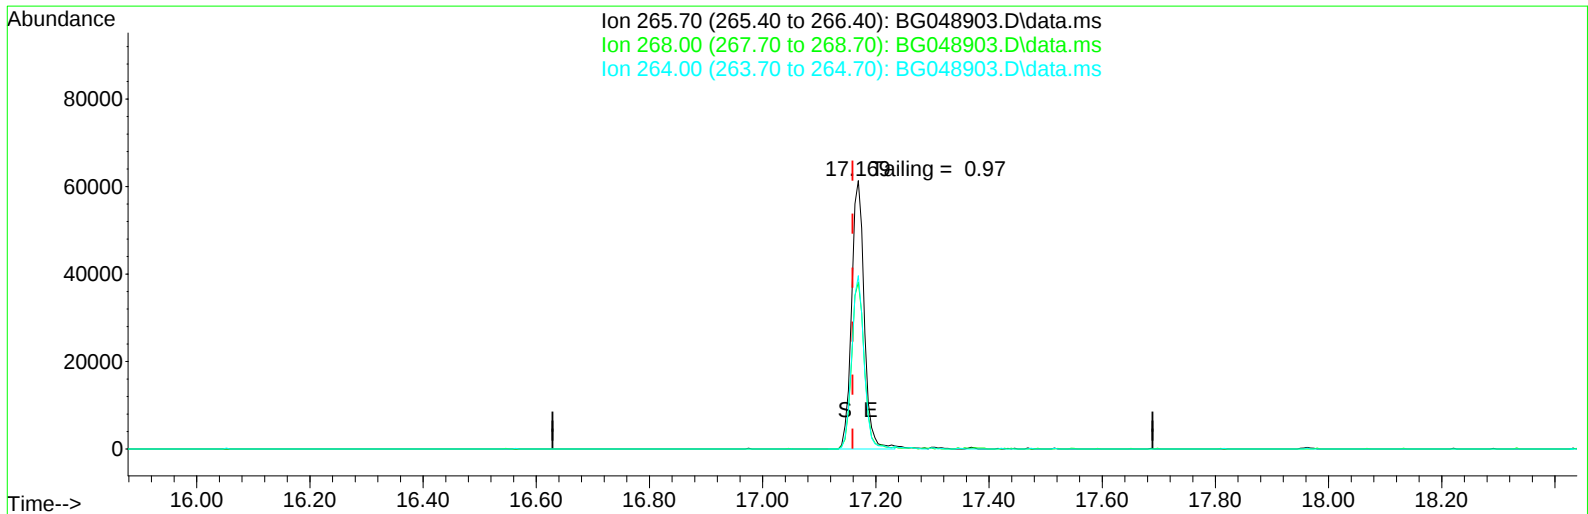

TIC: BG048903.D\data.ms

(70) Pentachlorophenol (C)

17.169min (+ 0.010) 22826.99 ng

response 94727

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.19
264.00	61.30	64.58
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/11/2021	BNA_G	BG048903.D
Compound Name	Response	Retention Time
DDT	263932	20.99
DDD	2247	20.54
DDE	378	20.03
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2625	266557	0.98