
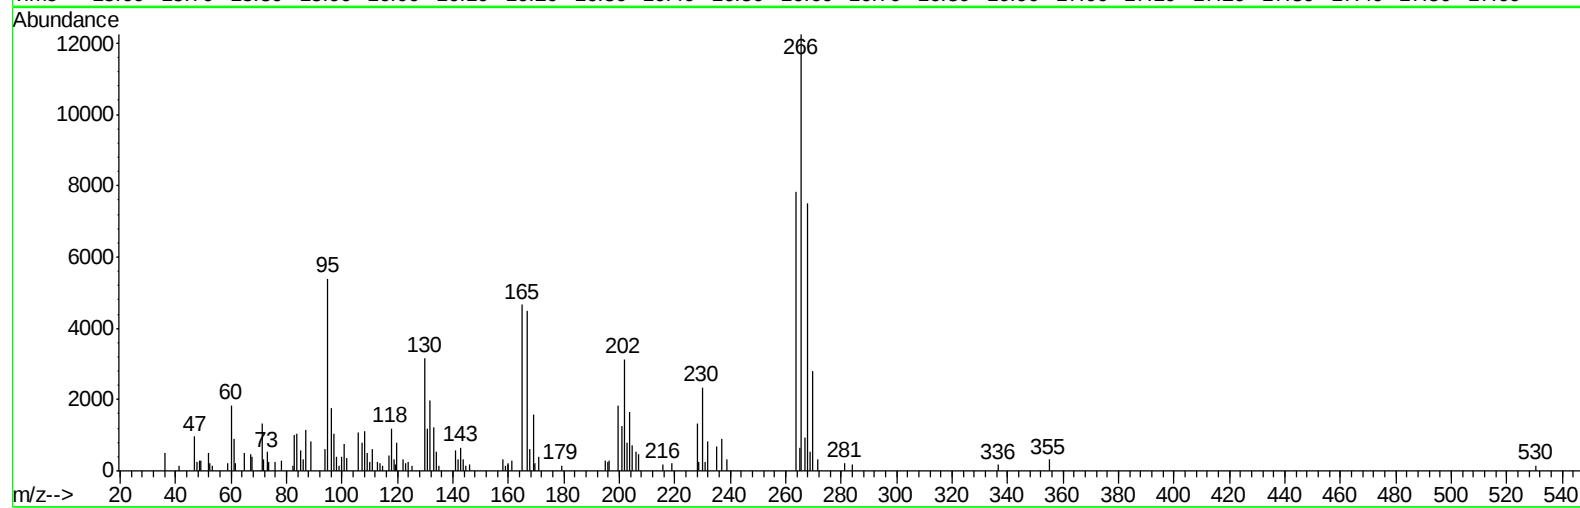


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061215\
Data File : BG017637.D
Acq On : 12 Jun 2015 14:18
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 07:28:44 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 13 02:22:44 2015
Response via : Initial Calibration

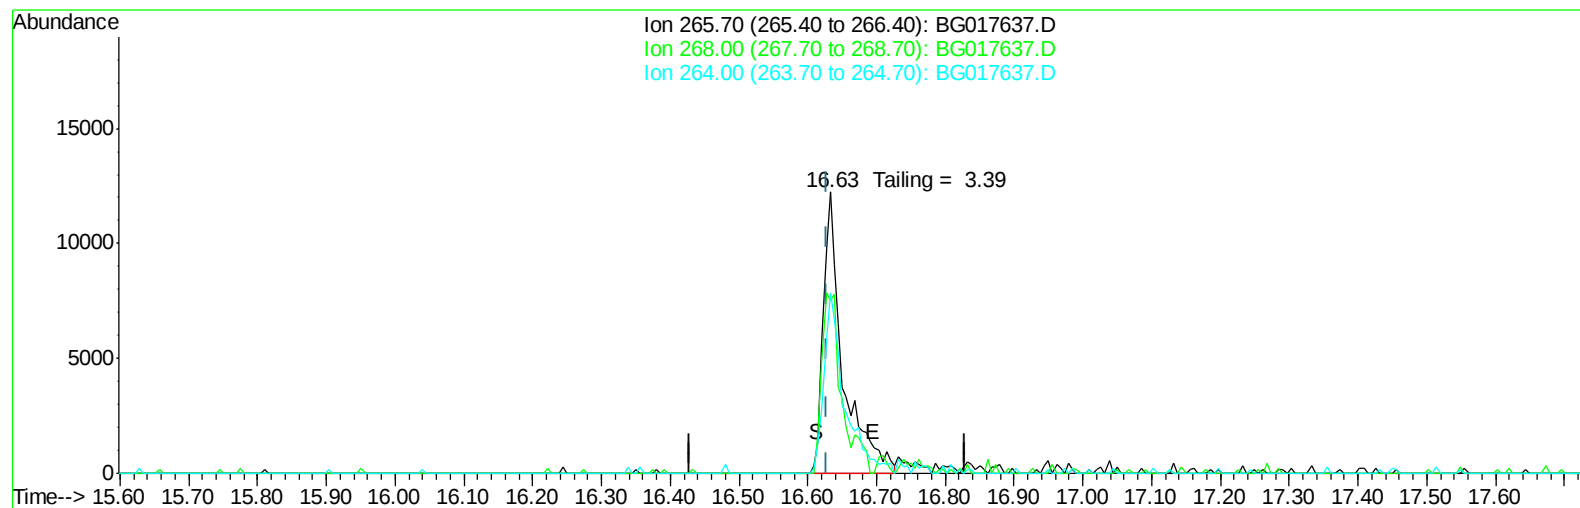

TIC: BG017637.D

(69) Pentachlorophenol (C)



16.633min (+0.004) 41668.09ng

response 24399

Ion	Exp%	Act%
265.70	100	100
268.00	65.90	65.64
264.00	65.30	63.91
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061215\
Data File : BG017637.D
Acq On : 12 Jun 2015 14:18
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 07:28:44 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 13 02:22:44 2015
Response via : Initial Calibration

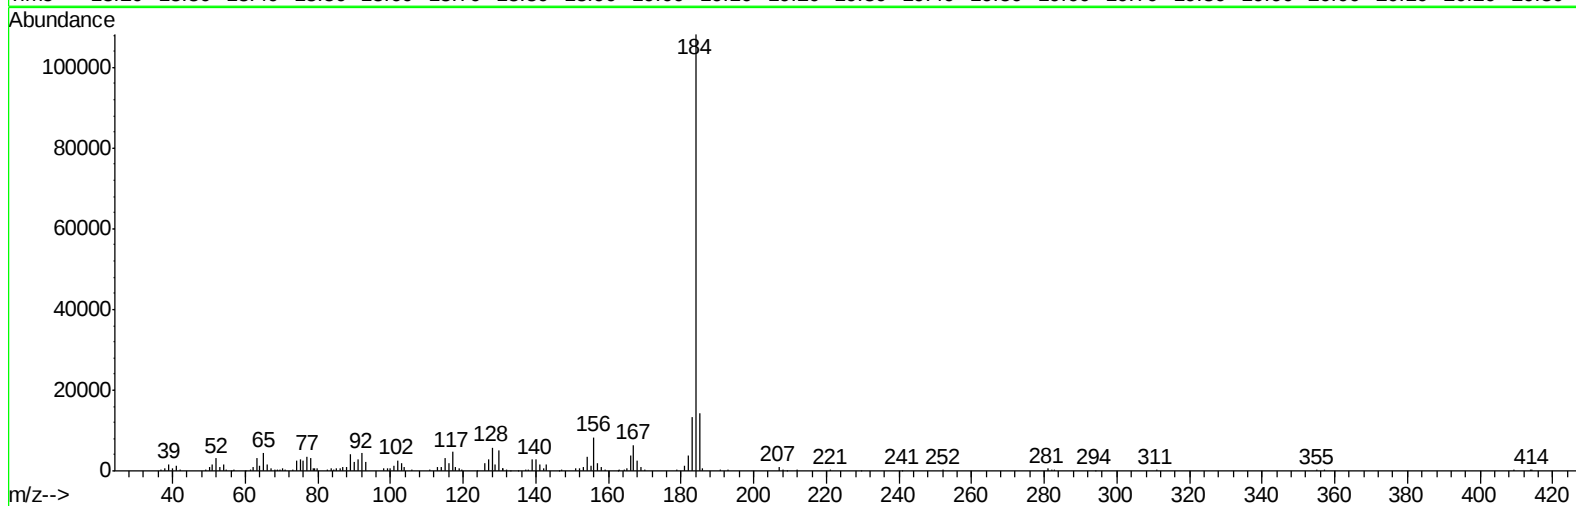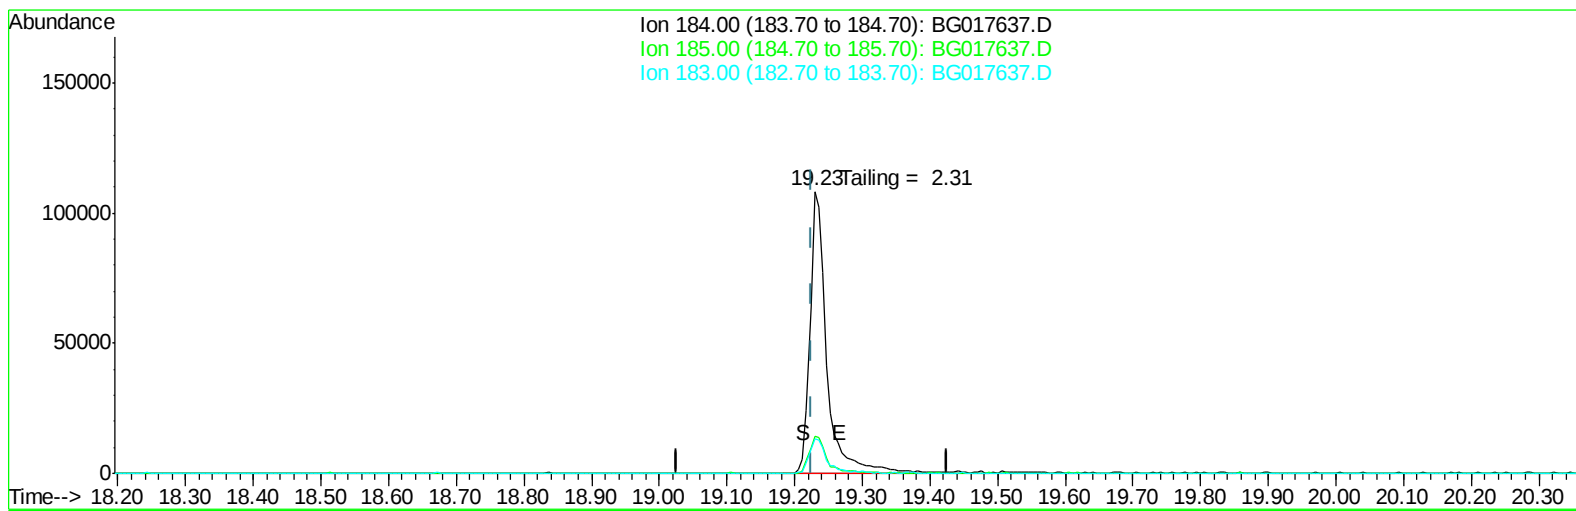

TIC: BG017637.D

(76) Benzidine

19.229min (+0.003) 107163.34ng

response 185322

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	13.12
183.00	14.00	12.42
0.00	0.00	0.00