
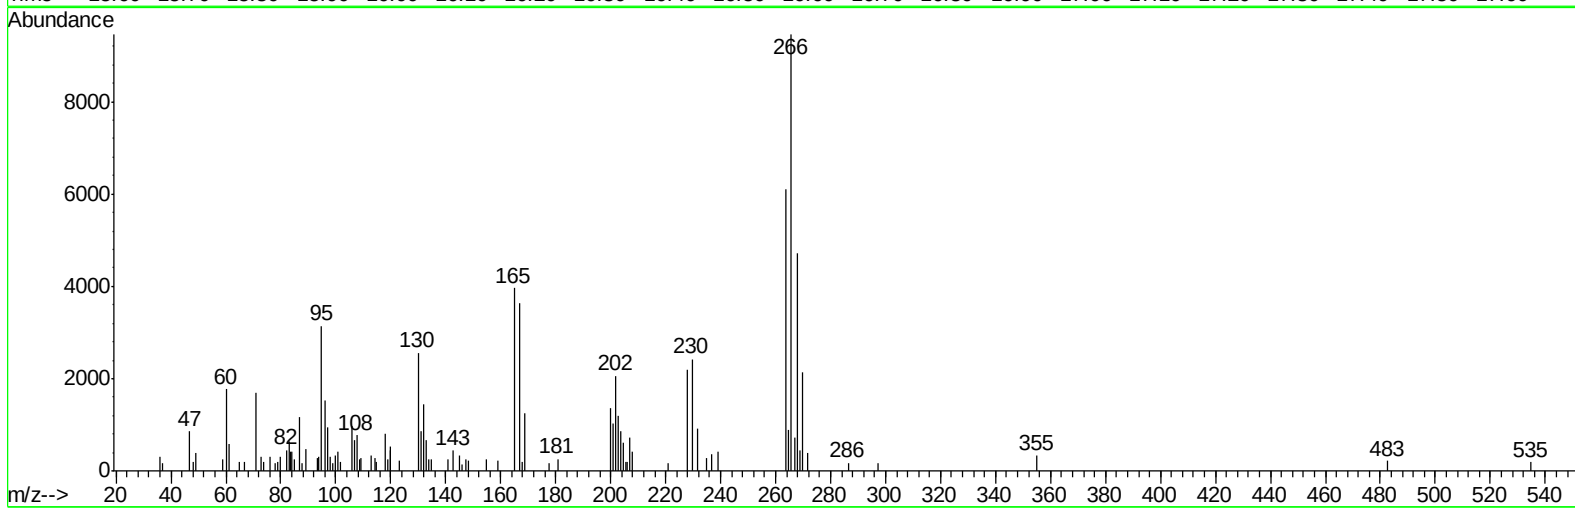


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061215\
Data File : BG017674.D
Acq On : 13 Jun 2015 14:46
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 07:31:52 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 13 02:22:44 2015
Response via : Initial Calibration

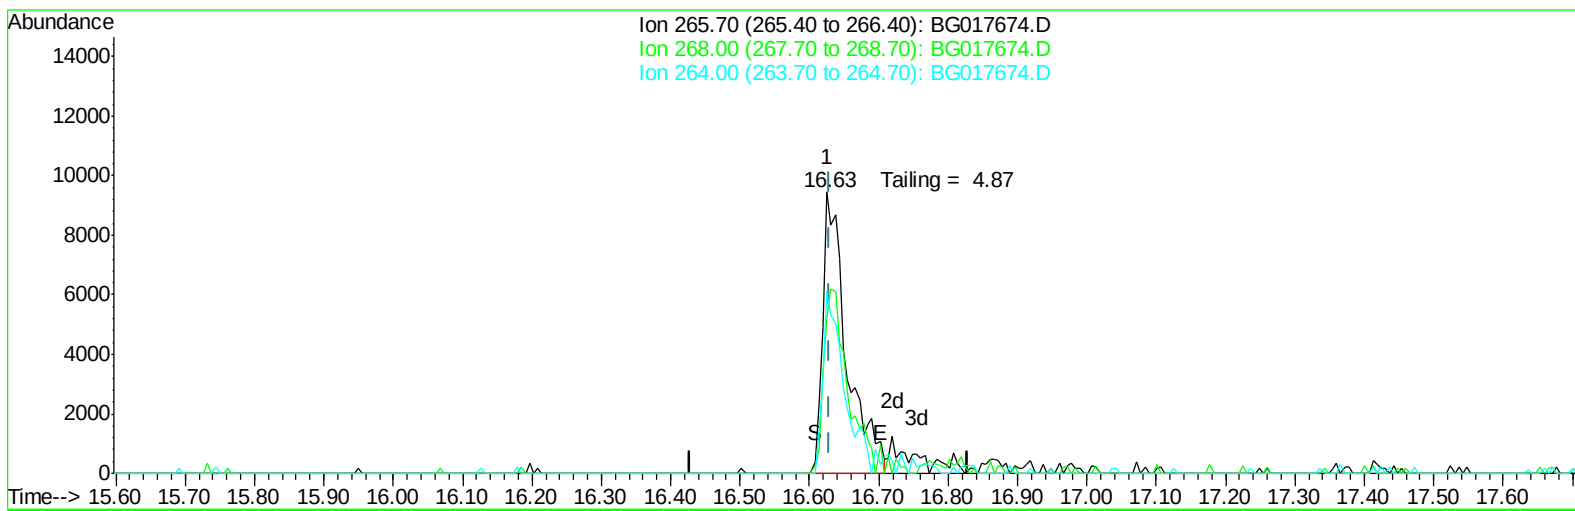

TIC: BG017674.D

(69) Pentachlorophenol (C)



16.625min (-0.004) 43974.99ng

response 22571

Ion	Exp%	Act%
265.70	100	100
268.00	65.90	54.80
264.00	65.30	64.45
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061215\
Data File : BG017674.D
Acq On : 13 Jun 2015 14:46
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 07:31:52 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 13 02:22:44 2015
Response via : Initial Calibration

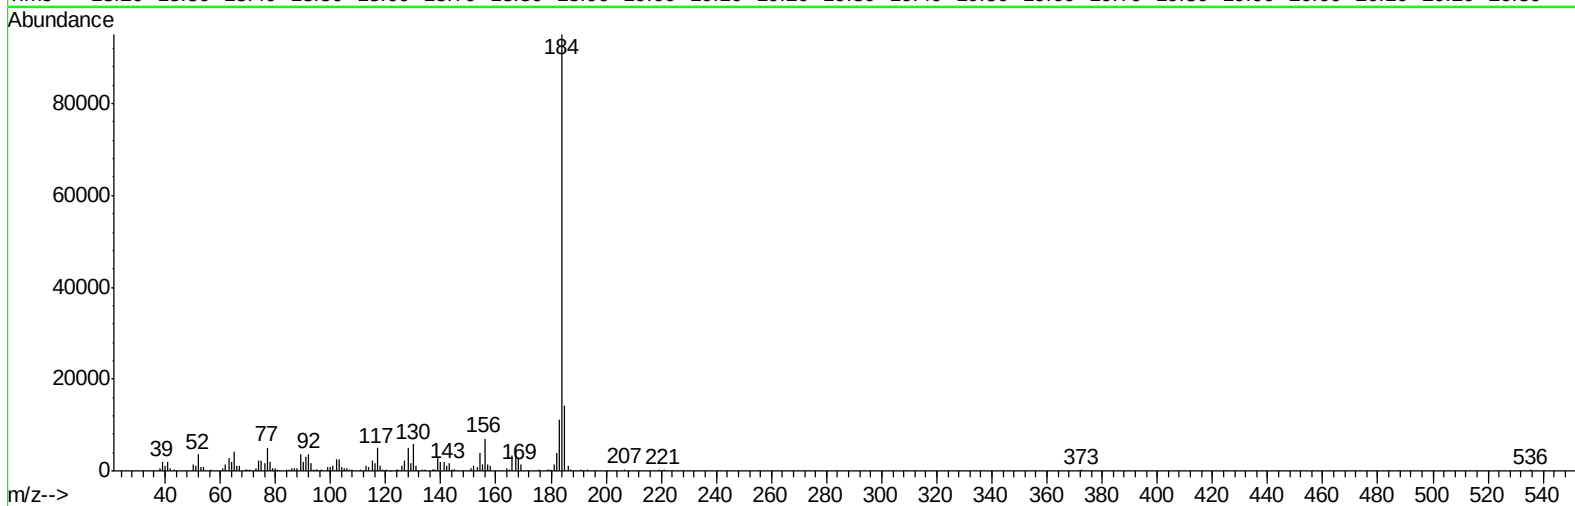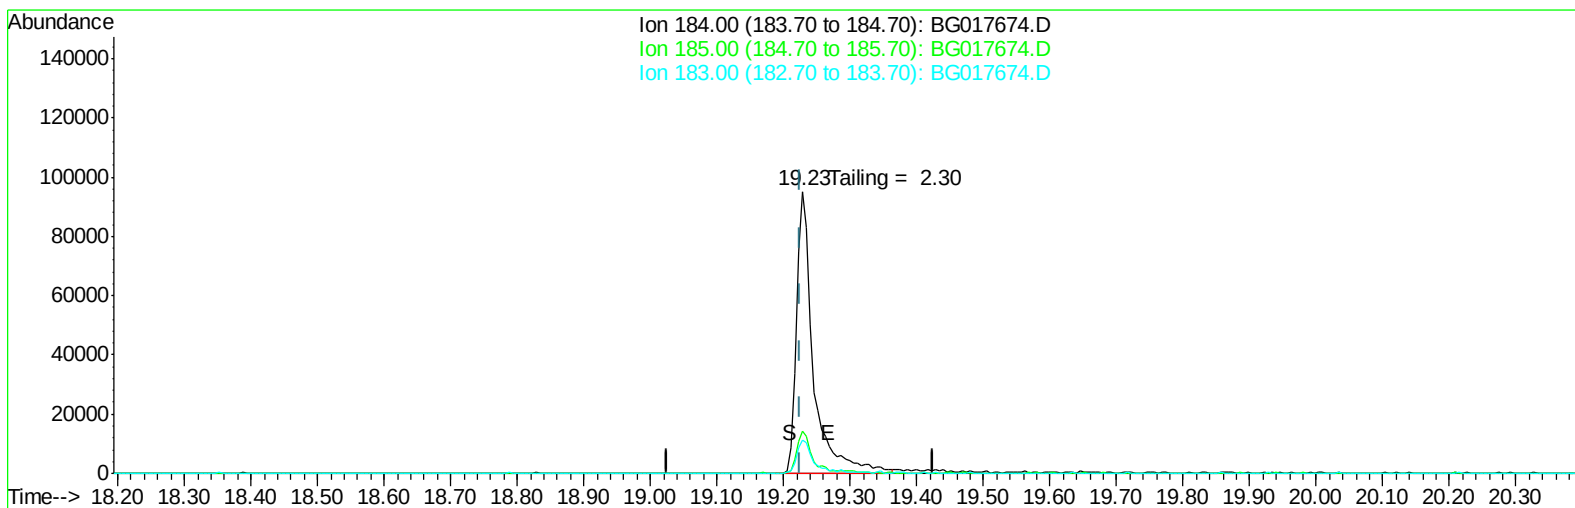

TIC: BG017674.D

(76) Benzidine

19.228min (+0.002) 125394.61ng

response 172894

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.89
183.00	14.00	11.75
0.00	0.00	0.00