

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061215\
 Data File : BG017679.D
 Acq On : 13 Jun 2015 18:16
 Operator : TP/IZ
 Sample : G2592-10
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TEC-C1

Quant Time: Jun 15 05:52:52 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 13 02:22:44 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	16804	20.00	ng	-0.01
21) Naphthalene-d8	10.32	136	63107	20.00	ng	0.00
38) Acenaphthene-d10	14.21	164	52955	20.00	ng	0.00
63) Phenanthrene-d10	16.96	188	150991	20.00	ng	0.00
75) Chrysene-d12	21.16	240	224190	20.00	ng	0.00
86) Perylene-d12	23.36	264	223943	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.11	112	113845	131.21	ng	0.00
7) Phenol-d6	6.74	99	146102	114.92	ng	0.00
23) Nitrobenzene-d5	8.69	82	130276	86.66	ng	0.00
41) 2,4,6-Tribromophenol	15.71	330	110951	121.38	ng	0.00
44) 2-Fluorobiphenyl	12.82	172	313724	81.94	ng	0.00
78) Terphenyl-d14	19.61	244	929532	86.49	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061215\
Data File : BG017679.D
Acq On : 13 Jun 2015 18:16
Operator : TP/IZ
Sample : G2592-10
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TEC-C1

Quant Time: Jun 15 05:52:52 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 13 02:22:44 2015
Response via : Initial Calibration

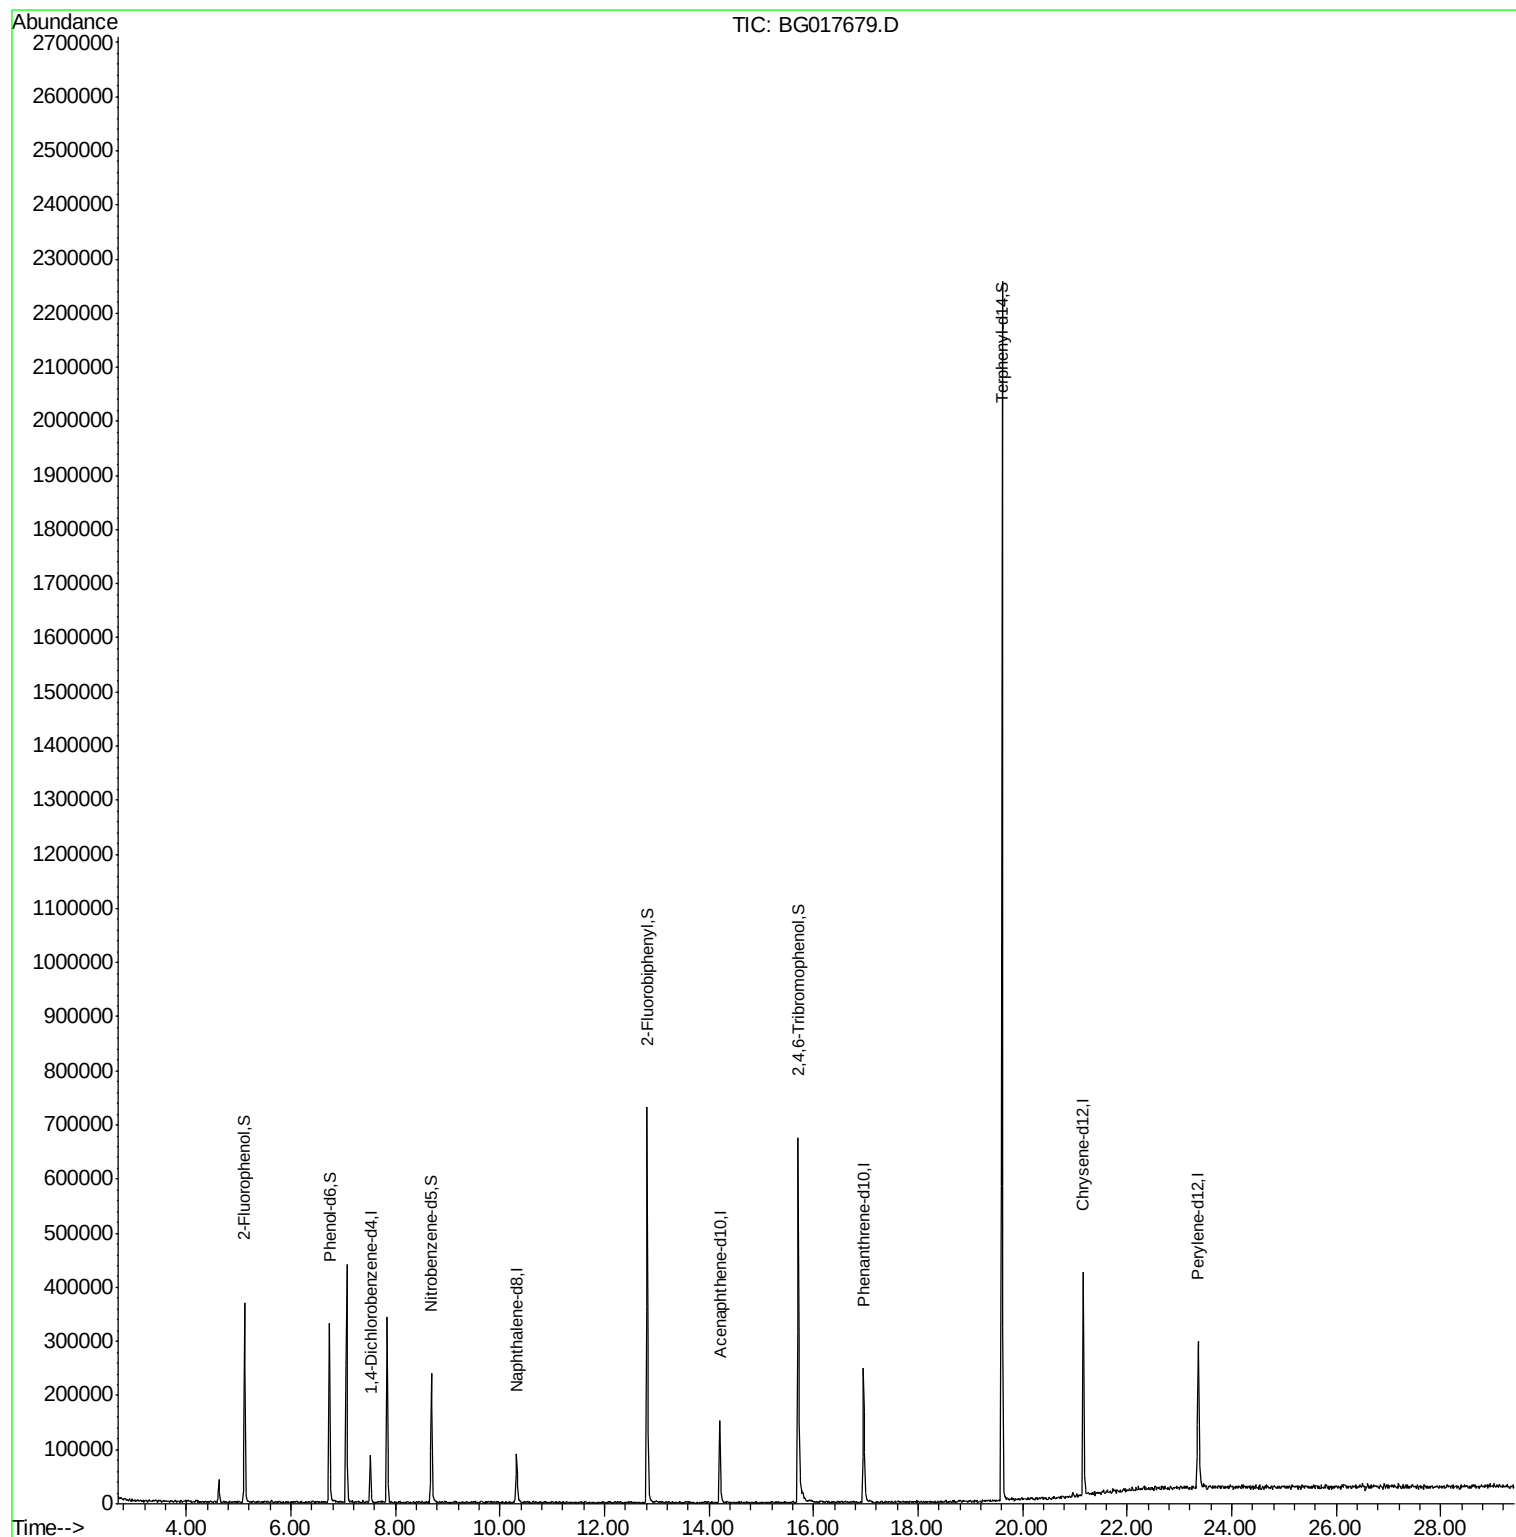




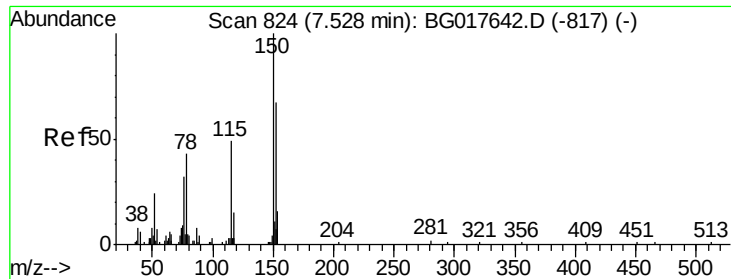


#1

1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.52 min Scan# 822
Delta R.T. -0.01 min
Lab File: BG017679.D
Acq: 13 Jun 2015 18:16

Instrument :
BNA_G
ClientSampleId :
TEC-C1




Tgt Ion:152 Resp: 16804
Ion Ratio Lower Upper
152 100
150 138.8 119.4 179.0
115 56.9 58.2 87.2#

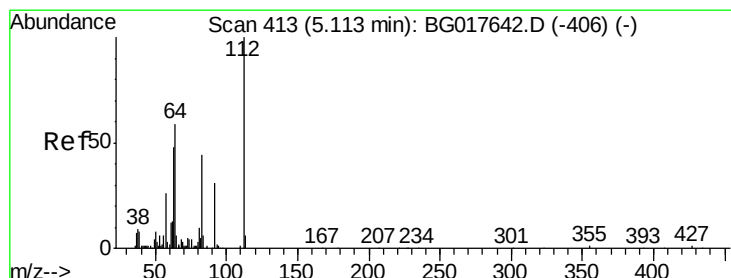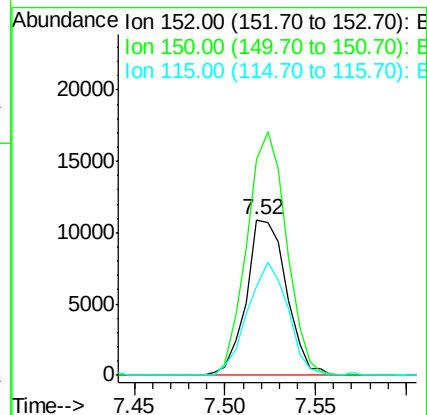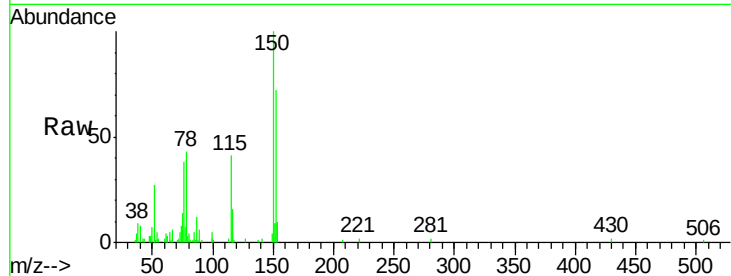


#5

2-Fluorophenol
Concen: 131.21 ng
RT: 5.11 min Scan# 413
Delta R.T. 0.00 min
Lab File: BG017679.D
Acq: 13 Jun 2015 18:16

Tgt Ion:112 Resp: 113845
Ion Ratio Lower Upper
112 100
64 57.3 47.0 70.6
63 41.7 38.6 58.0

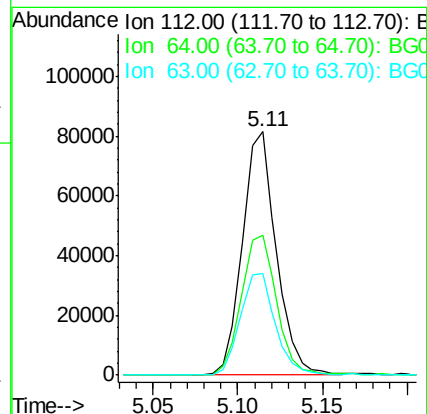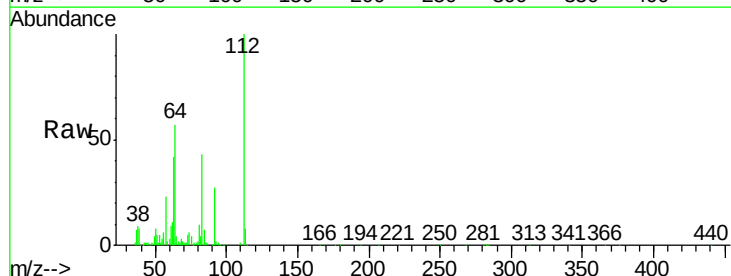



#7

Phenol-d6

Concen: 114.92 ng

RT: 6.74 min Scan# 689

Delta R.T. 0.00 min

Lab File: BG017679.D

Acq: 13 Jun 2015 18:16

Instrument :

BNA_G

ClientSampleId :

TEC-C1


Tgt Ion: 99 Resp: 146102

Ion Ratio Lower Upper




99 100

42 20.5 17.4 26.2

71 61.8 47.4 71.0

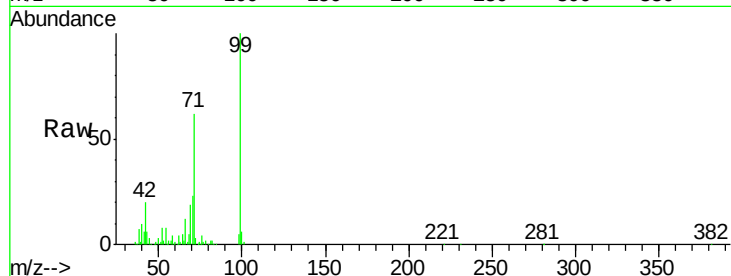

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

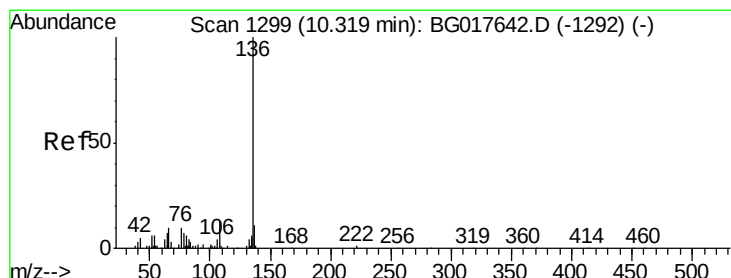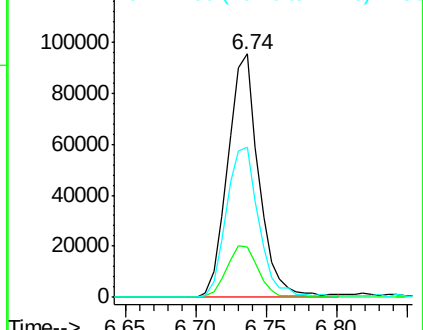

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.32 min Scan# 1299

Delta R.T. 0.00 min

Lab File: BG017679.D

Acq: 13 Jun 2015 18:16

Tgt Ion: 136 Resp: 63107


Ion Ratio Lower Upper

136 100



137 9.8 8.7 13.1


54 6.6 4.7 7.1

68 3.6 2.4 3.6

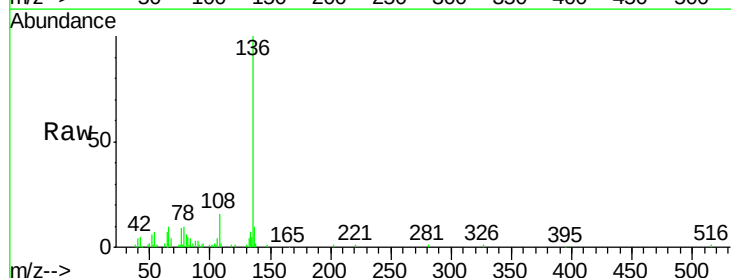

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



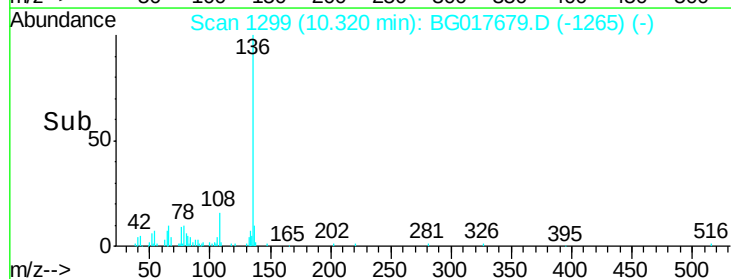
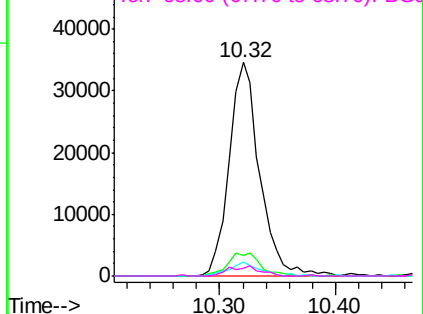




#23
 Nitrobenzene-d5
 Concen: 86.66 ng
 RT: 8.69 min Scan# 1022
 Delta R.T. 0.00 min
 Lab File: BG017679.D
 Acq: 13 Jun 2015 18:16




Instrument :
 BNA_G
 ClientSampleId :
 TEC-C1


Tgt Ion: 82 Resp: 130276
 Ion Ratio Lower Upper
 82 100
 128 35.7 27.3 40.9
 54 51.7 37.0 55.4

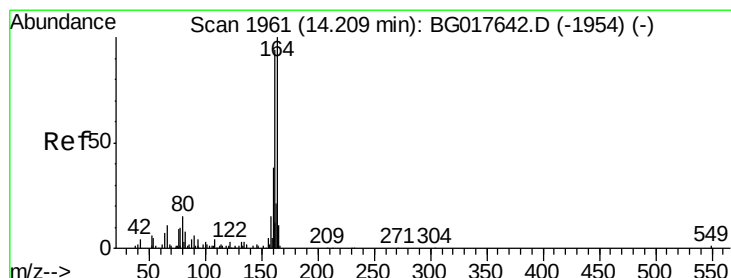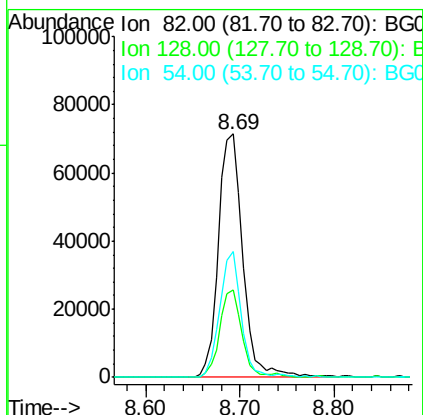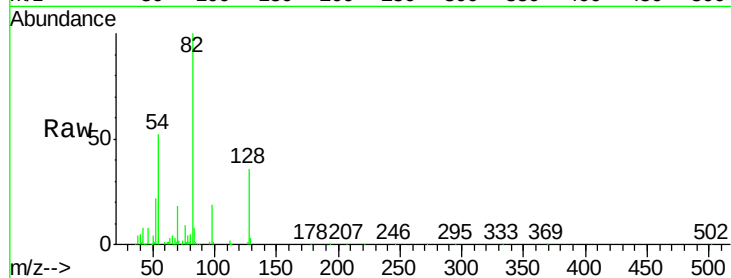

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.21 min Scan# 1961
 Delta R.T. 0.00 min
 Lab File: BG017679.D
 Acq: 13 Jun 2015 18:16

Tgt Ion: 164 Resp: 52955
 Ion Ratio Lower Upper
 164 100
 162 90.5 75.0 112.4
 160 36.3 30.3 45.5

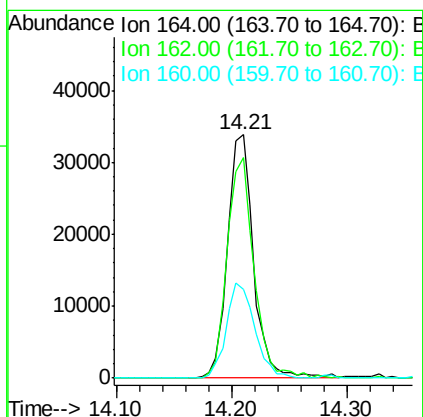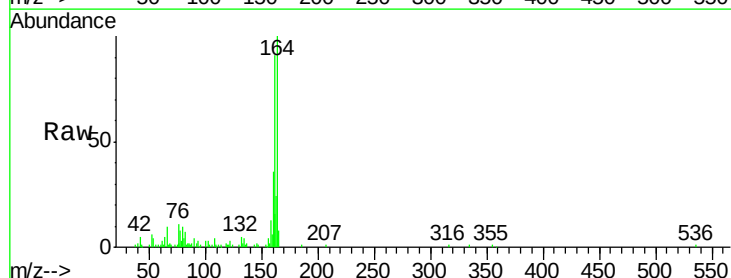







#41
 2,4,6-Tribromophenol
 Concen: 121.38 ng
 RT: 15.71 min Scan# 2216
 Delta R.T. -0.00 min
 Lab File: BG017679.D
 Acq: 13 Jun 2015 18:16

Instrument :
 BNA_G
 ClientSampled :
 TEC-C1

Tgt Ion:330 Resp: 110951
 Ion Ratio Lower Upper
 330 100
 332 98.0 76.6 114.8
 141 44.2 34.6 51.8

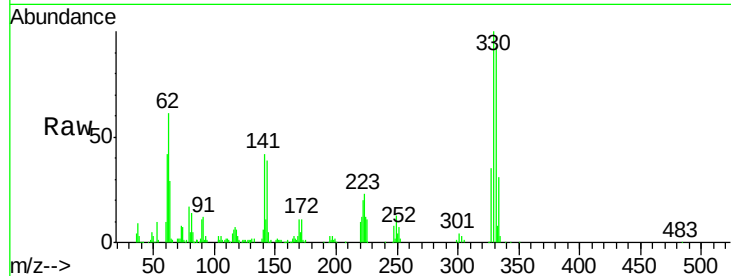


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

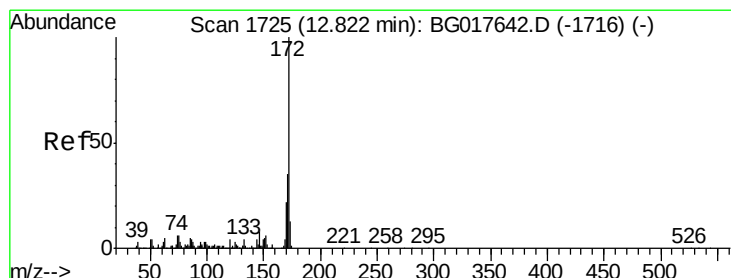
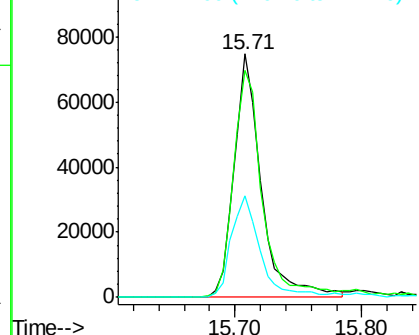



#44
 2-Fluorobiphenyl
 Concen: 81.94 ng
 RT: 12.82 min Scan# 1724
 Delta R.T. -0.00 min
 Lab File: BG017679.D
 Acq: 13 Jun 2015 18:16

Tgt Ion:172 Resp: 313724
 Ion Ratio Lower Upper
 172 100
 171 37.3 28.2 42.2
 170 22.8 17.4 26.2

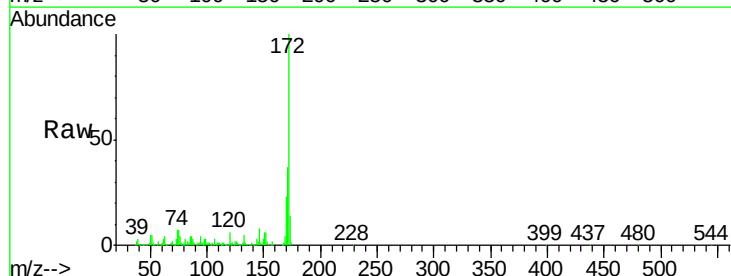

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

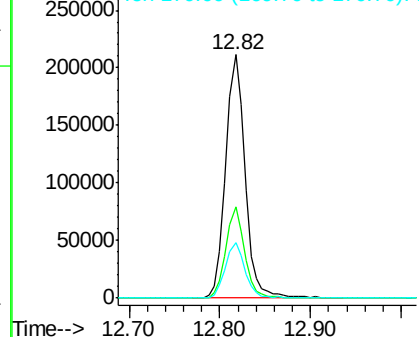







#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 16.96 min Scan# 2429
Delta R.T. -0.00 min
Lab File: BG017679.D
Acq: 13 Jun 2015 18:16

Instrument :
BNA_G
ClientSampleId :
TEC-C1

Tgt Ion:188 Resp: 150991
Ion Ratio Lower Upper
188 100
94 5.8 3.9 5.9
80 5.7 5.0 7.6

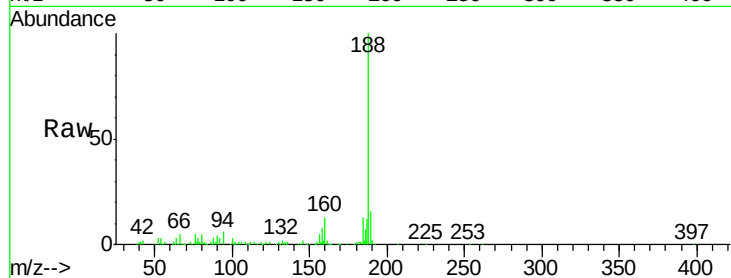


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

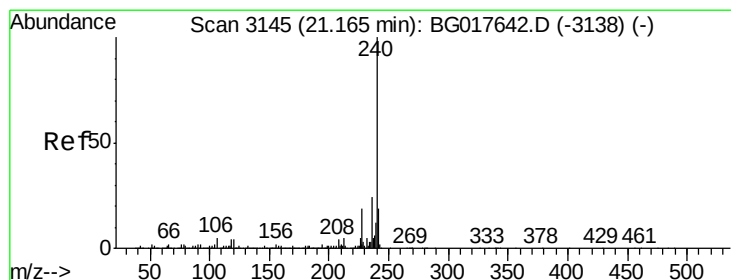
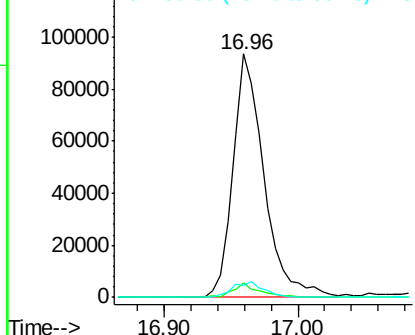



#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.16 min Scan# 3144
Delta R.T. -0.00 min
Lab File: BG017679.D
Acq: 13 Jun 2015 18:16

Tgt Ion:240 Resp: 224190
Ion Ratio Lower Upper
240 100
120 3.6 3.5 5.3
236 26.6 19.5 29.3

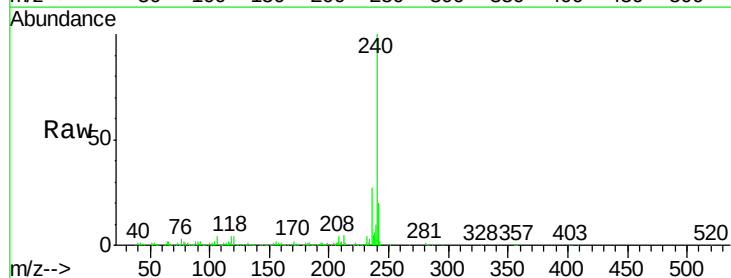

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

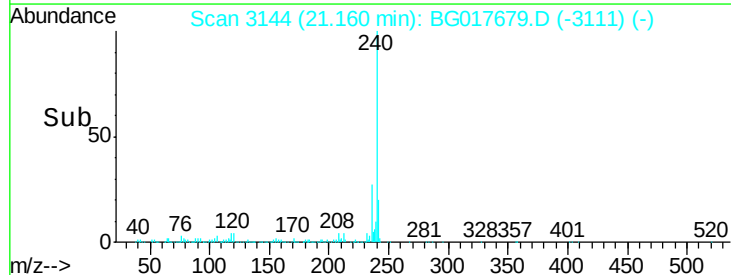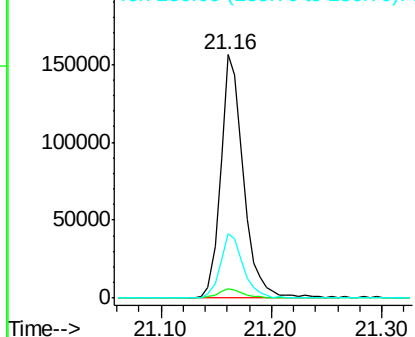

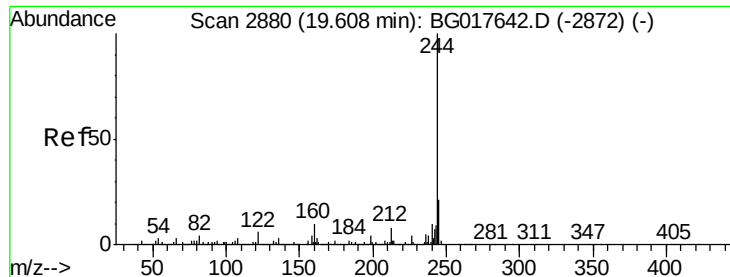

#78

Terphenyl-d14

Concen: 86.49 ng

RT: 19.61 min Scan# 2880

Delta R.T. 0.00 min

Lab File: BG017679.D

Acq: 13 Jun 2015 18:16

Instrument :

BNA_G

ClientSampleId :

TEC-C1


Tgt Ion:244 Resp: 929532

Ion Ratio Lower Upper




244 100

212 8.5 6.3 9.5

122 5.0 4.6 6.8

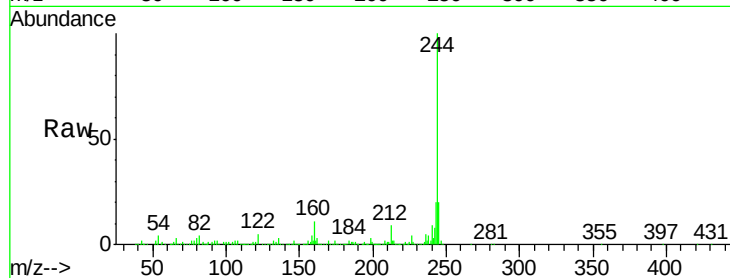

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

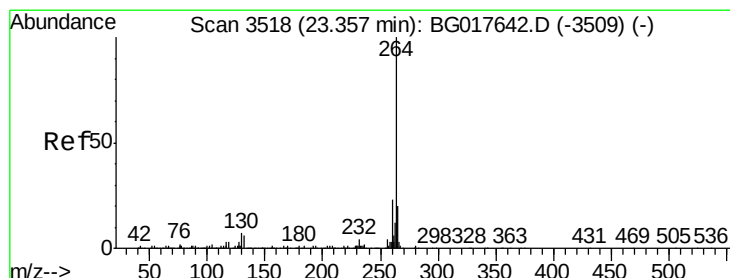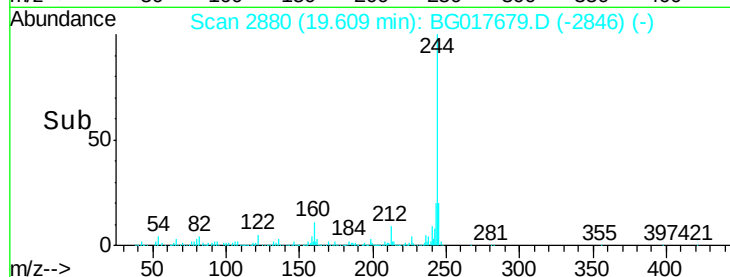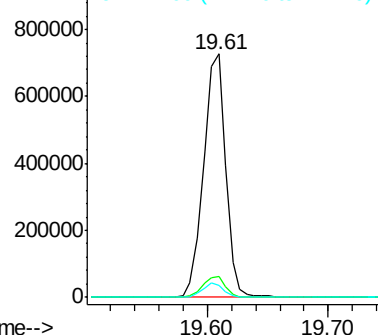

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.36 min Scan# 3519

Delta R.T. 0.01 min

Lab File: BG017679.D

Acq: 13 Jun 2015 18:16


Tgt Ion:264 Resp: 223943

Ion Ratio Lower Upper

264 100

260 21.7 18.3 27.5

265 22.0 16.2 24.2

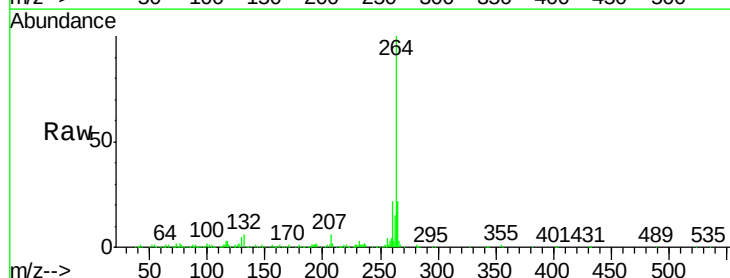

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

