

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061215\
 Data File : BG017648.D
 Acq On : 12 Jun 2015 21:53
 Operator : TP/IZ
 Sample : G2627-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-20

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.116	405	413	421	rBV	200281	301000	10.13%	3.051%
2	6.732	683	688	695	rBV	129040	192186	6.47%	1.948%
3	7.067	739	745	757	rVB	404073	628957	21.17%	6.375%
4	7.525	817	823	833	rVB	96648	139940	4.71%	1.419%
5	7.842	870	877	884	rBV	371524	579819	19.52%	5.877%
6	8.694	1012	1022	1032	rBV	267324	457631	15.40%	4.639%
7	10.322	1292	1299	1311	rBV2	90873	179046	6.03%	1.815%
8	12.819	1717	1724	1733	rBV	860402	1213057	40.83%	12.296%
9	14.206	1955	1960	1970	rVB2	167153	266095	8.96%	2.697%
10	15.710	2209	2216	2228	rBV	929175	1365044	45.95%	13.837%
11	16.961	2424	2429	2437	rBV	274344	386827	13.02%	3.921%
12	19.605	2874	2879	2886	rBV	2355296	2970877	100.00%	30.114%
13	21.162	3138	3144	3150	rBV	479569	621246	20.91%	6.297%
14	23.360	3512	3518	3527	rVB	309593	563587	18.97%	5.713%


Sum of corrected areas: 9865312

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061215\
Data File : BG017648.D
Acq On : 12 Jun 2015 21:53
Operator : TP/IZ
Sample : G2627-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-20

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

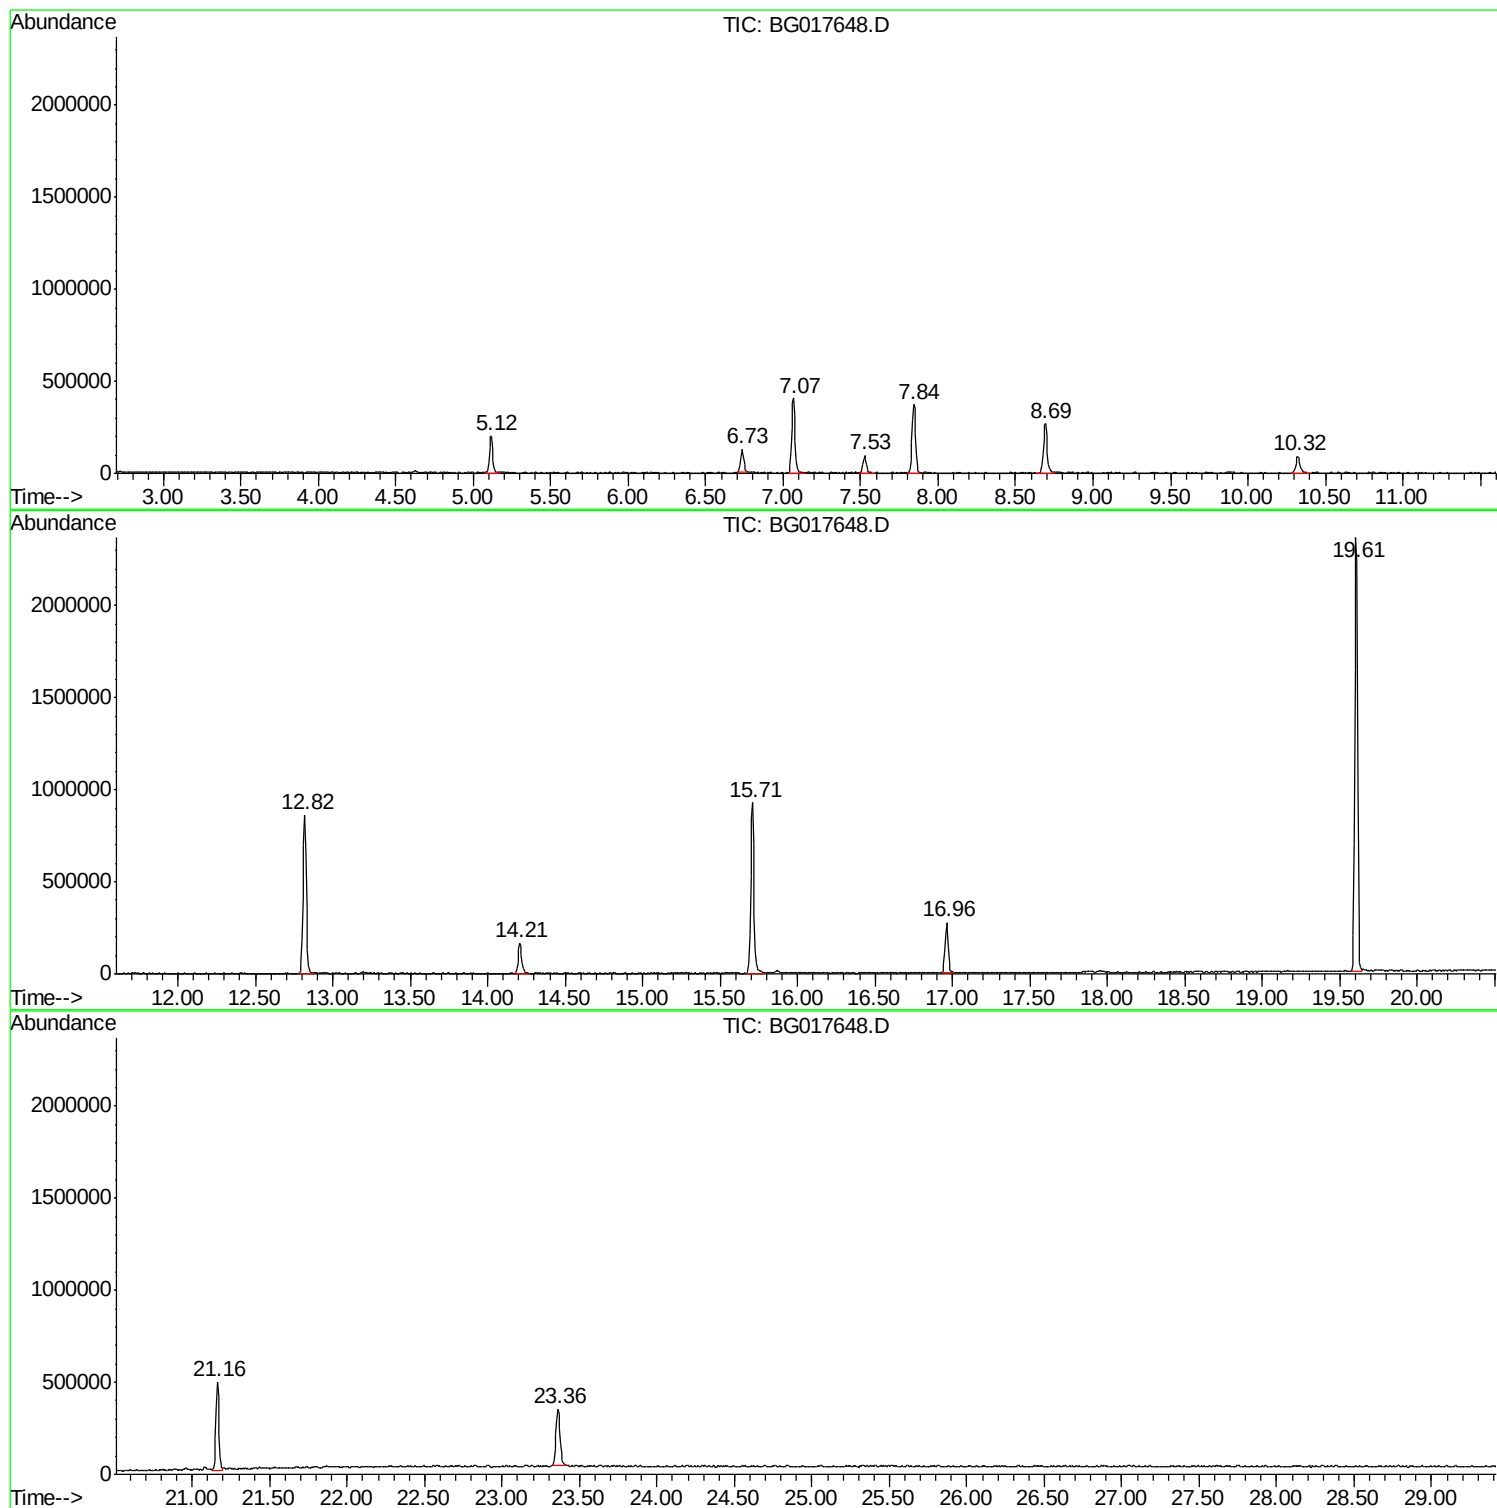

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061215\
Data File : BG017648.D
Acq On : 12 Jun 2015 21:53
Operator : TP/IZ
Sample : G2627-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-20










Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.07 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.07	89.89 ng	628957	1,4-Dichlorobenzene-d4	7.53

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	18
2		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	14
3		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	14
4		Xenon	132	Xe	007440-63-3	12
5		3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	10

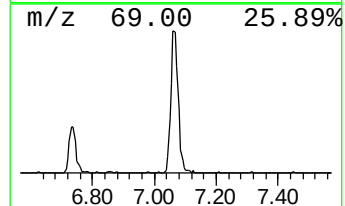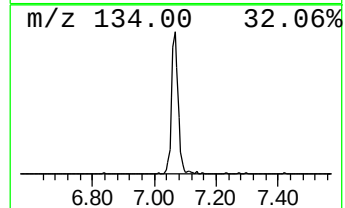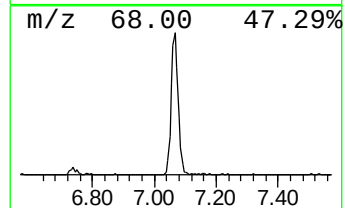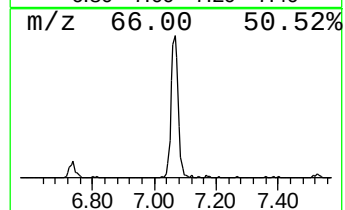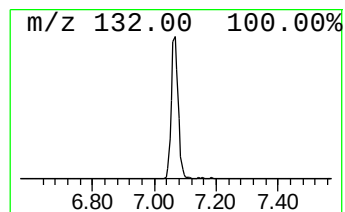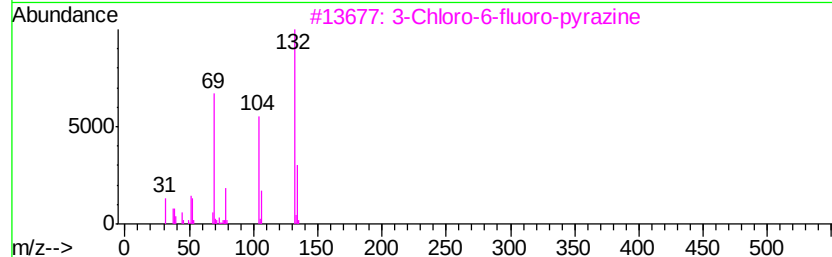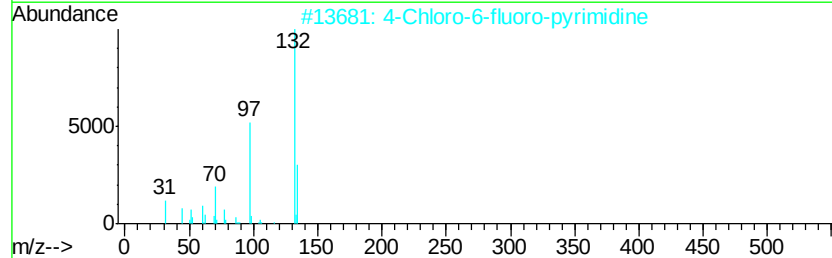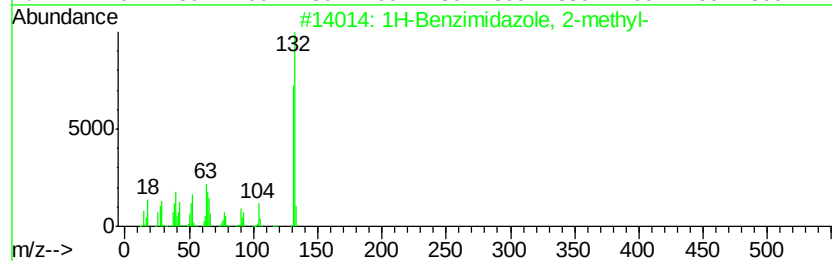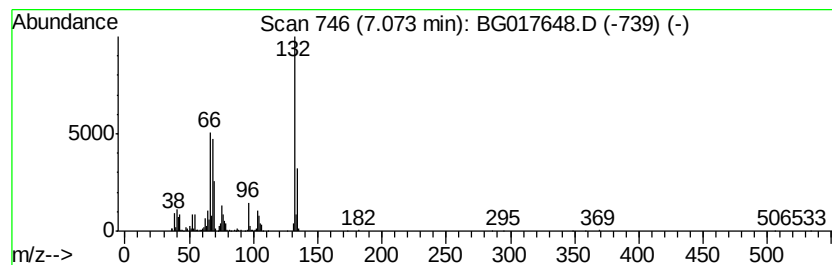

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061215\
Data File : BG017648.D
Acq On : 12 Jun 2015 21:53
Operator : TP/IZ
Sample : G2627-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-20

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.07	7.07	89.9	ng	628957	1	7.53	139940	20.0