

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061215\
 Data File : BG017676.D
 Acq On : 13 Jun 2015 16:31
 Operator : TP/IZ
 Sample : PB83969BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB83969BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.113	409	413	421	rVB	39459	63569	10.94%	2.079%
2	6.735	684	689	699	rBV2	30343	62110	10.69%	2.031%
3	7.064	740	745	753	rBV3	44645	71622	12.32%	2.342%
4	7.522	818	823	830	rBV2	92279	134376	23.12%	4.394%
5	7.845	871	878	885	rBV	37773	62008	10.67%	2.028%
6	8.697	1018	1023	1030	rBV4	17243	32817	5.65%	1.073%
7	10.325	1291	1300	1311	rBV	77998	165671	28.50%	5.417%
8	12.822	1720	1725	1730	rBV	55528	88333	15.20%	2.888%
9	14.209	1953	1961	1970	rBV3	143993	266331	45.82%	8.709%
10	15.713	2212	2217	2227	rBV8	39416	80515	13.85%	2.633%
11	16.964	2423	2430	2442	rBV	229620	400096	68.84%	13.082%
12	19.608	2875	2880	2891	rBV	182694	266487	45.85%	8.714%
13	20.959	3107	3110	3113	rBV4	9786	13402	2.31%	0.438%
14	21.048	3122	3125	3128	rBV5	4390	6836	1.18%	0.224%
15	21.165	3140	3145	3159	rVV	408435	581206	100.00%	19.004%
16	21.430	3186	3190	3193	rBV6	8445	8564	1.47%	0.280%
17	21.588	3213	3217	3218	rBV3	7130	6036	1.04%	0.197%
18	21.794	3248	3252	3253	rBV4	7925	11007	1.89%	0.360%
19	21.923	3271	3274	3275	rBV3	8797	8442	1.45%	0.276%
20	22.270	3329	3333	3336	rBV5	8246	13295	2.29%	0.435%
21	22.693	3402	3405	3408	rBV4	5453	6660	1.15%	0.218%
22	22.857	3431	3433	3434	rBV2	8434	7502	1.29%	0.245%
23	22.957	3448	3450	3453	rBV4	7513	7163	1.23%	0.234%
24	23.180	3486	3488	3491	rVB3	6640	6037	1.04%	0.197%
25	23.363	3512	3519	3528	rBV2	269731	545891	93.92%	17.850%
26	23.492	3539	3541	3542	rBV2	9204	6132	1.06%	0.201%
27	23.639	3564	3566	3567	rBV2	7911	6275	1.08%	0.205%
28	23.774	3587	3589	3591	rBV3	5464	7236	1.24%	0.237%
29	24.021	3629	3631	3635	rVB5	8127	6314	1.09%	0.206%
30	24.403	3694	3696	3699	rBV3	7519	9055	1.56%	0.296%
31	24.831	3767	3769	3773	rBV5	5874	7898	1.36%	0.258%
32	24.949	3787	3789	3794	rVB6	7262	9188	1.58%	0.300%
33	25.196	3830	3831	3834	rBV2	8411	6644	1.14%	0.217%
34	25.260	3841	3842	3847	rBV5	8026	10238	1.76%	0.335%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061215\
Data File : BG017676.D
Acq On : 13 Jun 2015 16:31
Operator : TP/IZ
Sample : PB83969BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB83969BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061215.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	25.343	3853	3856	3858	rVB4	7797	8445	1.45%	0.276%
36	25.366	3858	3860	3863	rBV3	7034	7994	1.38%	0.261%
37	26.206	4000	4003	4005	rBV4	10377	11456	1.97%	0.375%
38	26.294	4015	4018	4020	rBV4	8176	10207	1.76%	0.334%
39	26.383	4031	4033	4037	rBV5	6448	8001	1.38%	0.262%
40	27.587	4234	4238	4240	rBV4	6779	9024	1.55%	0.295%
41	27.987	4303	4306	4309	rBV5	8821	12109	2.08%	0.396%
42	28.227	4345	4347	4350	rBV4	6129	6084	1.05%	0.199%


Sum of corrected areas: 3058276

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061215\
Data File : BG017676.D
Acq On : 13 Jun 2015 16:31
Operator : TP/IZ
Sample : PB83969BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB83969BL

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

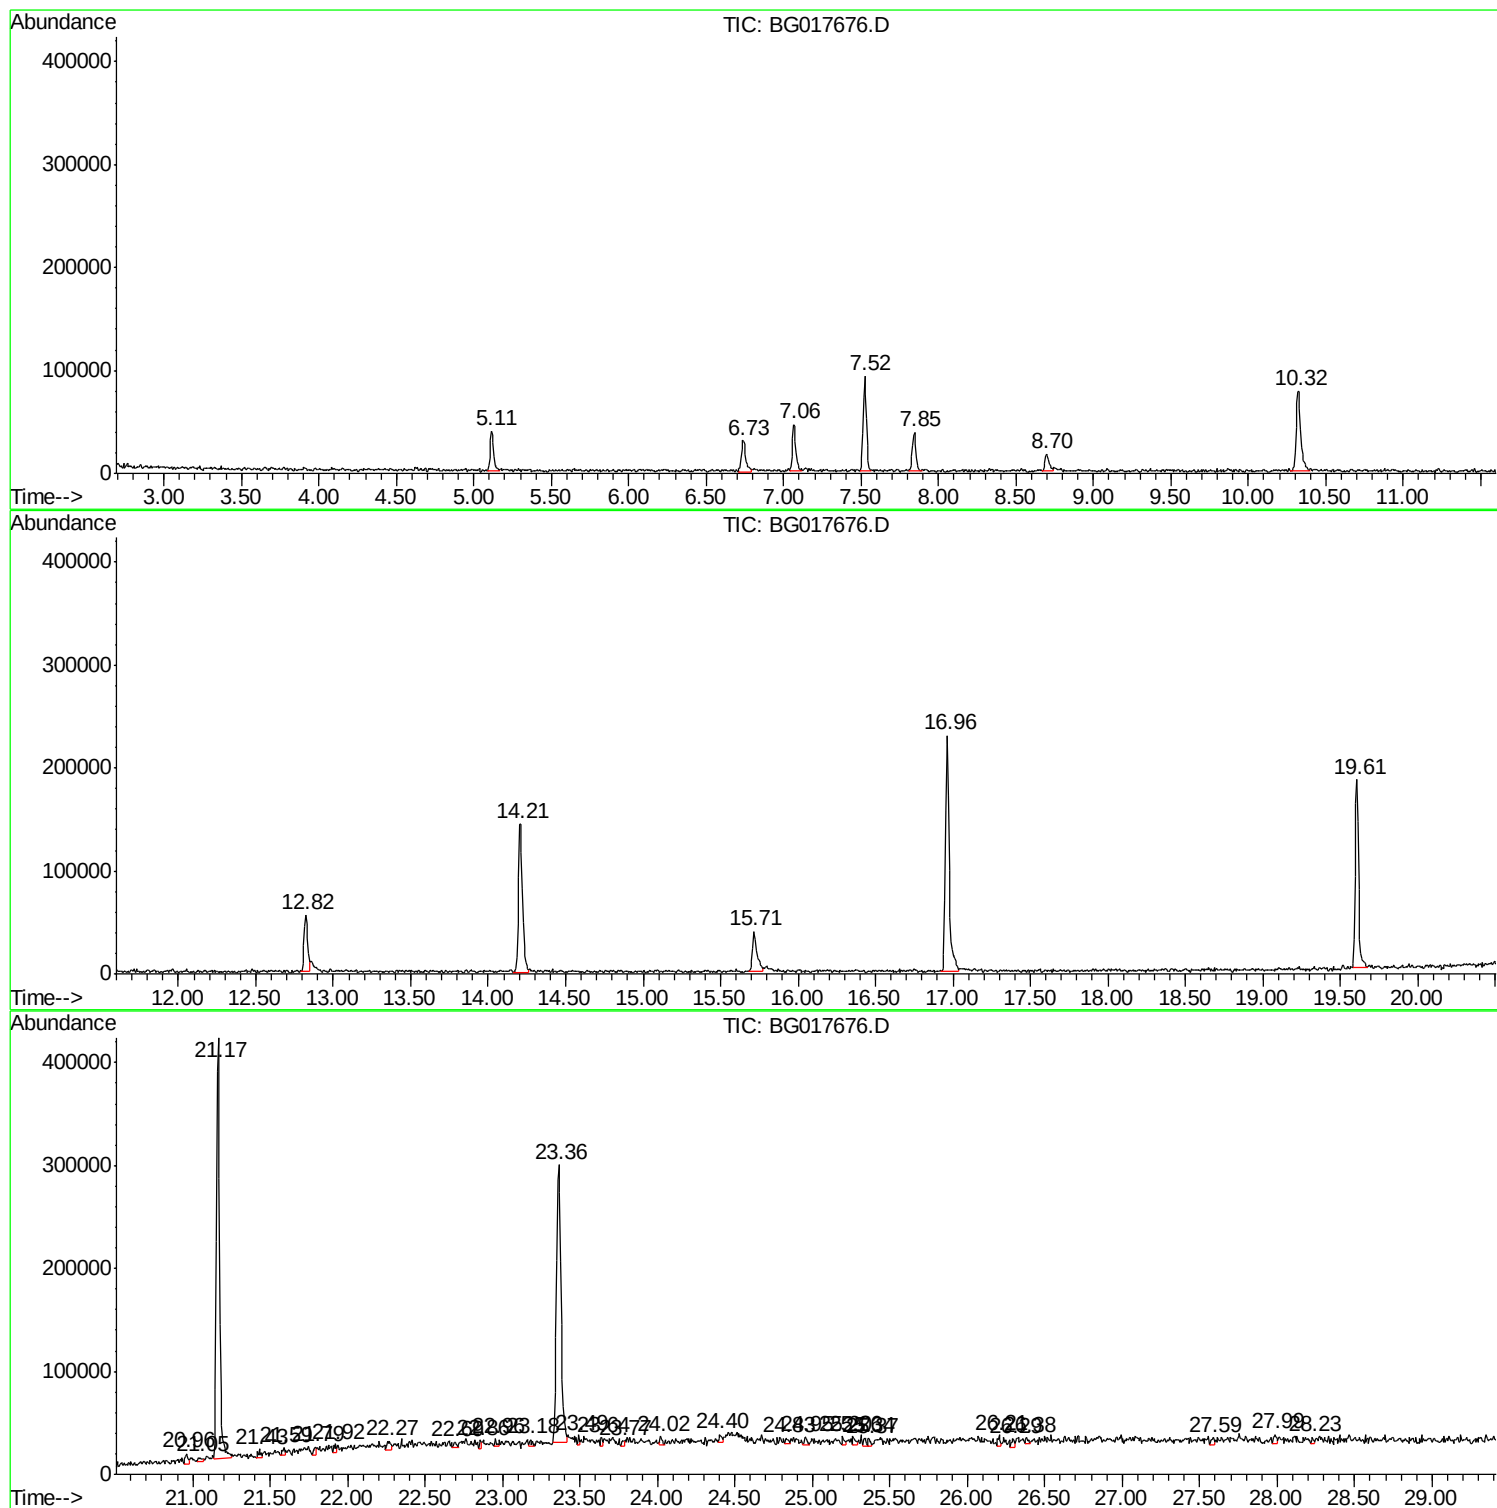

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061215\
Data File : BG017676.D
Acq On : 13 Jun 2015 16:31
Operator : TP/IZ
Sample : PB83969BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampled :
PB83969BL










Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.06 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.06	10.66 ng	71622	1,4-Dichlorobenzene-d4	7.52

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Hexenedinitrile	106	C6H6N2	001119-85-3	27
2		3-Oxabicyclo[3.2.0]hept-6-ene-2,...	138	C7H6O3	064197-88-2	27
3		1,3-Cyclopentadiene	66	C5H6	000542-92-7	25
4		1-Penten-3-yne	66	C5H6	000646-05-9	12
5		3-Penten-1-yne, (E)-	66	C5H6	002004-69-5	12

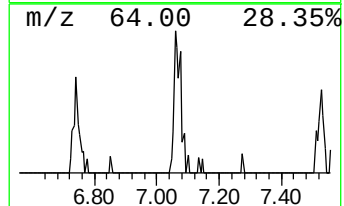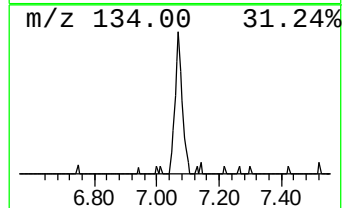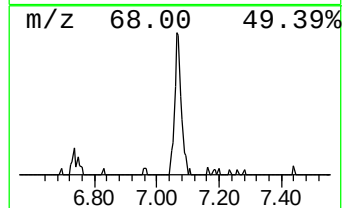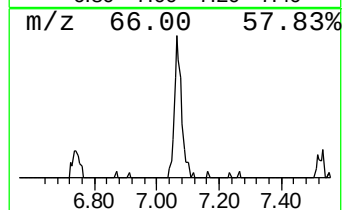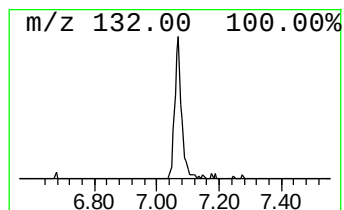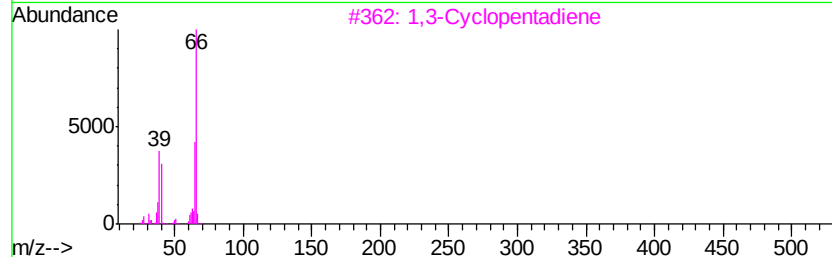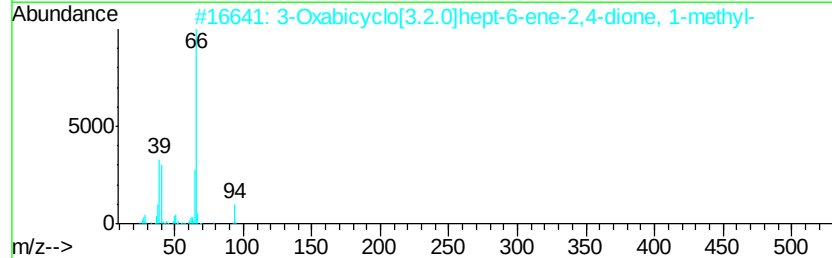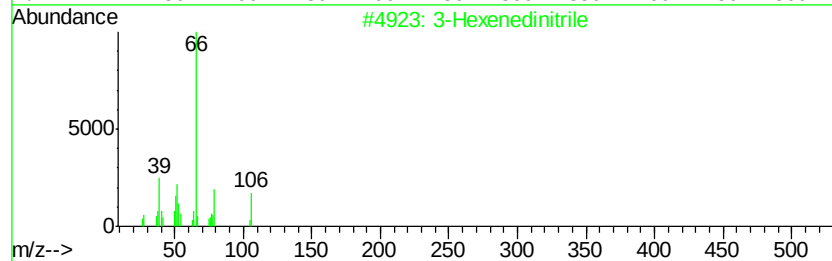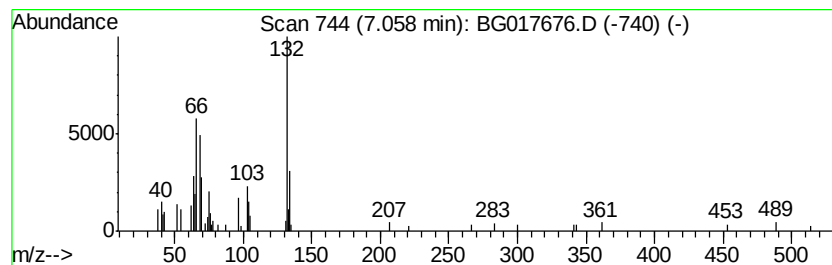

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061215\
Data File : BG017676.D
Acq On : 13 Jun 2015 16:31
Operator : TP/IZ
Sample : PB83969BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB83969BL

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.06	7.06	10.7	ng	71622	1	7.52	134376	20.0