


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061215\
 Data File : BG017637.D
 Acq On : 12 Jun 2015 14:18
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jun 13 02:22:44 2015

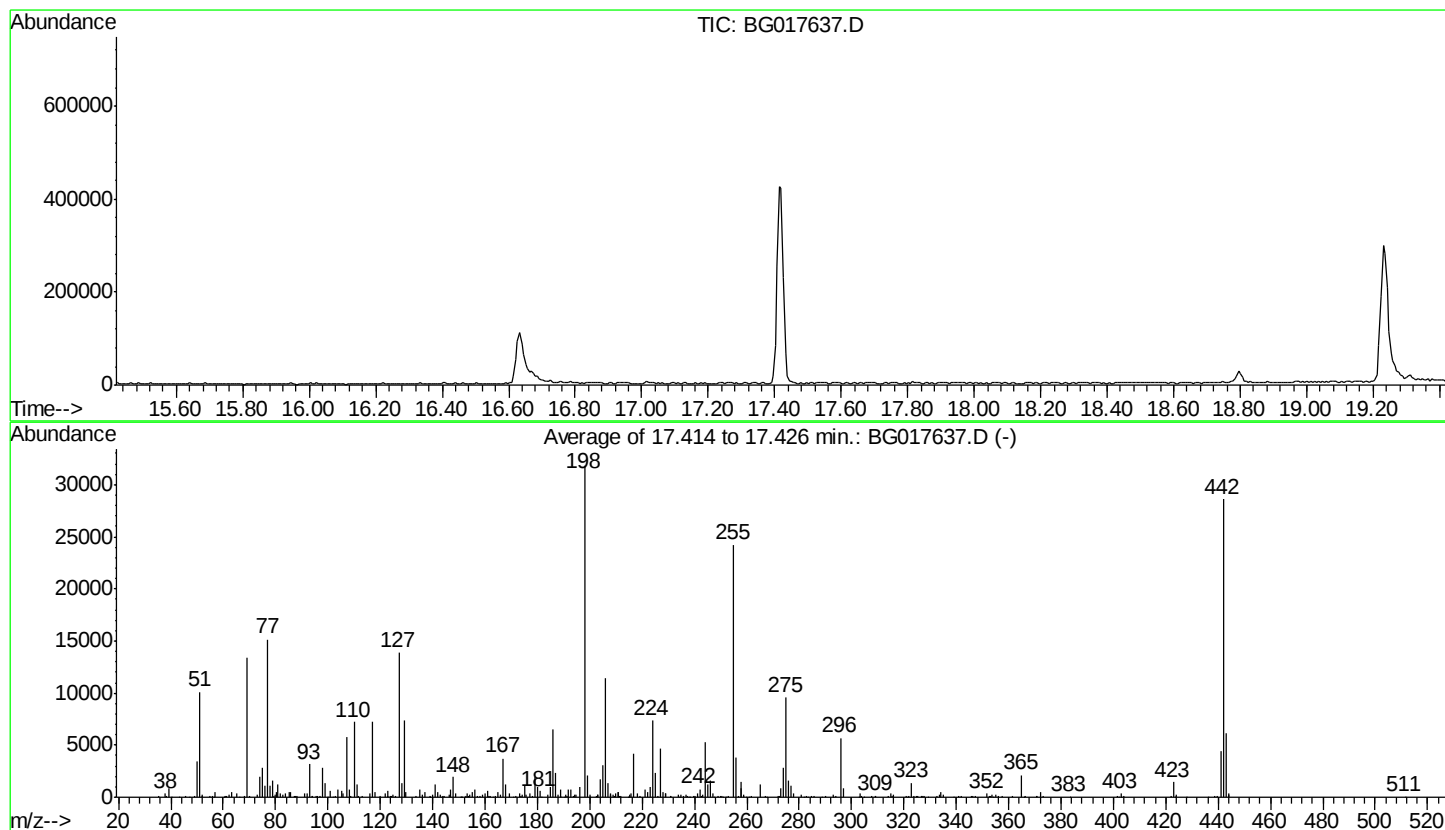

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.7	10096	PASS
68	69	0.00	2	1.4	185	PASS
69	198	0.00	100	42.0	13359	PASS
70	69	0.00	2	1.1	147	PASS
127	198	10	80	43.4	13830	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	31832	PASS
199	198	5	9	6.6	2116	PASS
275	198	10	60	30.0	9548	PASS
365	198	1	100	6.6	2099	PASS
441	442	0.01	24	15.4	4397	PASS
442	198	50	100	89.8	28584	PASS
443	442	15	24	21.7	6198	PASS