


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061215\
 Data File : BG017654.D
 Acq On : 13 Jun 2015 1:24
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jun 13 02:22:44 2015

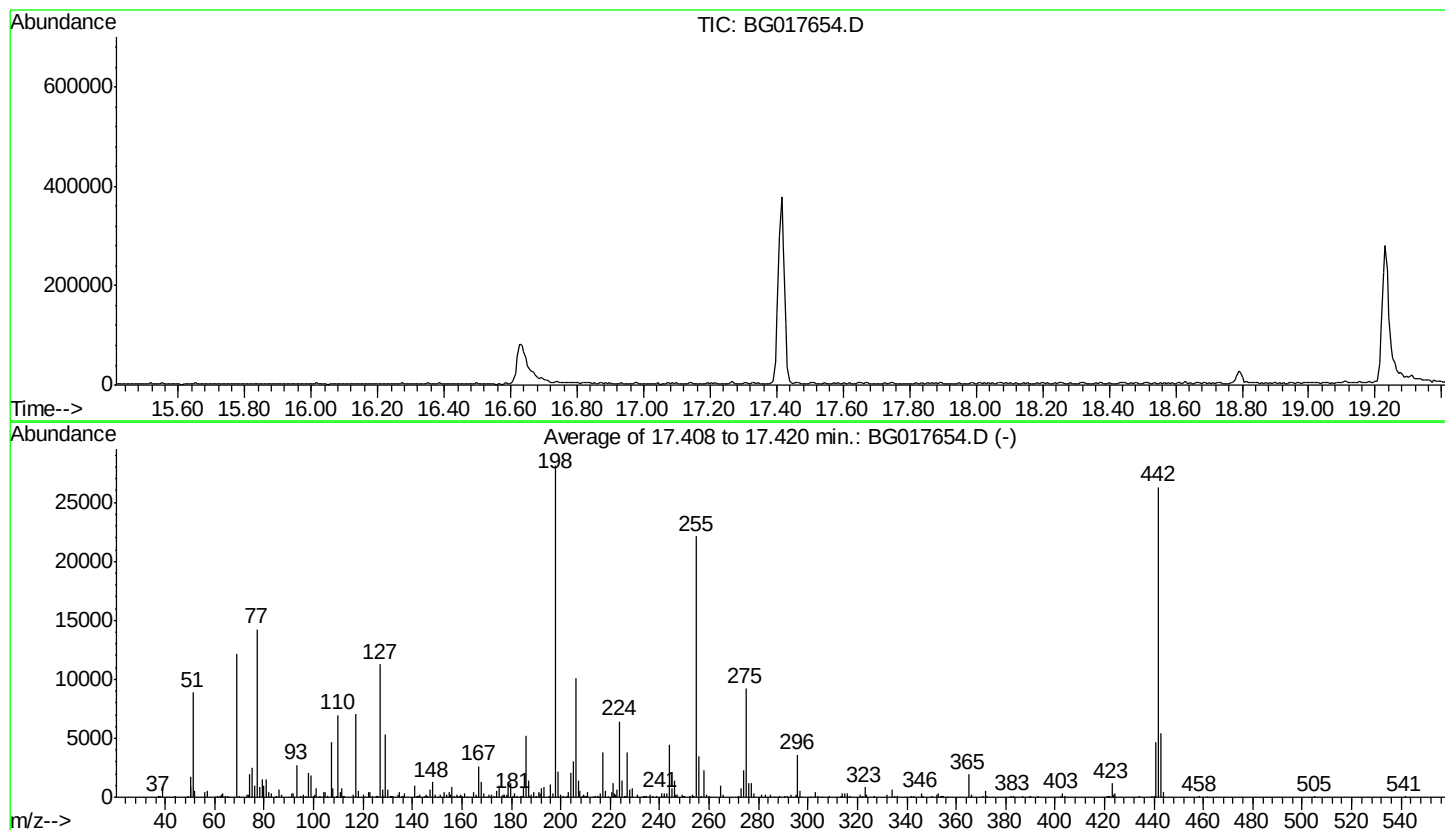

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.6	8893	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.4	12200	PASS
70	69	0.00	2	0.5	64	PASS
127	198	10	80	40.1	11265	PASS
197	198	0.00	2	1.1	297	PASS
198	198	100	100	100.0	28114	PASS
199	198	5	9	7.8	2186	PASS
275	198	10	60	32.8	9220	PASS
365	198	1	100	6.9	1942	PASS
441	442	0.01	24	17.9	4700	PASS
442	198	50	100	93.6	26317	PASS
443	442	15	24	20.5	5401	PASS