


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061215\
Data File : BG017674.D
Acq On : 13 Jun 2015 14:46
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061215.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jun 13 02:22:44 2015

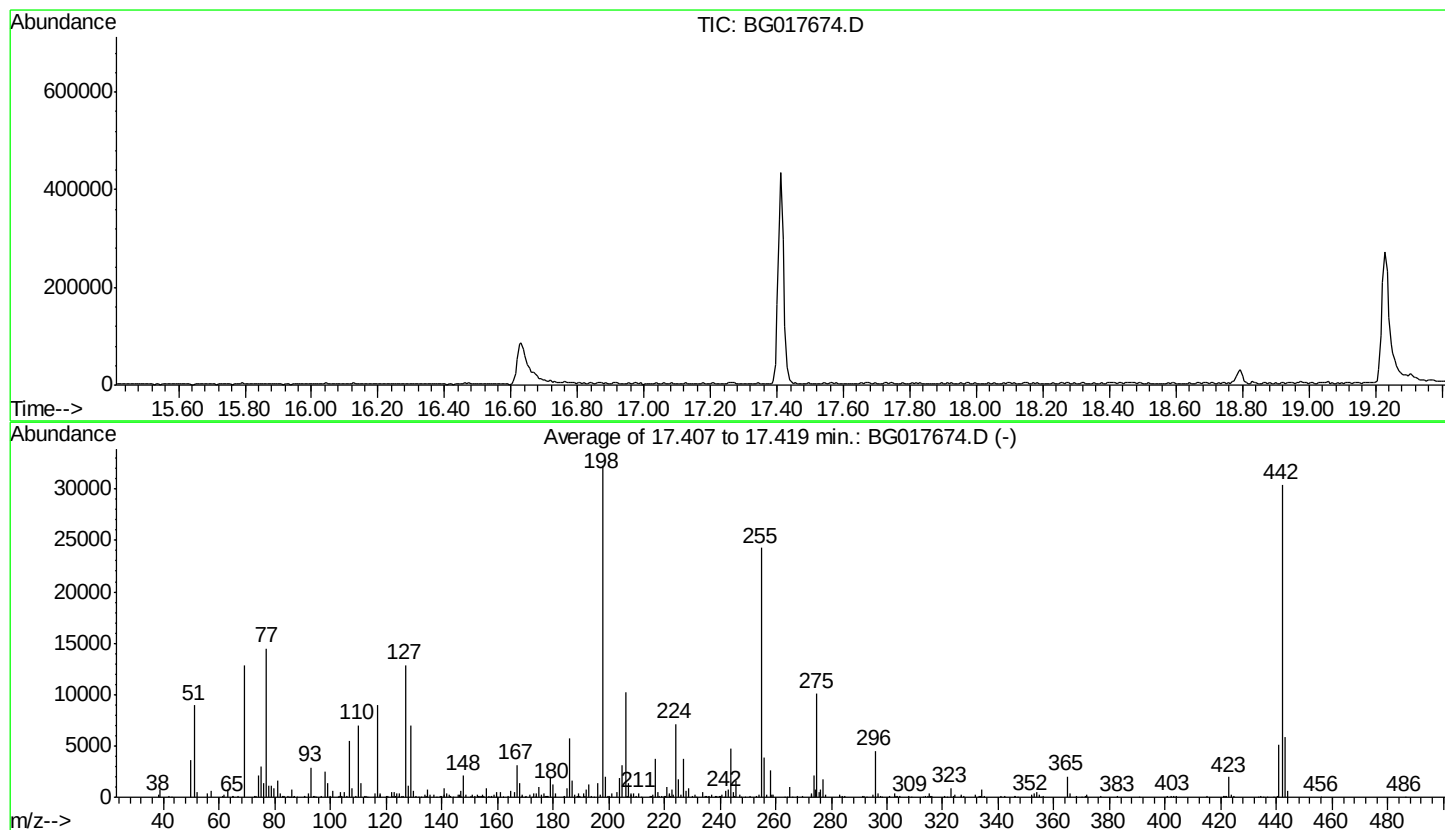

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.7	8947	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.9	12865	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.9	12876	PASS
197	198	0.00	2	0.7	223	PASS
198	198	100	100	100.0	32282	PASS
199	198	5	9	6.0	1944	PASS
275	198	10	60	31.3	10093	PASS
365	198	1	100	6.4	2057	PASS
441	442	0.01	24	16.9	5146	PASS
442	198	50	100	94.3	30442	PASS
443	442	15	24	19.4	5904	PASS