

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061217\
 Data File : BG027385.D
 Acq On : 12 Jun 2017 21:28
 Operator : SJ/MA
 Sample : I3624-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jun 13 03:53:47 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 05 16:00:35 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.54	152	49585	20.00	ng	-0.04
21) Naphthalene-d8	11.36	136	215568	20.00	ng	-0.04
38) Acenaphthene-d10	15.12	164	107513	20.00	ng	-0.04
63) Phenanthrene-d10	17.87	188	319372	20.00	ng	-0.04
75) Chrysene-d12	22.25	240	341098	20.00	ng	-0.06
86) Perylene-d12	25.92	264	78376	20.00	ng	-0.11
System Monitoring Compounds						
5) 2-Fluorophenol	6.13	112	437172	134.54	ng	-0.02
7) Phenol-d6	7.68	99	546071	114.49	ng	-0.02
23) Nitrobenzene-d5	9.71	82	356942	104.13	ng	-0.04
41) 2,4,6-Tribromophenol	16.60	330	262974	185.75	ng	-0.04
44) 2-Fluorobiphenyl	13.75	172	786587	102.35	ng	-0.04
78) Terphenyl-d14	20.45	244	1531798	114.56	ng	-0.05


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061217\
Data File : BG027385.D
Acq On : 12 Jun 2017 21:28
Operator : SJ/MA
Sample : I3624-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jun 13 03:53:47 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:00:35 2017
Response via : Initial Calibration

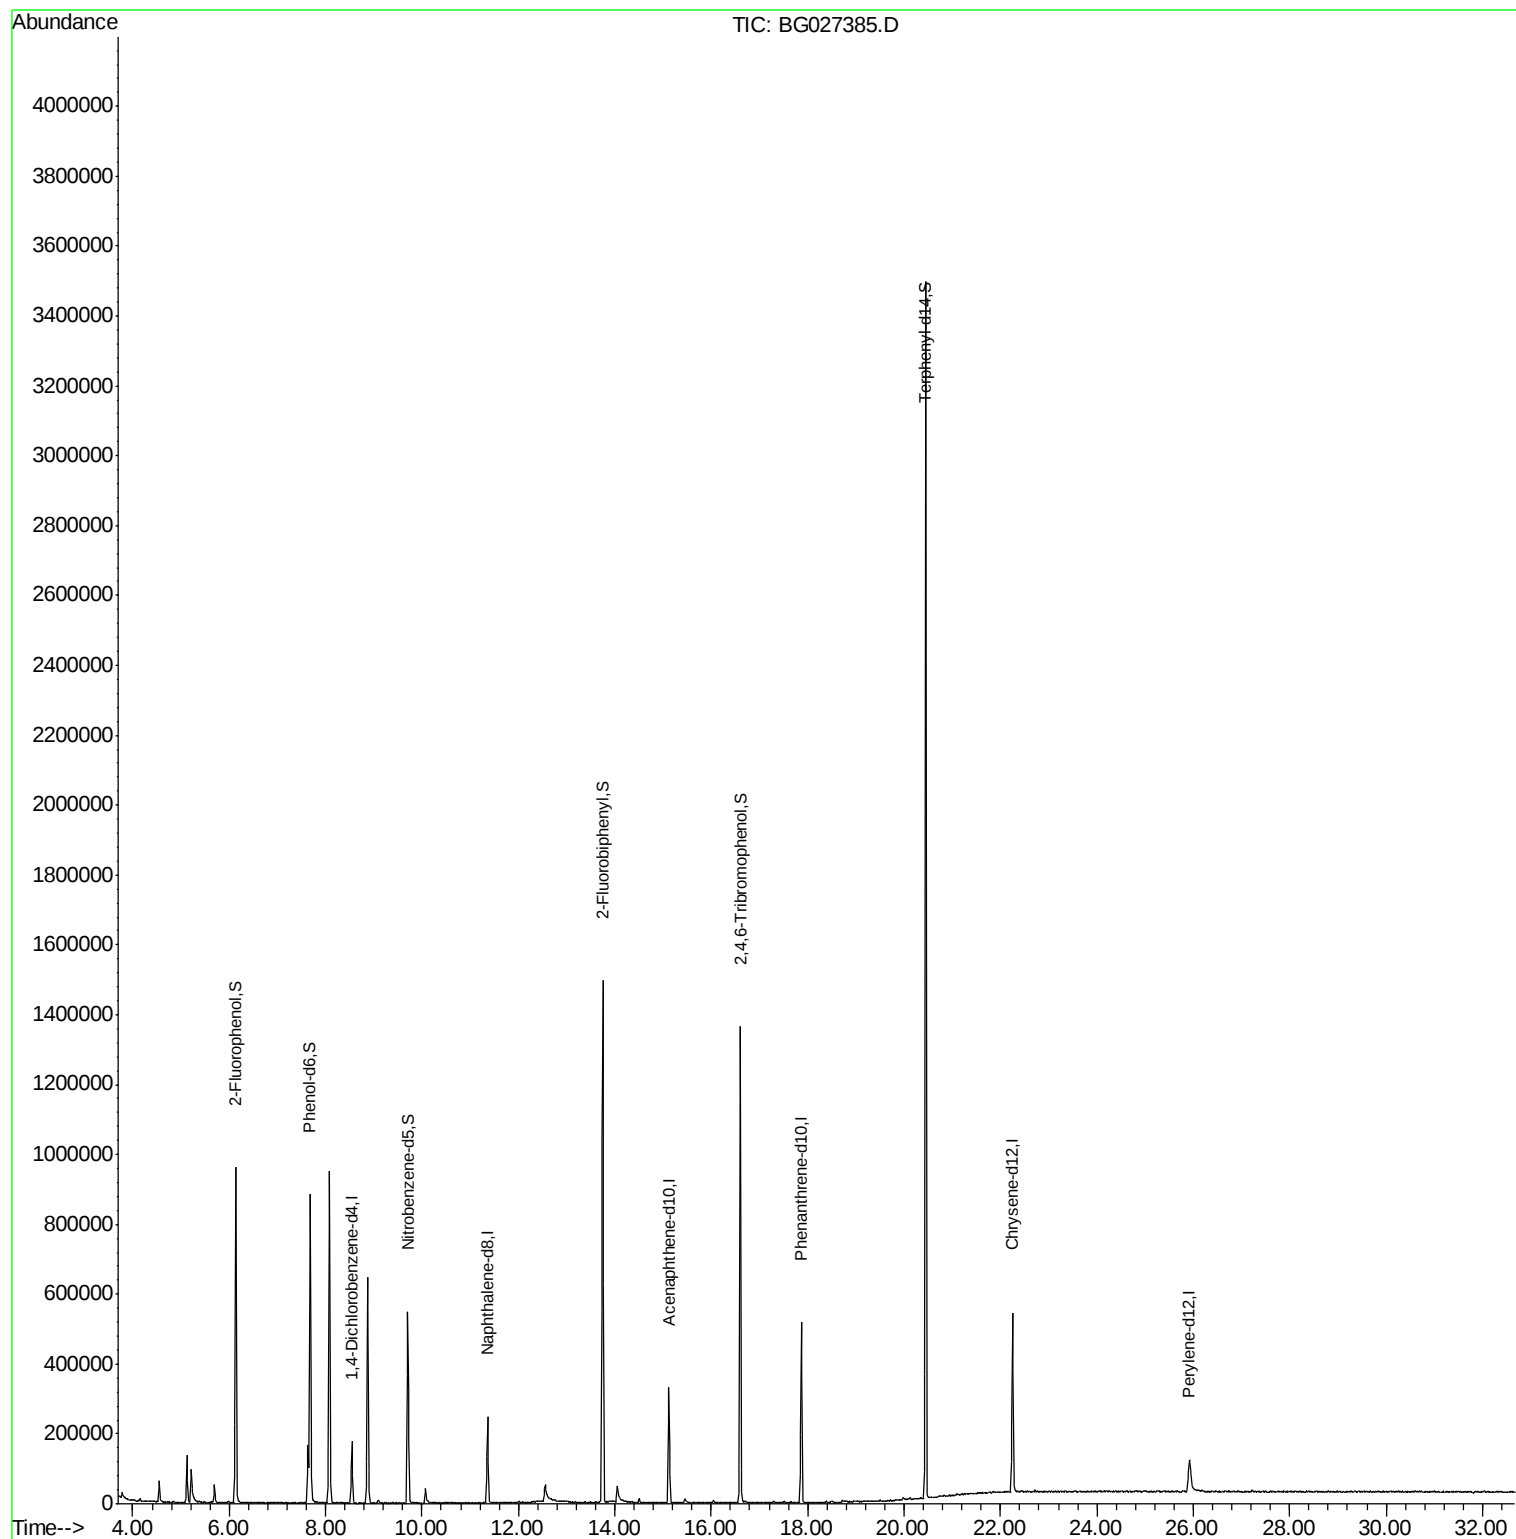



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.54 min Scan# 826

Delta R.T. -0.04 min

Lab File: BG027385.D

Acq: 12 Jun 2017 21:28

Instrument :

BNA_G

ClientSampleId :


Tot Ion:152 Resp: 49585

Ion Ratio Lower Upper

152 100

150 156.3 114.0 171.0




115 68.5 48.1 72.1



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

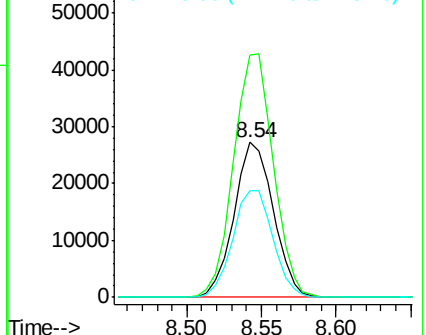

#5

2-Fluorophenol

Concen: 134.54 ng

RT: 6.13 min Scan# 416

Delta R.T. -0.02 min

Lab File: BG027385.D

Acq: 12 Jun 2017 21:28


Tgt Ion:112 Resp: 437172

Ion Ratio Lower Upper

112 100

64 72.4 61.8 92.6



63 35.6 37.2 55.8#




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

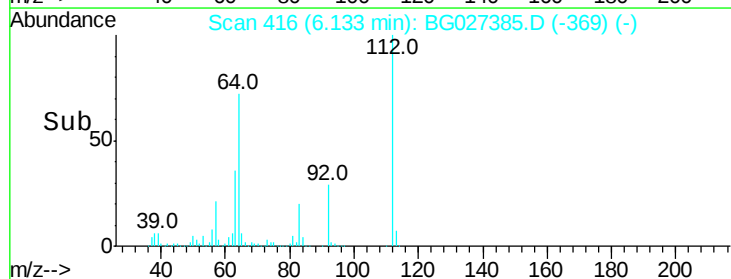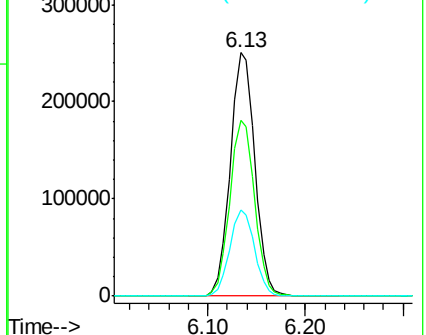

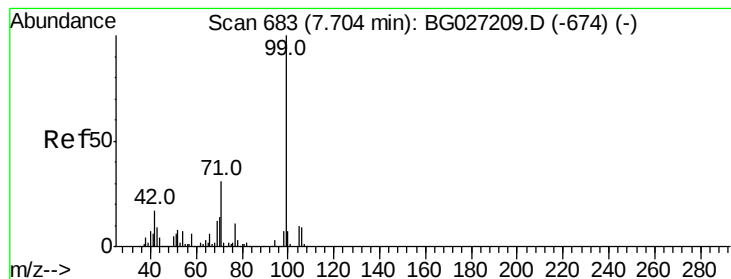

#7

Phenol-d6

Concen: 114.49 ng

RT: 7.68 min Scan# 679

Delta R.T. -0.02 min

Lab File: BG027385.D

Acq: 12 Jun 2017 21:28

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 546071

Ion Ratio Lower Upper




99 100

42 18.2 20.5 30.7#

71 33.3 37.6 56.4#



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

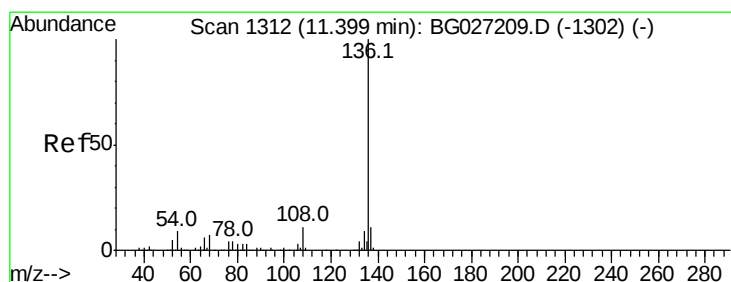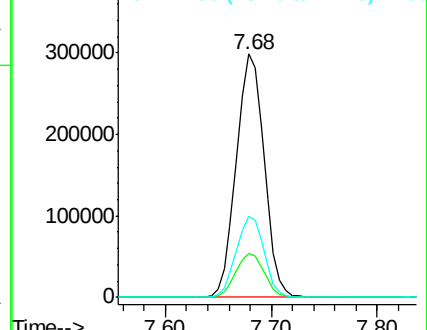

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 11.36 min Scan# 1305

Delta R.T. -0.04 min

Lab File: BG027385.D

Acq: 12 Jun 2017 21:28

Tgt Ion: 136 Resp: 215568


Ion Ratio Lower Upper

136 100



137 11.1 8.9 13.3


54 11.8 9.3 13.9

68 8.7 5.1 7.7#

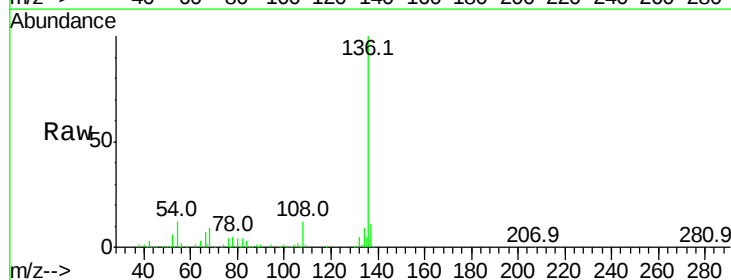

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




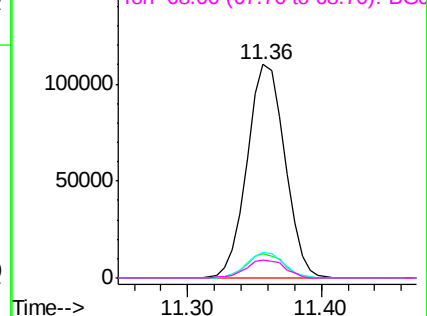




#23
Nitrobenzene-d5
Concen: 104.13 ng
RT: 9.71 min Scan# 1024
Delta R.T. -0.04 min
Lab File: BG027385.D
Acq: 12 Jun 2017 21:28




Instrument :
BNA_G
ClientSampled :


Tot Ion	82	Resp	356942
Ion	Ratio	Lower	Upper
82	100		
128	39.2	26.4	39.6
54	52.0	49.4	74.2

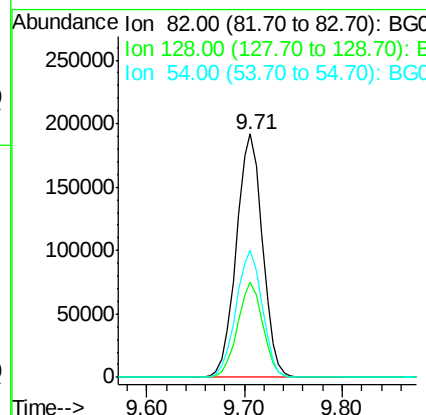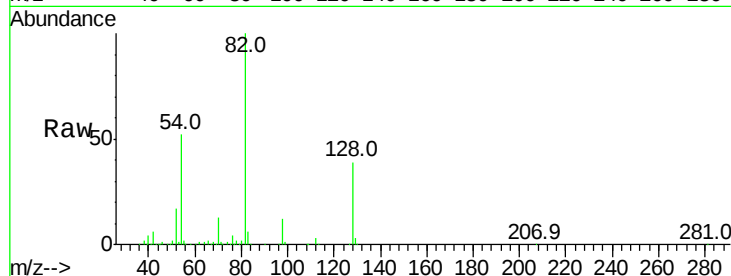

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 15.12 min Scan# 1946
Delta R.T. -0.04 min
Lab File: BG027385.D
Acq: 12 Jun 2017 21:28

Tgt Ion	164	Resp	107513
Ion	Ratio	Lower	Upper
164	100		
162	105.6	85.1	127.7
160	45.7	34.7	52.1

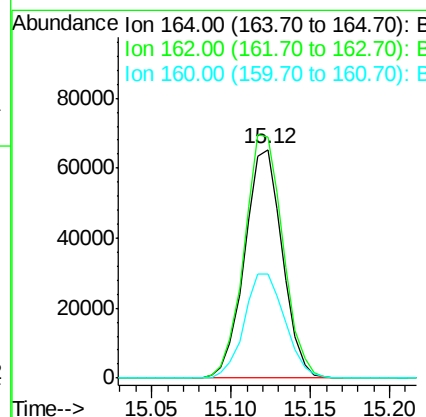


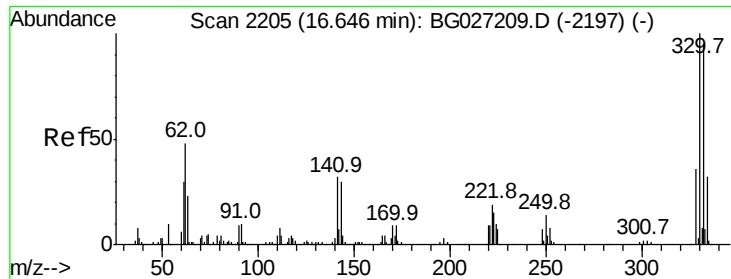




#41
 2,4,6-Tribromophenol
 Concen: 185.75 ng
 RT: 16.60 min Scan# 2198
 Delta R.T. -0.04 min
 Lab File: BG027385.D
 Acq: 12 Jun 2017 21:28

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.2	77.3	115.9
141	33.5	32.1	48.1




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


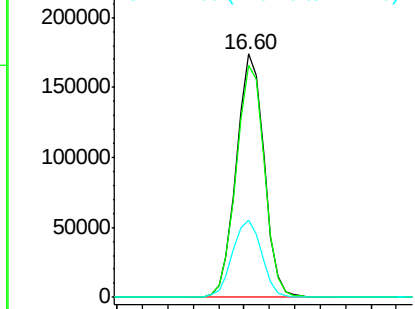



#44
 2-Fluorobiphenyl
 Concen: 102.35 ng
 RT: 13.75 min Scan# 1712
 Delta R.T. -0.04 min
 Lab File: BG027385.D
 Acq: 12 Jun 2017 21:28

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.7	32.2	48.2
170	24.7	21.8	32.6



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

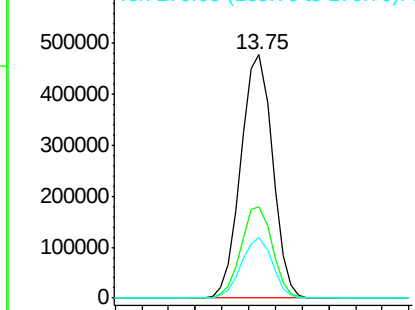







#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.87 min Scan# 2414
Delta R.T. -0.04 min
Lab File: BG027385.D
Acq: 12 Jun 2017 21:28

Instrument :
BNA_G
ClientSampled :

Tot Ion:188 Resp: 319372
Ion Ratio Lower Upper
188 100
94 11.5 5.8 8.8#
80 13.6 7.5 11.3#

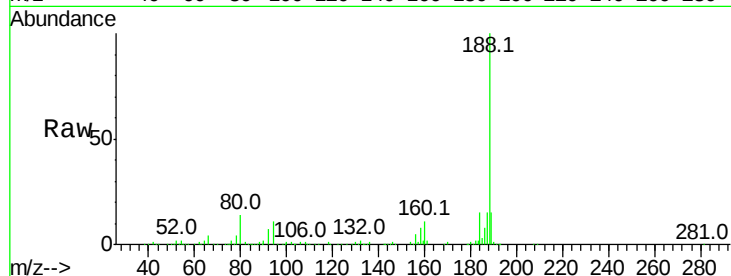


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

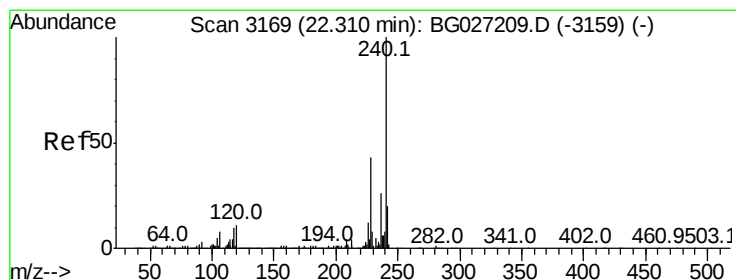
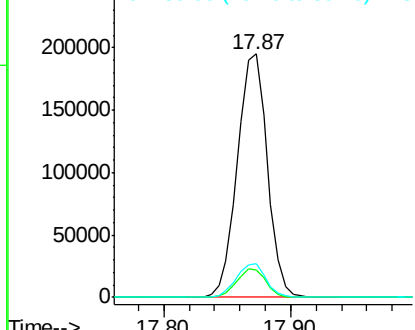



#75
Chrysene-d12
Concen: 20.00 ng
RT: 22.25 min Scan# 3159
Delta R.T. -0.06 min
Lab File: BG027385.D
Acq: 12 Jun 2017 21:28

Tgt Ion:240 Resp: 341098
Ion Ratio Lower Upper
240 100
120 11.6 5.7 8.5#
236 26.8 22.2 33.4



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

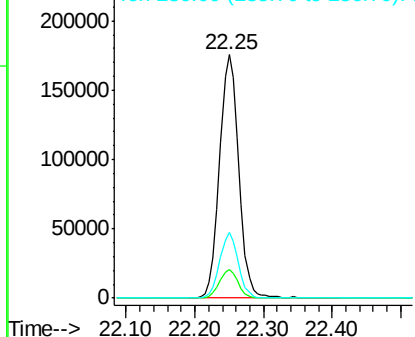

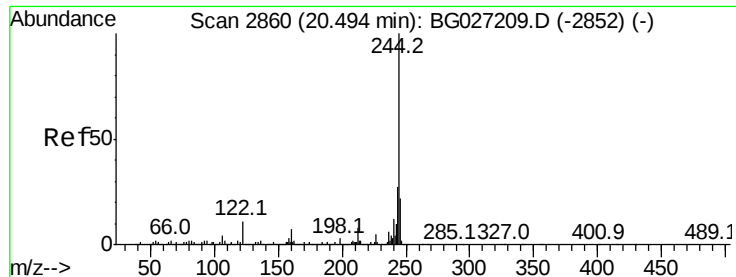

#78

Terphenyl-d14

Concen: 114.56 ng

RT: 20.45 min Scan# 2852

Delta R.T. -0.05 min

Lab File: BG027385.D

Acq: 12 Jun 2017 21:28

Instrument :

BNA_G

ClientSampled :


Tot Ion:244 Resp: 1531798

Ion Ratio Lower Upper

244 100

212 8.4 10.0 15.0#




122 12.4 8.6 12.8

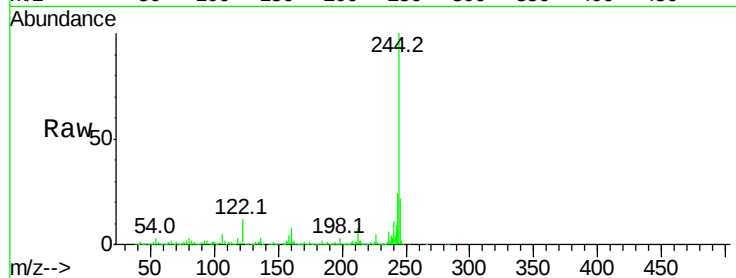

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

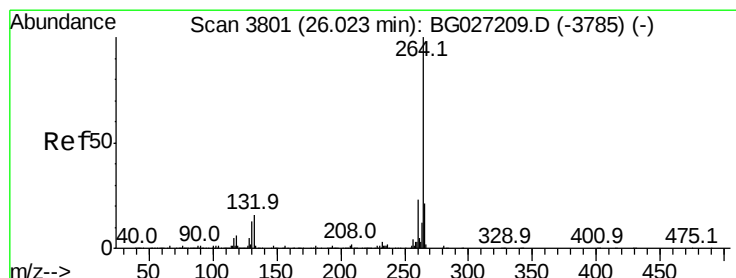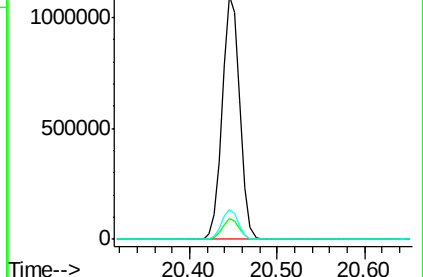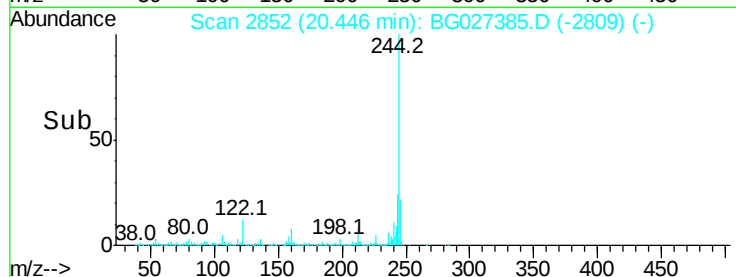

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.92 min Scan# 3783

Delta R.T. -0.11 min

Lab File: BG027385.D

Acq: 12 Jun 2017 21:28


Tgt Ion:264 Resp: 78376

Ion Ratio Lower Upper

264 100

260 25.2 21.8 32.8

265 23.9 18.2 27.4

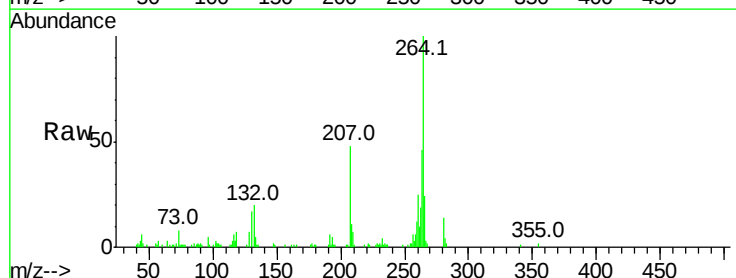

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

