
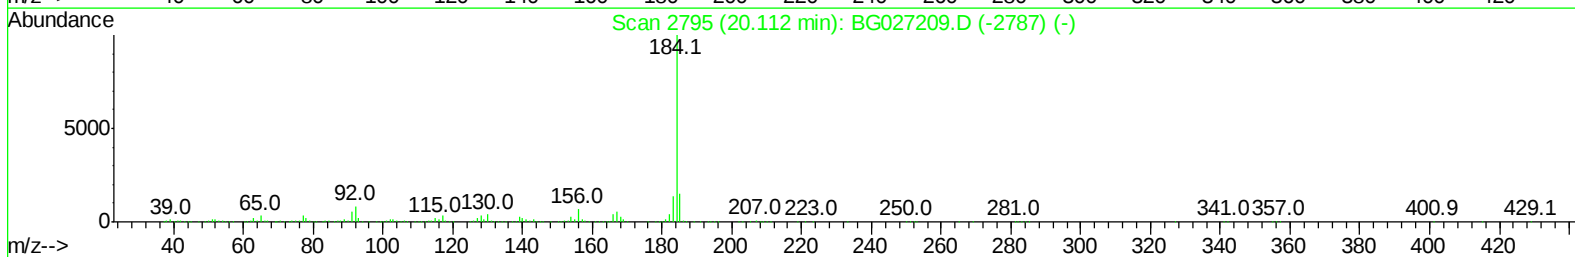
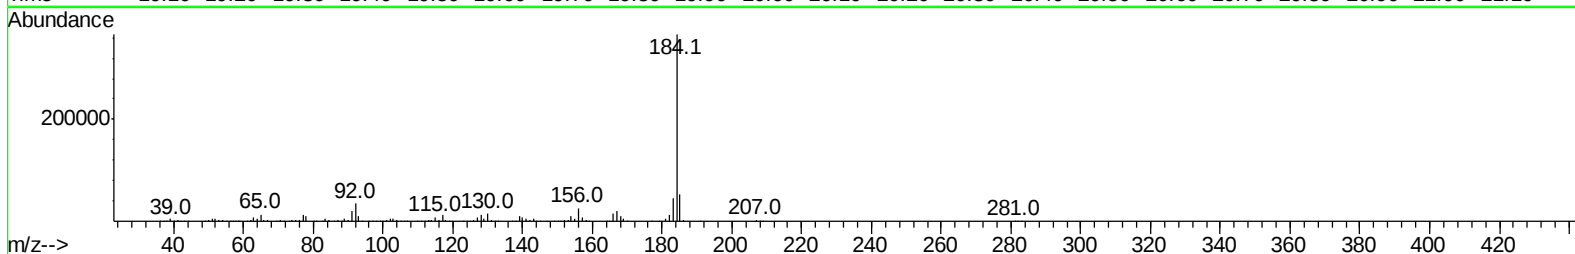


Data Path : Z:\HPCHEM1\BNA G\DATA\BG061217\
Data File : BG027377.D
Acq On : 12 Jun 2017 16:11
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 04:41:41 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:00:35 2017
Response via : Initial Calibration

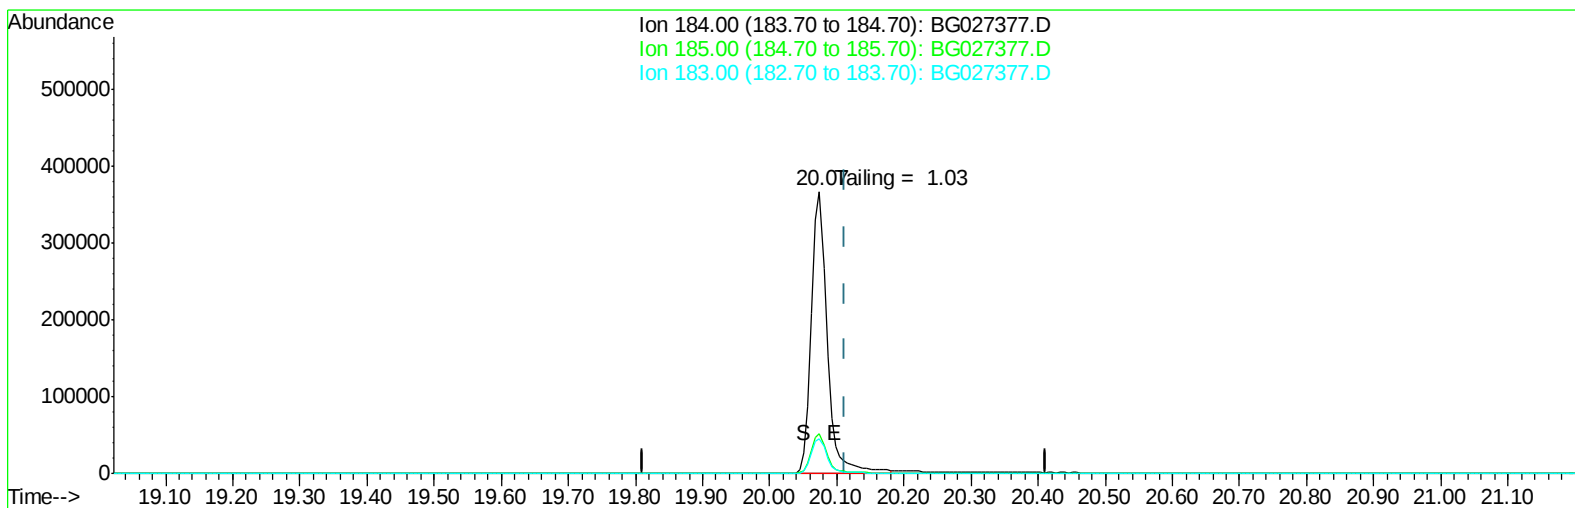

TIC: BG027377.D

(76) Benzidine




20.074min (-0.038) 5223.87ng

response 594355

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.31
183.00	13.80	12.49
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061217\
Data File : BG027377.D
Acq On : 12 Jun 2017 16:11
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 04:41:41 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:00:35 2017
Response via : Initial Calibration

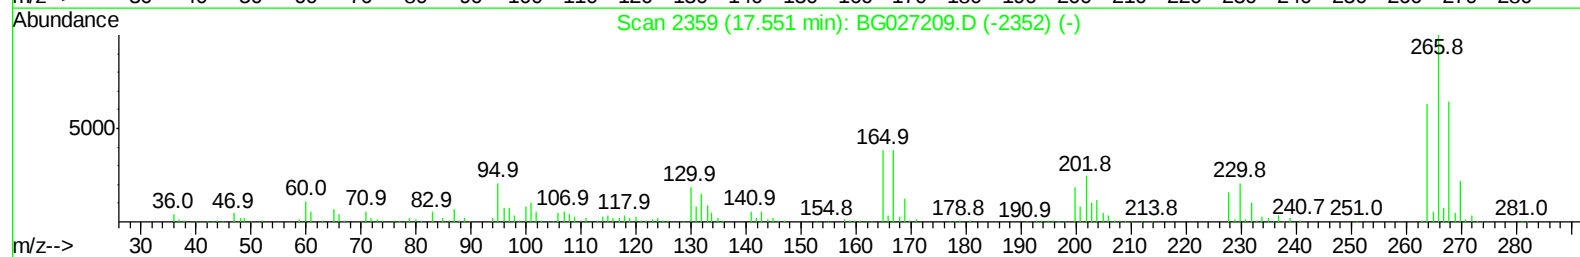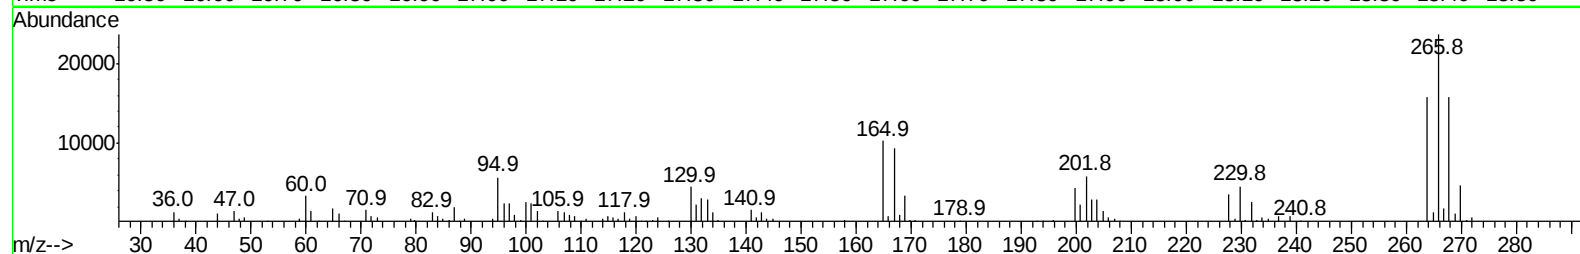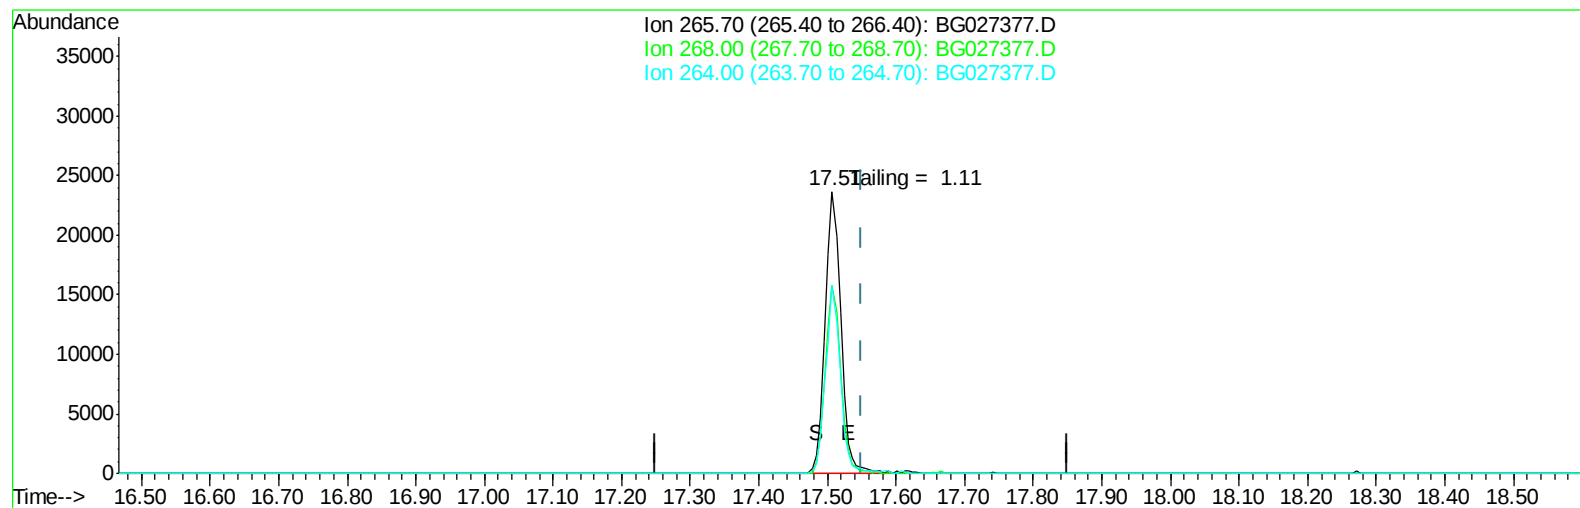

TIC: BG027377.D

(69) Pentachlorophenol (C)

17.507min (-0.043) 2139.17ng

response 37289

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	66.72
264.00	62.60	66.81
0.00	0.00	0.00