

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061217\
 Data File : BG027379.D
 Acq On : 12 Jun 2017 17:30
 Operator : SJ/MA
 Sample : I3576-06
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-OGR1-OGR2

Quant Time: Jun 13 04:13:43 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 05 16:00:35 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.54	152	49346	20.00	ng	-0.03
21) Naphthalene-d8	11.36	136	211995	20.00	ng	-0.04
38) Acenaphthene-d10	15.12	164	122671	20.00	ng	-0.04
63) Phenanthrene-d10	17.87	188	317166	20.00	ng	-0.05
75) Chrysene-d12	22.25	240	383175	20.00	ng	-0.06
86) Perylene-d12	25.92	264	307069	20.00	ng	-0.10
System Monitoring Compounds						
5) 2-Fluorophenol	6.14	112	508955	157.39	ng	-0.02
7) Phenol-d6	7.68	99	632045	133.15	ng	-0.02
23) Nitrobenzene-d5	9.71	82	423822	125.73	ng	-0.03
41) 2,4,6-Tribromophenol	16.61	330	301663	186.75	ng	-0.04
44) 2-Fluorobiphenyl	13.74	172	926206	105.63	ng	-0.05
78) Terphenyl-d14	20.45	244	1739050	115.78	ng	-0.05


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061217\
Data File : BG027379.D
Acq On : 12 Jun 2017 17:30
Operator : SJ/MA
Sample : I3576-06
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-OGR1-OGR2

Quant Time: Jun 13 04:13:43 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:00:35 2017
Response via : Initial Calibration

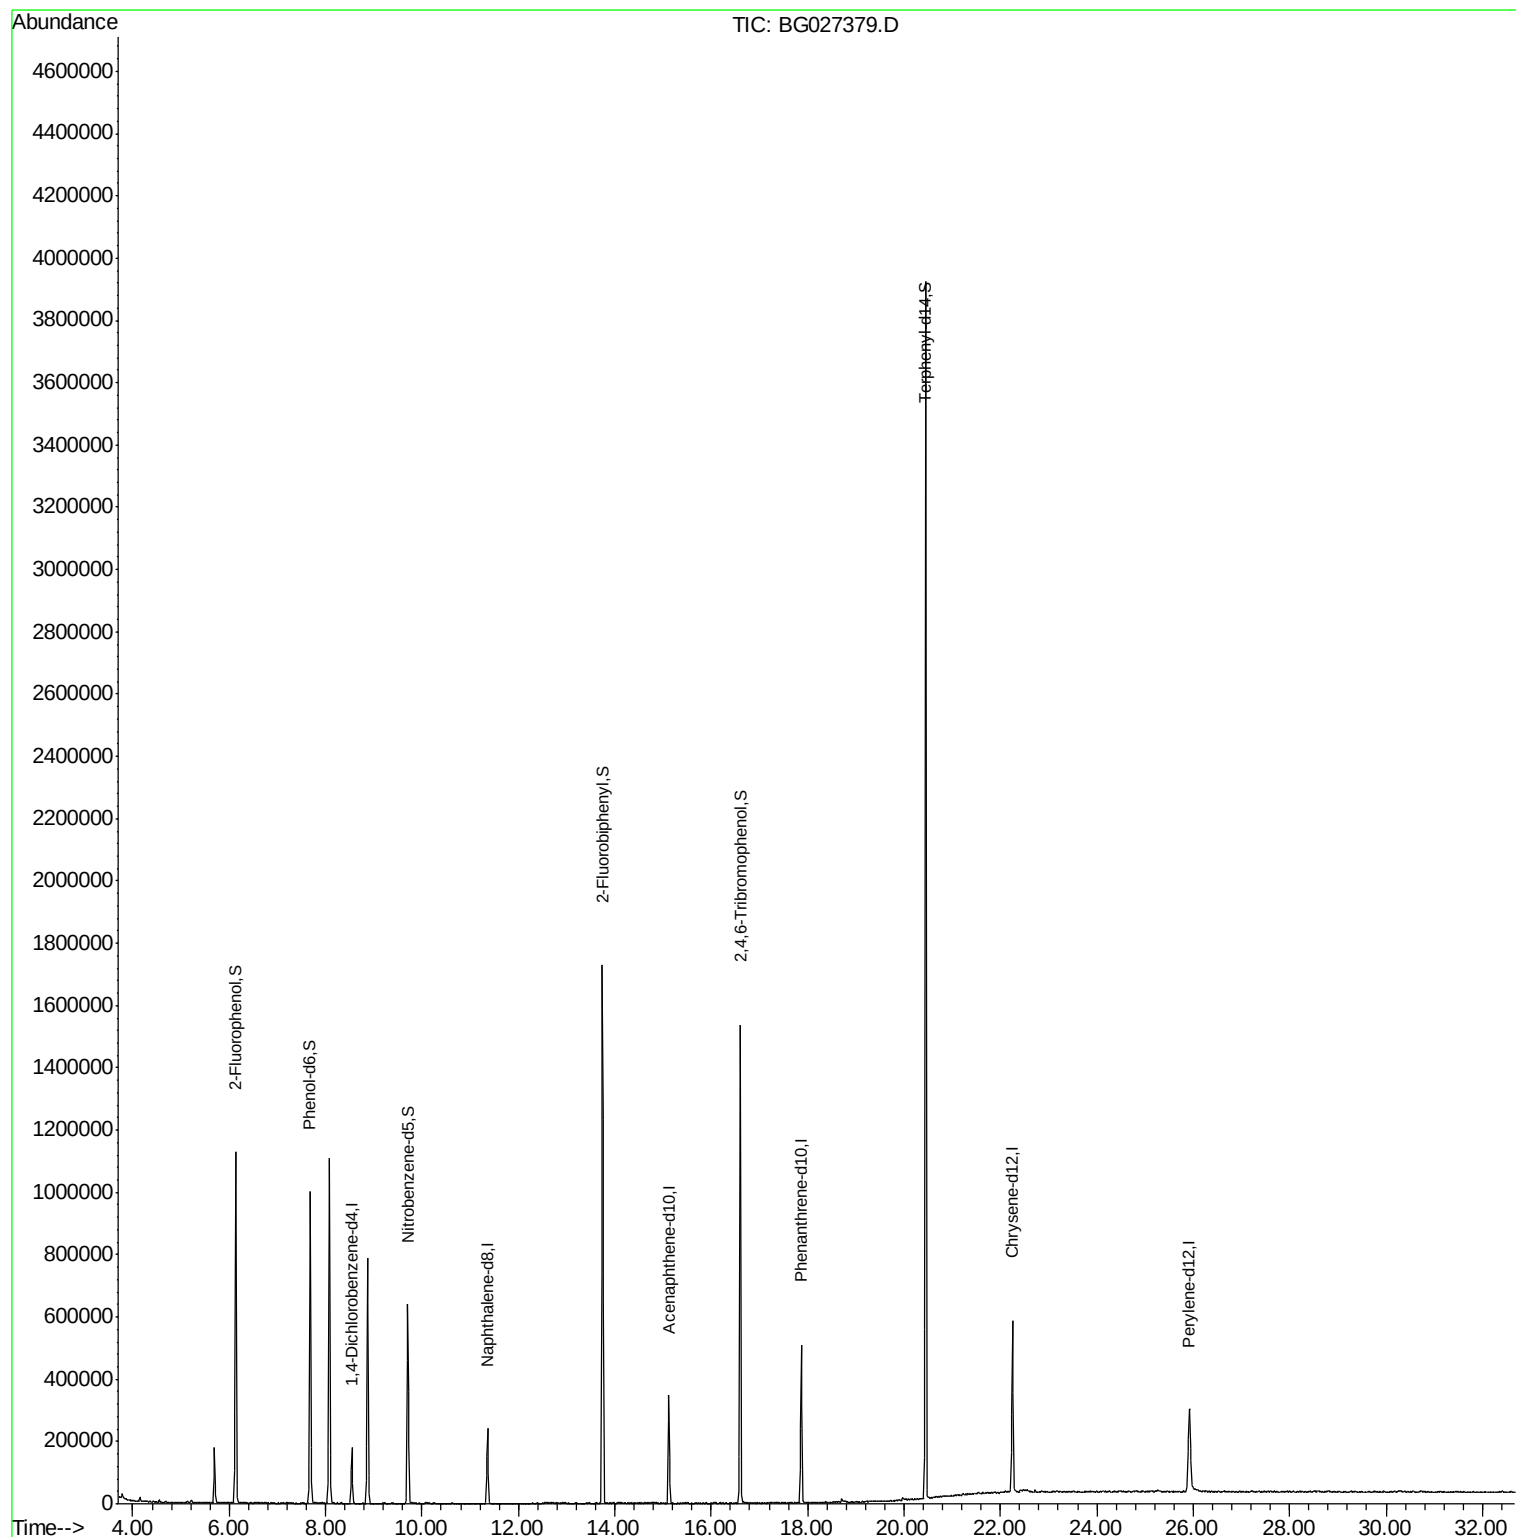




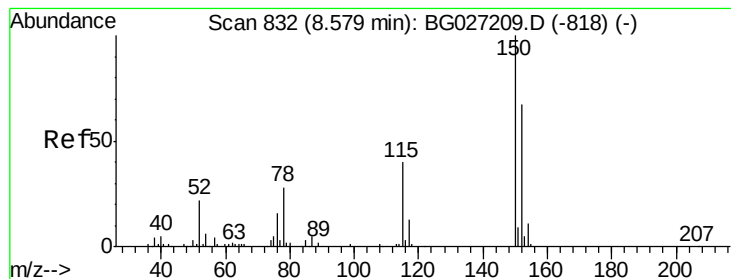


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.54 min Scan# 826
Delta R.T. -0.03 min
Lab File: BG027379.D
Acq: 12 Jun 2017 17:30

Instrument :
BNA_G
ClientSampleId :
TP-OGR1-OGR2




Tgt Ion:152 Resp: 49346
Ion Ratio Lower Upper
152 100
150 159.0 114.0 171.0
115 70.1 48.1 72.1

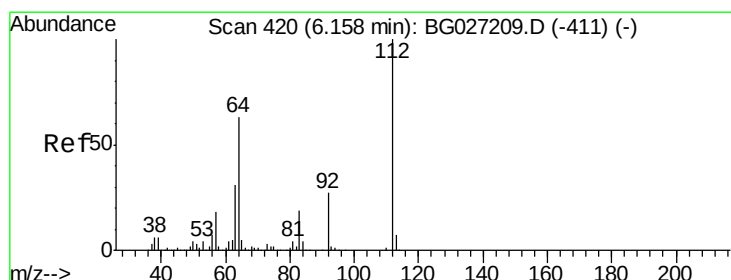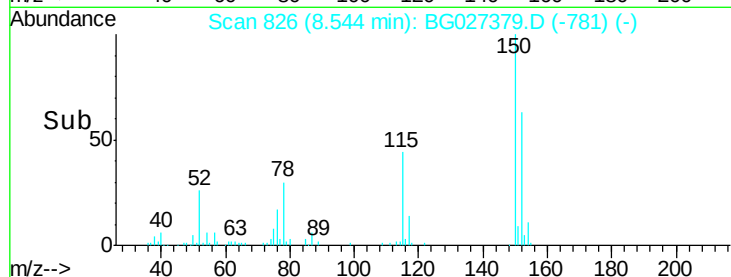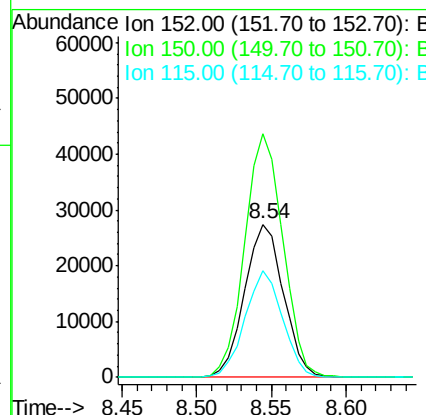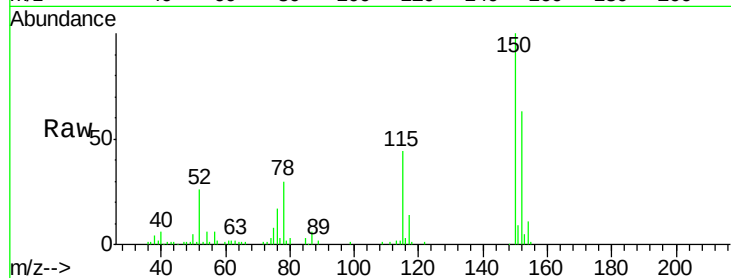


#5

2-Fluorophenol
Concen: 157.388 ng
RT: 6.14 min Scan# 416
Delta R.T. -0.02 min
Lab File: BG027379.D
Acq: 12 Jun 2017 17:30

Tgt Ion:112 Resp: 508955
Ion Ratio Lower Upper
112 100
64 72.4 61.8 92.6
63 34.6 37.2 55.8#

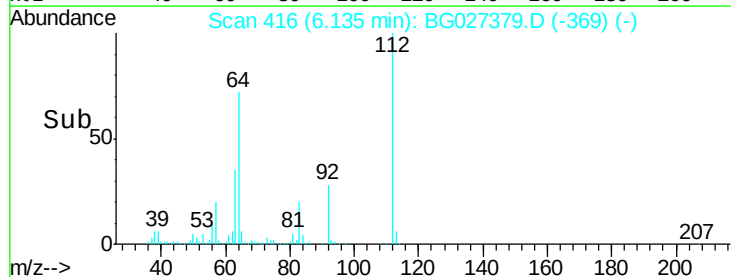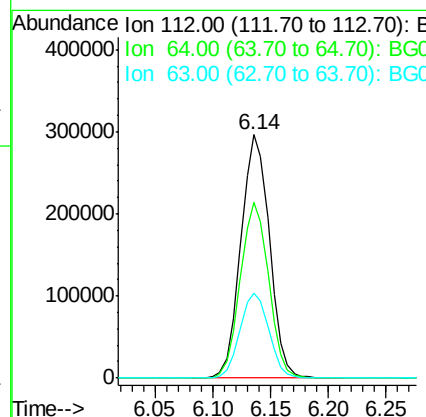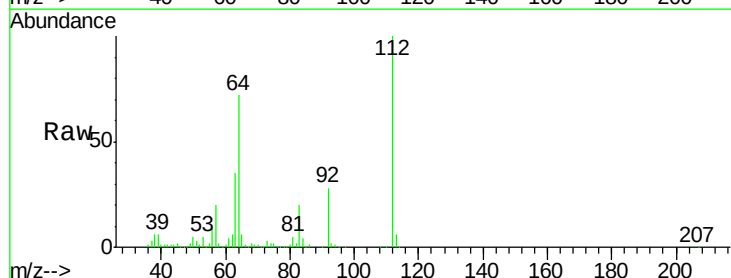

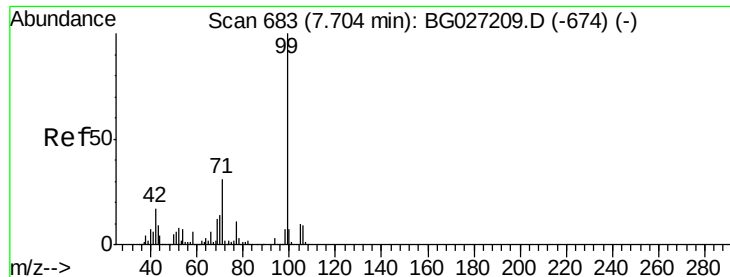

#7

Phenol-d6

Concen: 133.152 ng

RT: 7.68 min Scan# 679

Delta R.T. -0.02 min

Lab File: BG027379.D

Acq: 12 Jun 2017 17:30

Instrument :

BNA_G

ClientSampleId :

TP-OGR1-OGR2


Tgt Ion: 99 Resp: 632045

Ion Ratio Lower Upper




99 100

42 18.0 20.5 30.7#

71 34.6 37.6 56.4#

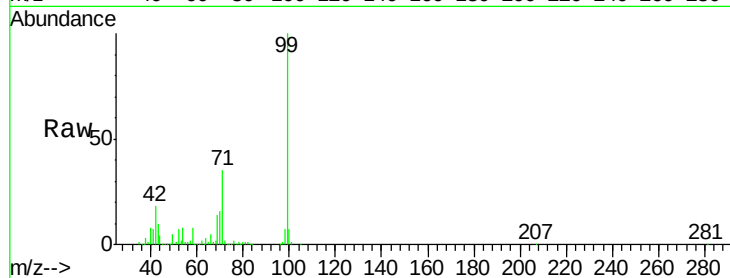

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

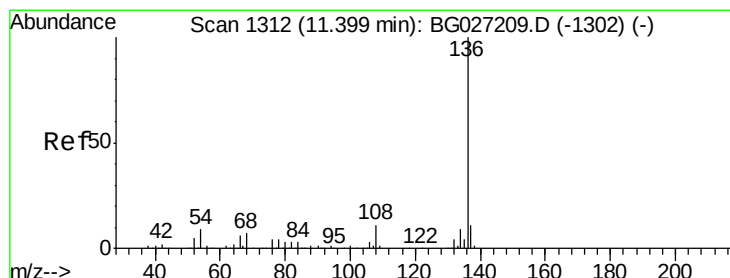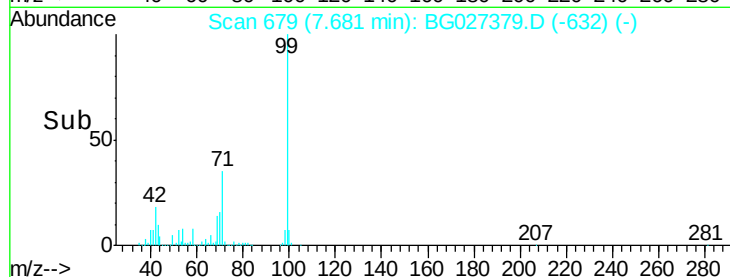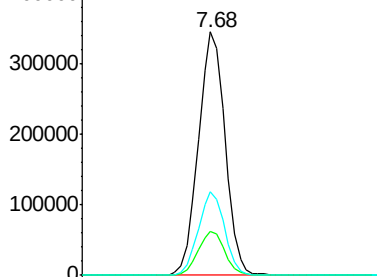

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.36 min Scan# 1305

Delta R.T. -0.04 min

Lab File: BG027379.D

Acq: 12 Jun 2017 17:30

Tgt Ion: 136 Resp: 211995


Ion Ratio Lower Upper

136 100



137 11.1 8.9 13.3


54 11.6 9.3 13.9

68 7.8 5.1 7.7#

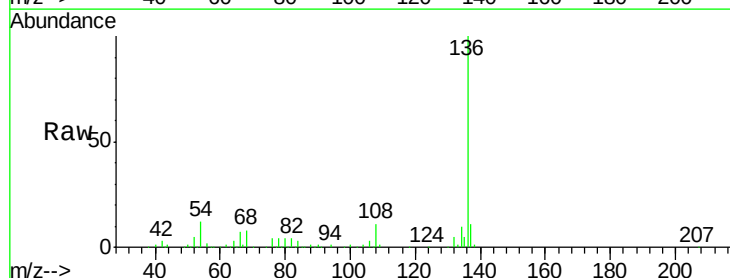

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

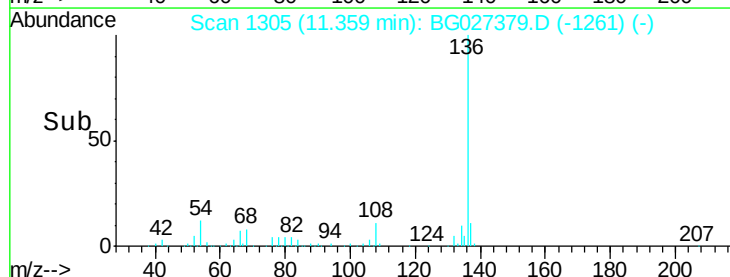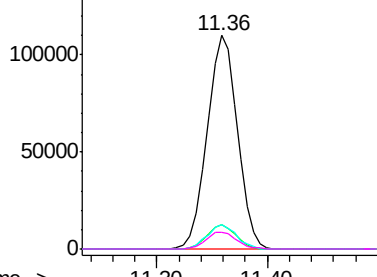


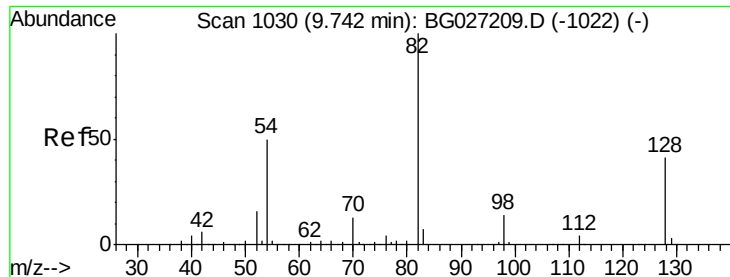




#23
 Nitrobenzene-d5
 Concen: 125.729 ng
 RT: 9.71 min Scan# 1024
 Delta R.T. -0.03 min
 Lab File: BG027379.D
 Acq: 12 Jun 2017 17:30

Instrument :
 BNA_G
 ClientSampleId :
 TP-OGR1-OGR2

Tgt Ion: 82 Resp: 423822
 Ion Ratio Lower Upper
 82 100
 128 38.5 26.4 39.6
 54 52.6 49.4 74.2

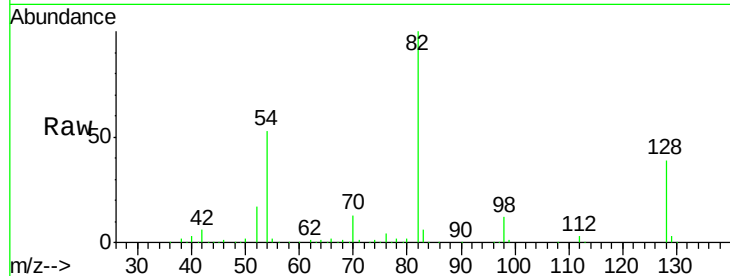


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

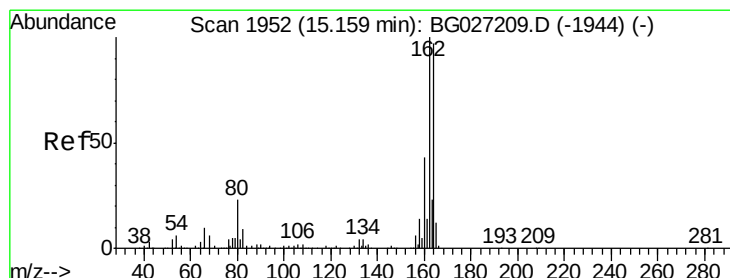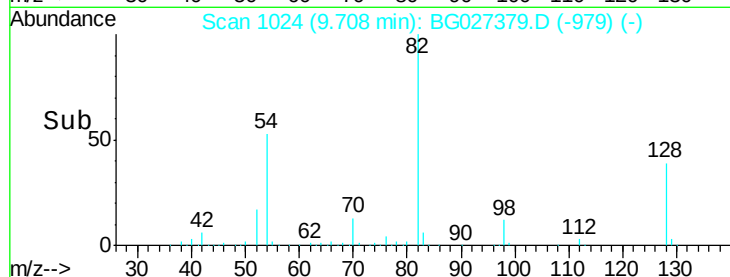
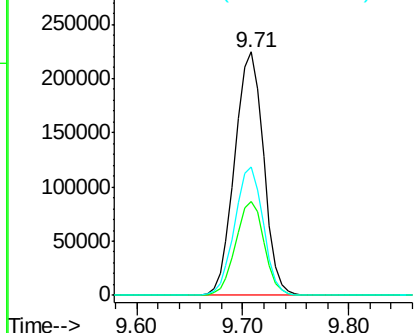



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 15.12 min Scan# 1945
 Delta R.T. -0.04 min
 Lab File: BG027379.D
 Acq: 12 Jun 2017 17:30

Tgt Ion: 164 Resp: 122671
 Ion Ratio Lower Upper
 164 100
 162 105.5 85.1 127.7
 160 45.2 34.7 52.1

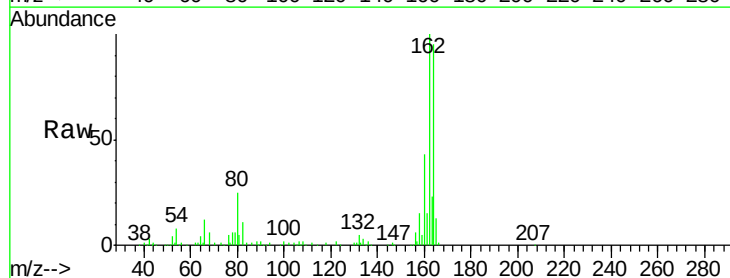

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

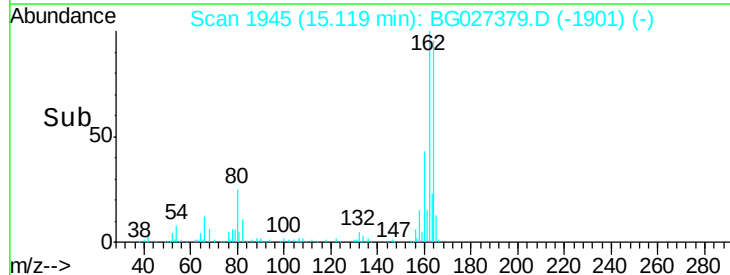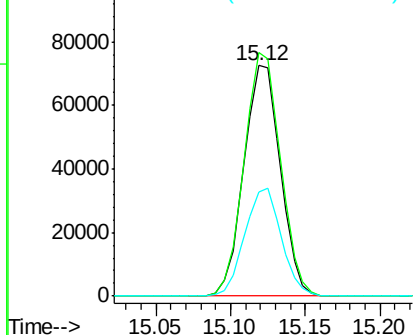


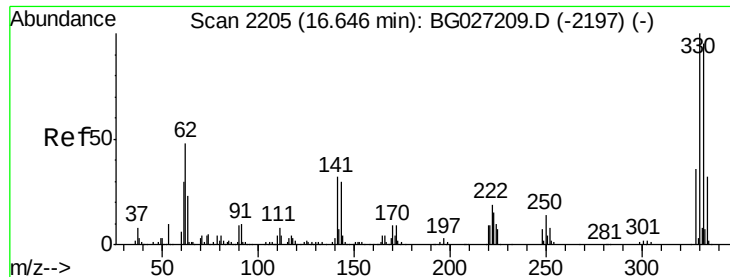




#41
 2,4,6-Tribromophenol
 Concen: 186.746 ng
 RT: 16.61 min Scan# 2198
 Delta R.T. -0.04 min
 Lab File: BG027379.D
 Acq: 12 Jun 2017 17:30

Instrument :
 BNA_G
 ClientSampleId :
 TP-OGR1-OGR2

Tgt Ion:330 Resp: 301663
 Ion Ratio Lower Upper
 330 100
 332 98.4 77.3 115.9
 141 33.5 32.1 48.1

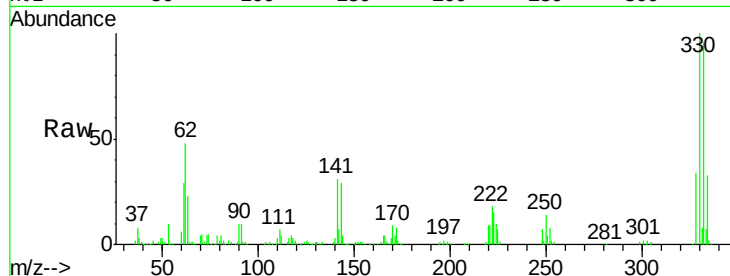


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

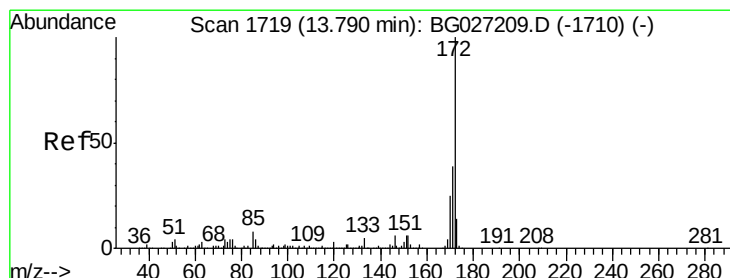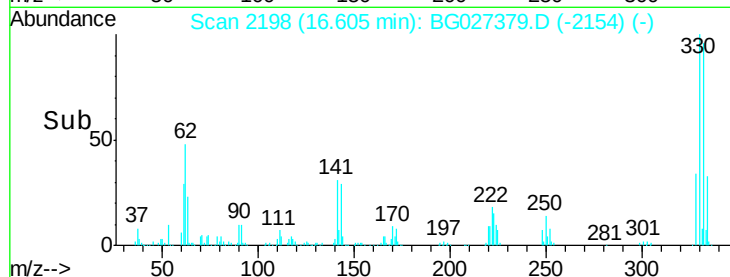
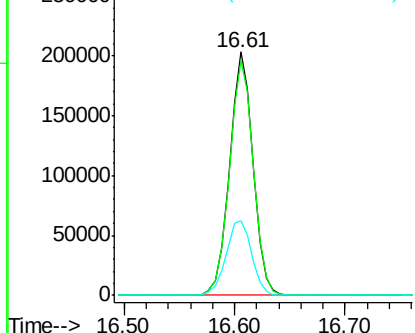



#44
 2-Fluorobiphenyl
 Concen: 105.627 ng
 RT: 13.74 min Scan# 1711
 Delta R.T. -0.05 min
 Lab File: BG027379.D
 Acq: 12 Jun 2017 17:30

Tgt Ion:172 Resp: 926206
 Ion Ratio Lower Upper
 172 100
 171 37.3 32.2 48.2
 170 24.5 21.8 32.6

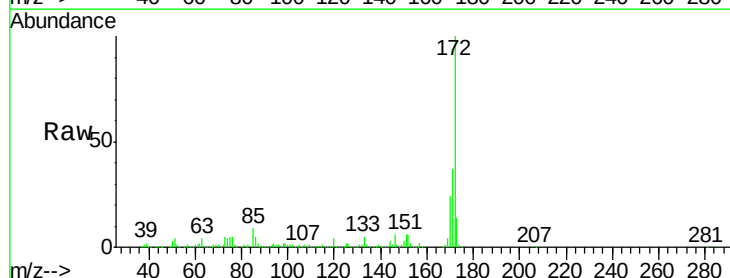

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

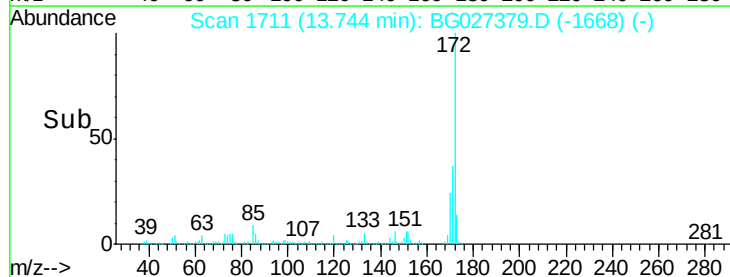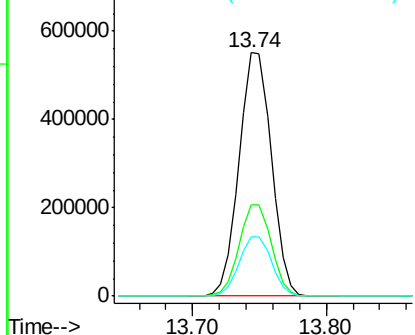


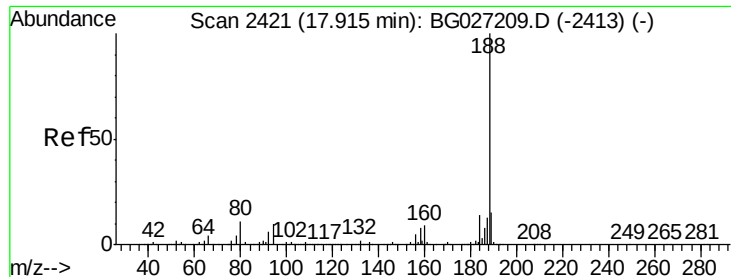




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.87 min Scan# 2413
Delta R.T. -0.05 min
Lab File: BG027379.D
Acq: 12 Jun 2017 17:30

Instrument :
BNA_G
ClientSampleId :
TP-OGR1-OGR2

Tgt Ion:188 Resp: 317166
Ion Ratio Lower Upper
188 100
94 11.5 5.8 8.8#
80 13.5 7.5 11.3#

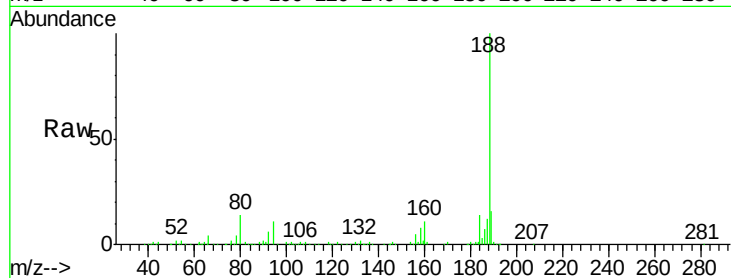


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

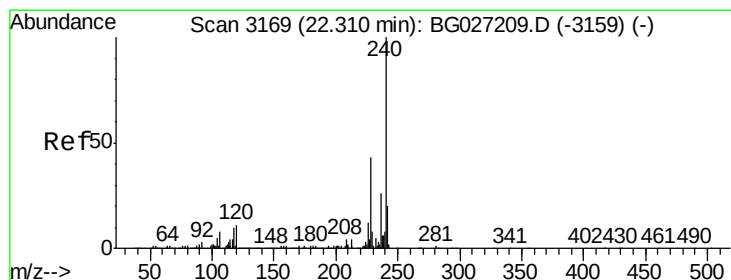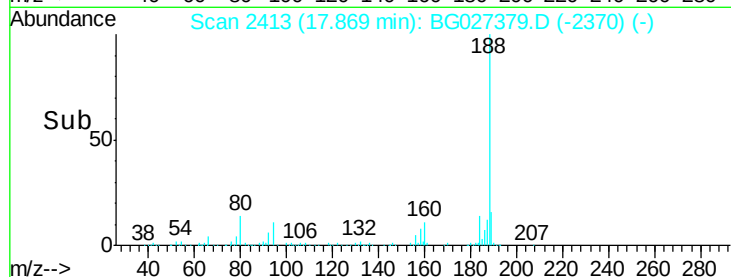
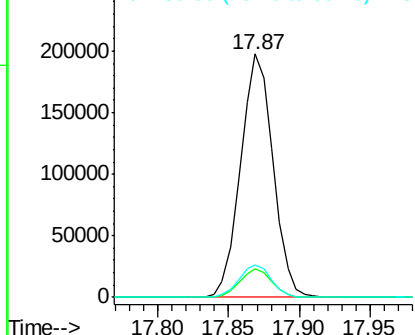



#75
Chrysene-d12
Concen: 20.000 ng
RT: 22.25 min Scan# 3159
Delta R.T. -0.06 min
Lab File: BG027379.D
Acq: 12 Jun 2017 17:30

Tgt Ion:240 Resp: 383175
Ion Ratio Lower Upper
240 100
120 11.3 5.7 8.5#
236 26.4 22.2 33.4

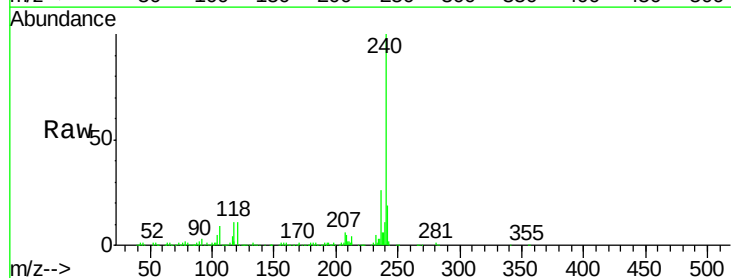

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

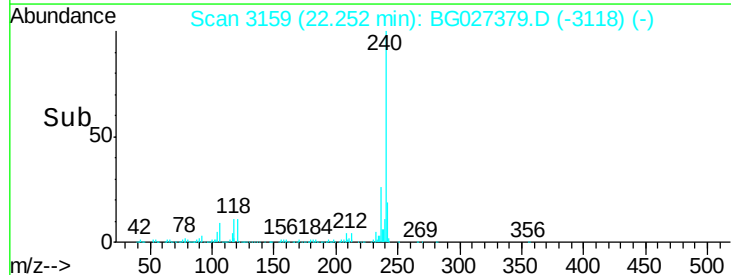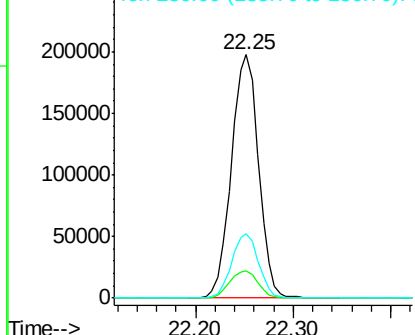

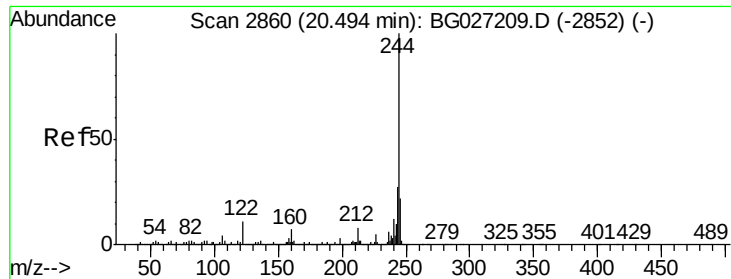

#78

Terphenyl-d14

Concen: 115.778 ng

RT: 20.45 min Scan# 2852

Delta R.T. -0.05 min

Lab File: BG027379.D

Acq: 12 Jun 2017 17:30

Instrument :

BNA_G

ClientSampleId :

TP-OGR1-OGR2


Tgt Ion:244 Resp: 1739050

Ion Ratio Lower Upper

244 100

212 8.3 10.0 15.0#




122 12.6 8.6 12.8

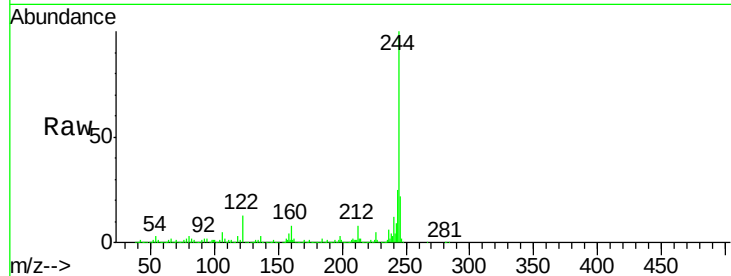

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

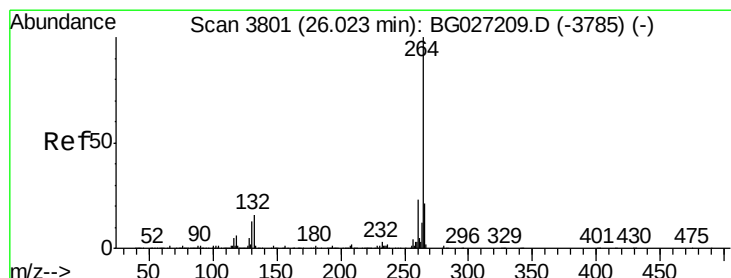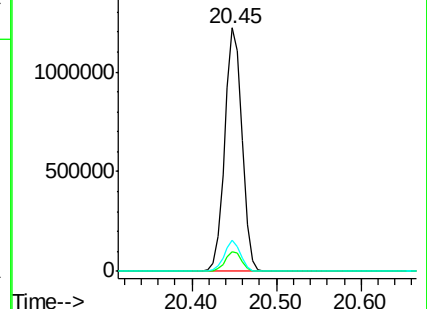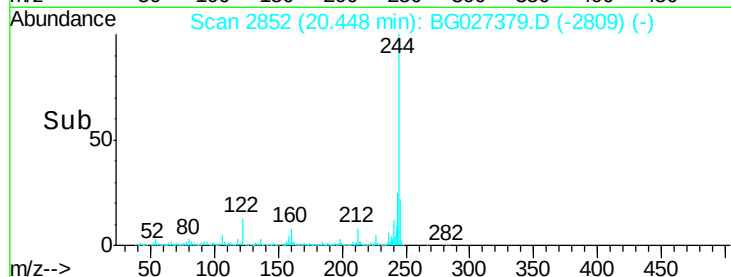

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.92 min Scan# 3784

Delta R.T. -0.10 min

Lab File: BG027379.D

Acq: 12 Jun 2017 17:30


Tgt Ion:264 Resp: 307069

Ion Ratio Lower Upper

264 100

260 24.8 21.8 32.8

265 20.8 18.2 27.4

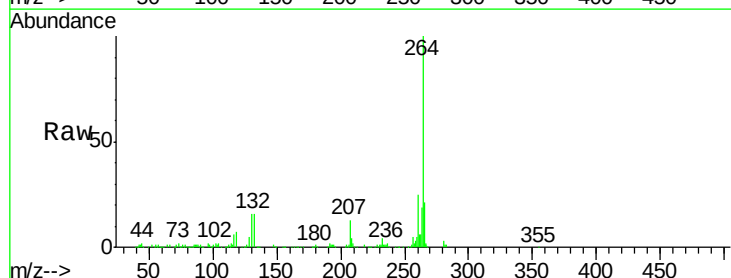

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

