

Data Path : Z:\HPCHEM1\BNA\_G\DATA\BG061217\  
 Data File : BG027384.D  
 Acq On : 12 Jun 2017 20:49  
 Operator : SJ/MA  
 Sample : I3624-03  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 NB-RO6151-060917

Quant Time: Jun 13 04:23:06 2017  
 Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG060517.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Jun 05 16:00:35 2017  
 Response via : Initial Calibration

| Internal Standards          | R.T.  | QIon | Response | Conc   | Units | Dev(Min) |
|-----------------------------|-------|------|----------|--------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4   | 8.54  | 152  | 45788    | 20.00  | ng    | -0.04    |
| 21) Naphthalene-d8          | 11.36 | 136  | 202156   | 20.00  | ng    | -0.04    |
| 38) Acenaphthene-d10        | 15.12 | 164  | 119854   | 20.00  | ng    | -0.04    |
| 63) Phenanthrene-d10        | 17.87 | 188  | 325928   | 20.00  | ng    | -0.05    |
| 75) Chrysene-d12            | 22.25 | 240  | 383440   | 20.00  | ng    | -0.06    |
| 86) Perylene-d12            | 25.92 | 264  | 272590   | 20.00  | ng    | -0.10    |
| System Monitoring Compounds |       |      |          |        |       |          |
| 5) 2-Fluorophenol           | 6.13  | 112  | 407140   | 135.69 | ng    | -0.02    |
| 7) Phenol-d6                | 7.68  | 99   | 534313   | 121.31 | ng    | -0.02    |
| 23) Nitrobenzene-d5         | 9.71  | 82   | 333971   | 103.90 | ng    | -0.04    |
| 41) 2,4,6-Tribromophenol    | 16.60 | 330  | 272985   | 172.97 | ng    | -0.04    |
| 44) 2-Fluorobiphenyl        | 13.75 | 172  | 751322   | 87.70  | ng    | -0.04    |
| 78) Terphenyl-d14           | 20.45 | 244  | 1564476  | 104.08 | ng    | -0.05    |


| Target Compounds | Qvalue |
|------------------|--------|
|------------------|--------|


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA\_G\DATA\BG061217\  
Data File : BG027384.D  
Acq On : 12 Jun 2017 20:49  
Operator : SJ/MA  
Sample : I3624-03  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
NB-RO6151-060917

Quant Time: Jun 13 04:23:06 2017  
Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG060517.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jun 05 16:00:35 2017  
Response via : Initial Calibration

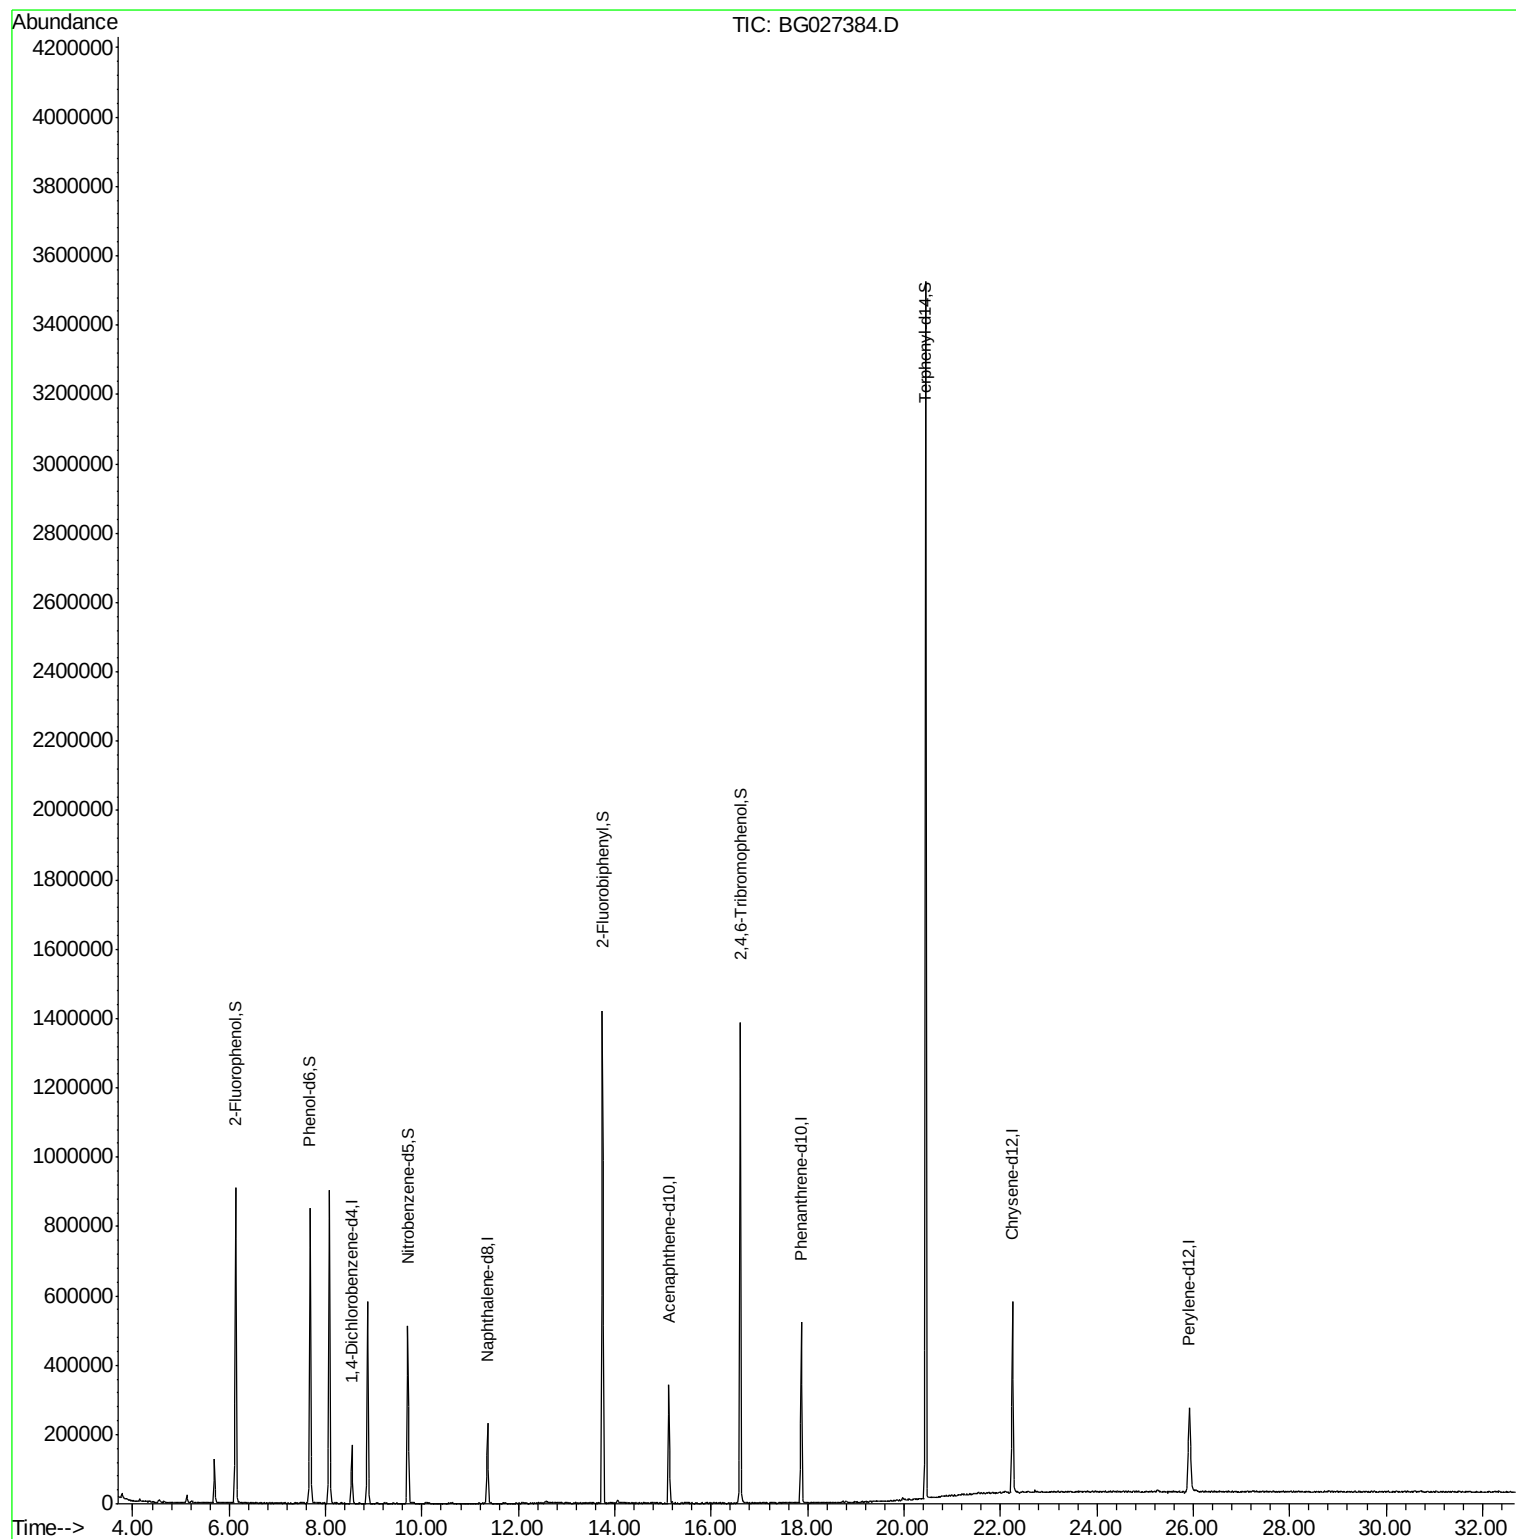

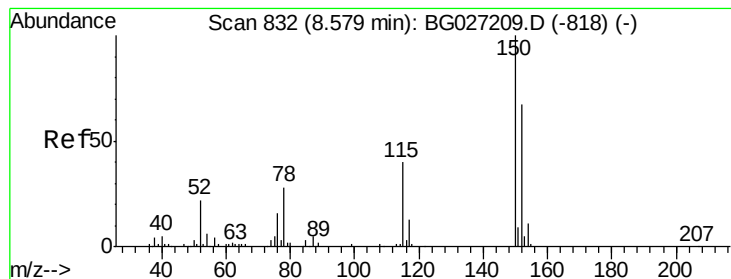


#1




1,4-Dichlorobenzene-d4  
Concen: 20.000 ng  
RT: 8.54 min Scan# 826  
Delta R.T. -0.04 min  
Lab File: BG027384.D  
Acq: 12 Jun 2017 20:49

Instrument :  
BNA\_G  
ClientSampleId :  
NB-RO6151-060917

Tgt Ion:152 Resp: 45788  
Ion Ratio Lower Upper  
152 100  
150 162.6 114.0 171.0  
115 66.5 48.1 72.1




Abundance Ion 152.00 (151.70 to 152.70): E  
Ion 150.00 (149.70 to 150.70): E  
Ion 115.00 (114.70 to 115.70): E

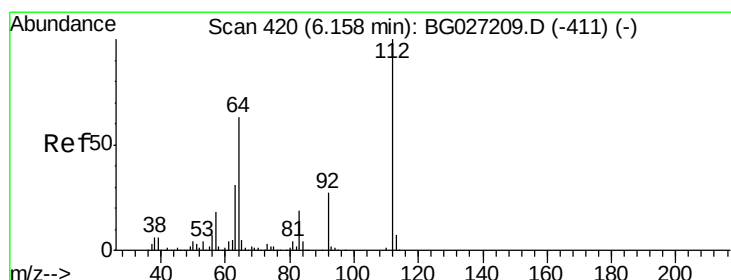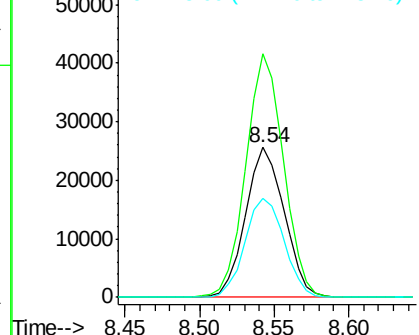



#5


2-Fluorophenol  
Concen: 135.687 ng  
RT: 6.13 min Scan# 416  
Delta R.T. -0.02 min  
Lab File: BG027384.D  
Acq: 12 Jun 2017 20:49

Tgt Ion:112 Resp: 407140  
Ion Ratio Lower Upper  
112 100  
64 70.0 61.8 92.6  
63 36.4 37.2 55.8#



Abundance Ion 112.00 (111.70 to 112.70): E  
Ion 64.00 (63.70 to 64.70): BGC  
Ion 63.00 (62.70 to 63.70): BGC

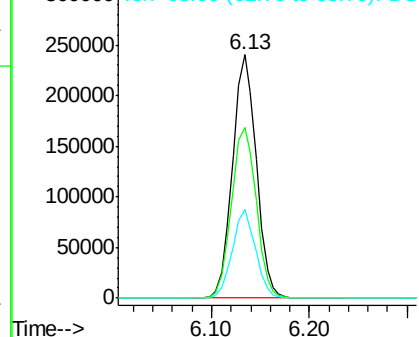

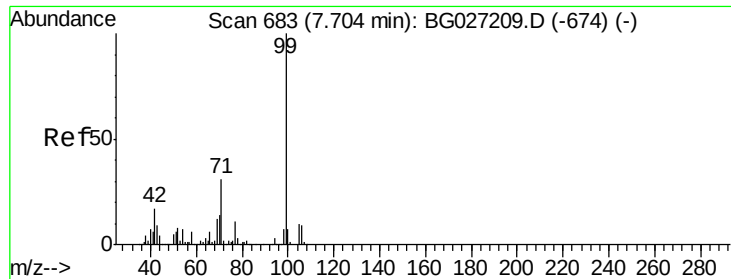

#7

Phenol-d6

Concen: 121.309 ng

RT: 7.68 min Scan# 679

Delta R.T. -0.02 min

Lab File: BG027384.D

Acq: 12 Jun 2017 20:49

Instrument :

BNA\_G

ClientSampleId :

NB-RO6151-060917


Tgt Ion: 99 Resp: 534313

Ion Ratio Lower Upper




99 100

42 18.1 20.5 30.7#

71 34.2 37.6 56.4#



Abundance Ion 99.00 (98.70 to 99.70): BGC  
Ion 42.00 (41.70 to 42.70): BGC  
Ion 71.00 (70.70 to 71.70): BGC

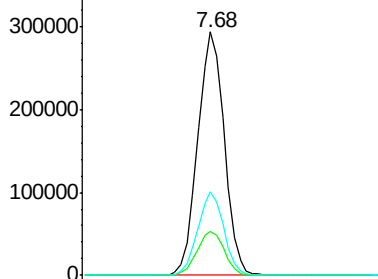

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.36 min Scan# 1305

Delta R.T. -0.04 min

Lab File: BG027384.D

Acq: 12 Jun 2017 20:49

Tgt Ion: 136 Resp: 202156


Ion Ratio Lower Upper

136 100



137 10.6 8.9 13.3


54 11.7 9.3 13.9

68 8.9 5.1 7.7#



Abundance Ion 136.00 (135.70 to 136.70): BGC  
Ion 137.00 (136.70 to 137.70): BGC  
Ion 54.00 (53.70 to 54.70): BGC  
Ion 68.00 (67.70 to 68.70): BGC




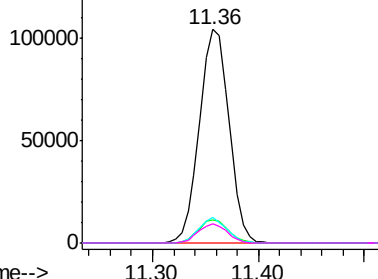




#23  
 Nitrobenzene-d5  
 Concen: 103.897 ng  
 RT: 9.71 min Scan# 1024  
 Delta R.T. -0.04 min  
 Lab File: BG027384.D  
 Acq: 12 Jun 2017 20:49




Instrument :  
 BNA\_G  
 ClientSampleId :  
 NB-RO6151-060917


Tgt Ion: 82 Resp: 333971  
 Ion Ratio Lower Upper  
 82 100  
 128 39.6 26.4 39.6#  
 54 52.4 49.4 74.2

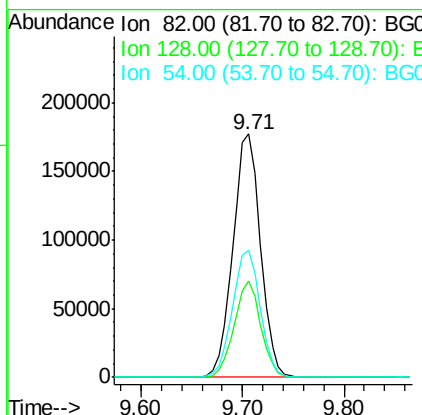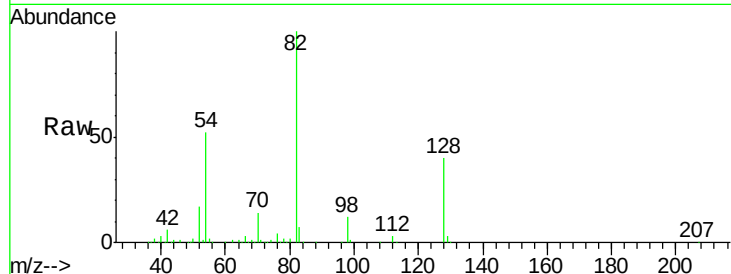

#38  
 Acenaphthene-d10  
 Concen: 20.000 ng  
 RT: 15.12 min Scan# 1945  
 Delta R.T. -0.04 min  
 Lab File: BG027384.D  
 Acq: 12 Jun 2017 20:49

Tgt Ion: 164 Resp: 119854  
 Ion Ratio Lower Upper  
 164 100  
 162 103.8 85.1 127.7  
 160 44.7 34.7 52.1

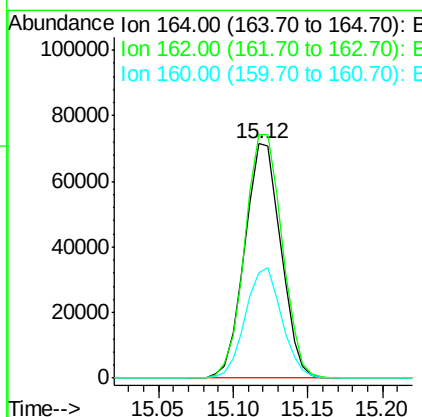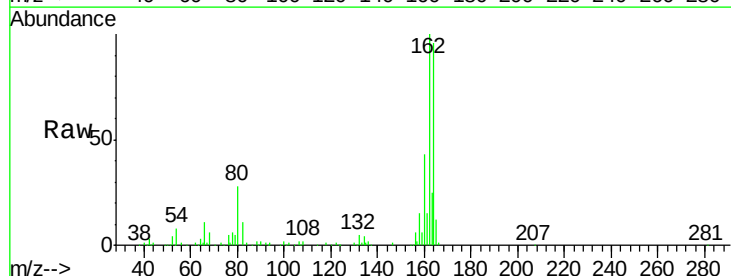


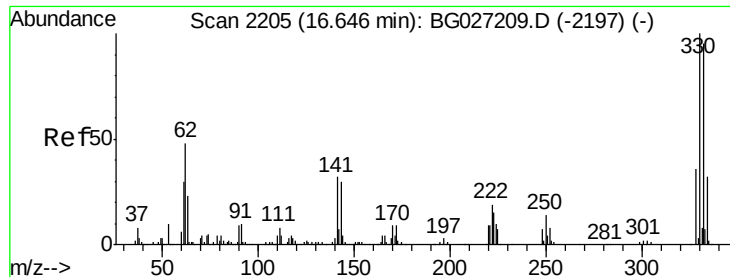




#41  
 2,4,6-Tribromophenol  
 Concen: 172.965 ng  
 RT: 16.60 min Scan# 2198  
 Delta R.T. -0.04 min  
 Lab File: BG027384.D  
 Acq: 12 Jun 2017 20:49

Instrument :  
 BNA\_G  
 ClientSampleId :  
 NB-RO6151-060917

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 330     | 100   |       |       |
| 332     | 95.8  | 77.3  | 115.9 |
| 141     | 33.2  | 32.1  | 48.1  |

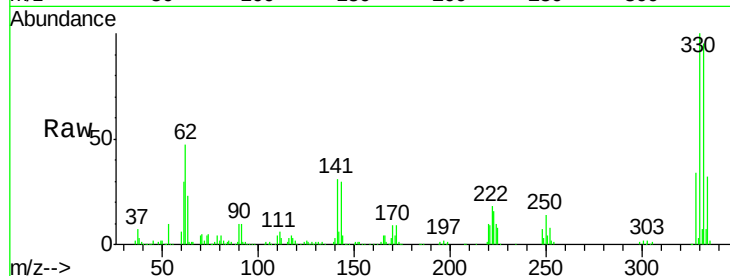


Abundance Ion 329.80 (329.50 to 330.50): E  
 Ion 331.80 (331.50 to 332.50): E  
 Ion 141.00 (140.70 to 141.70): E

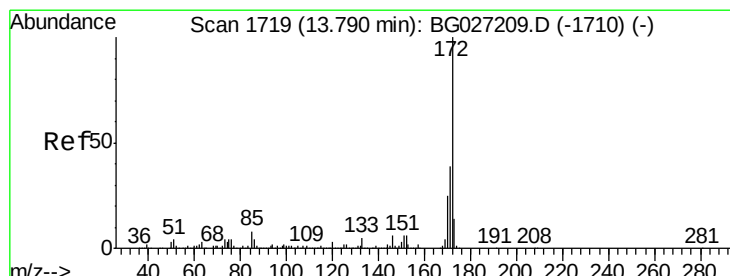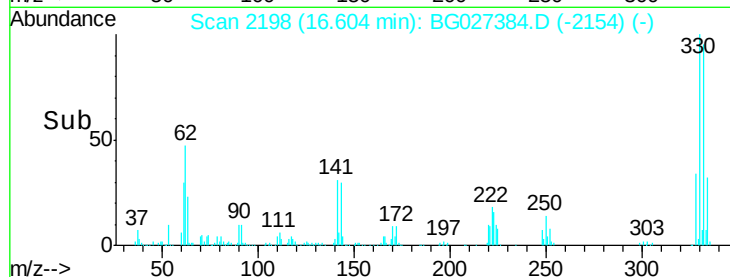
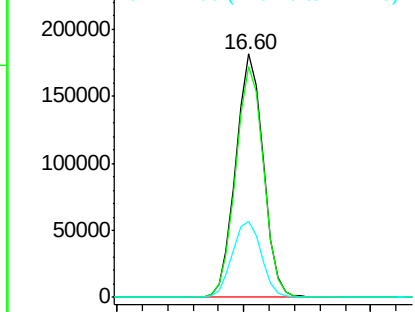



#44  
 2-Fluorobiphenyl  
 Concen: 87.697 ng  
 RT: 13.75 min Scan# 1712  
 Delta R.T. -0.04 min  
 Lab File: BG027384.D  
 Acq: 12 Jun 2017 20:49

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 172     | 100   |       |       |
| 171     | 36.4  | 32.2  | 48.2  |
| 170     | 24.7  | 21.8  | 32.6  |

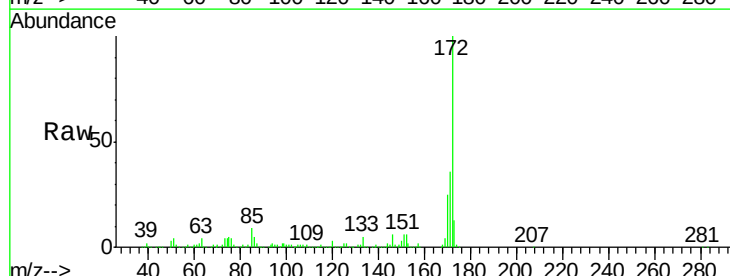

Abundance Ion 172.00 (171.70 to 172.70): E  
 Ion 171.00 (170.70 to 171.70): E  
 Ion 170.00 (169.70 to 170.70): E



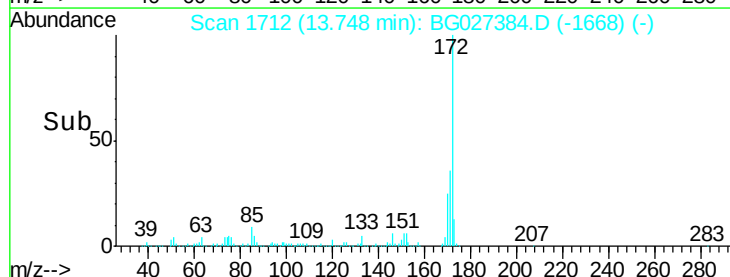
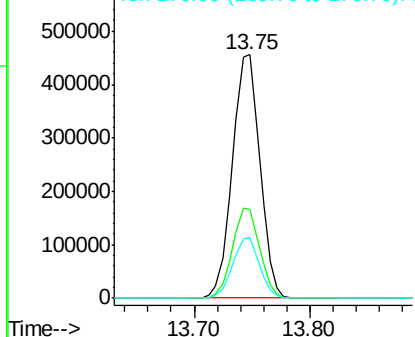




#63  
Phenanthrene-d10  
Concen: 20.000 ng  
RT: 17.87 min Scan# 2413  
Delta R.T. -0.05 min  
Lab File: BG027384.D  
Acq: 12 Jun 2017 20:49




Instrument :  
BNA\_G  
ClientSampleId :  
NB-RO6151-060917


Tgt Ion:188 Resp: 325928  
Ion Ratio Lower Upper  
188 100  
94 11.0 5.8 8.8#  
80 13.0 7.5 11.3#

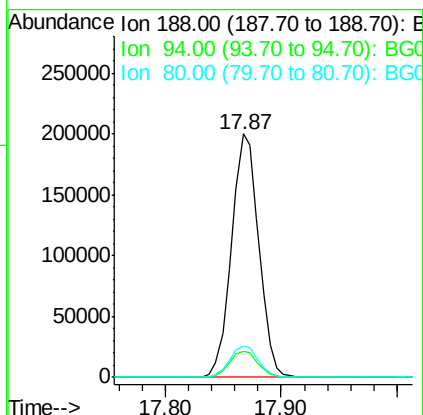

#75  
Chrysene-d12  
Concen: 20.000 ng  
RT: 22.25 min Scan# 3159  
Delta R.T. -0.06 min  
Lab File: BG027384.D  
Acq: 12 Jun 2017 20:49

Tgt Ion:240 Resp: 383440  
Ion Ratio Lower Upper  
240 100  
120 11.4 5.7 8.5#  
236 26.7 22.2 33.4

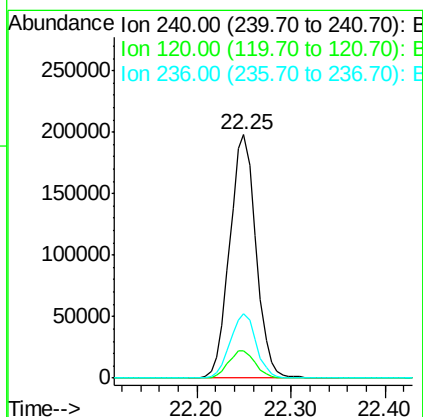

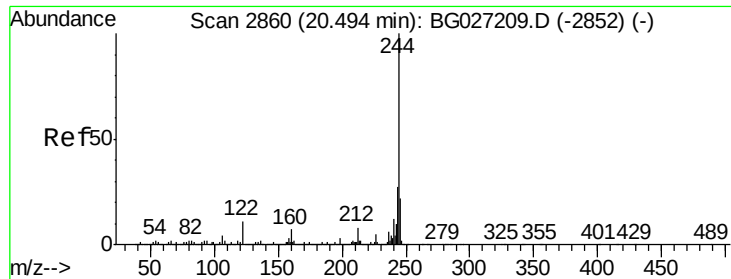

#78

Terphenyl-d14

Concen: 104.084 ng

RT: 20.45 min Scan# 2852

Delta R.T. -0.05 min

Lab File: BG027384.D

Acq: 12 Jun 2017 20:49

Instrument :

BNA\_G

ClientSampleId :

NB-RO6151-060917


Tgt Ion:244 Resp: 1564476

Ion Ratio Lower Upper

244 100

212 8.1 10.0 15.0#




122 12.4 8.6 12.8

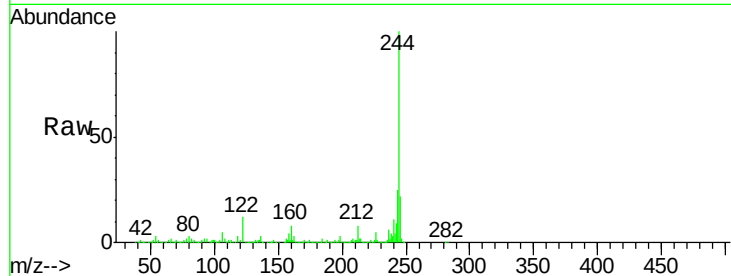

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

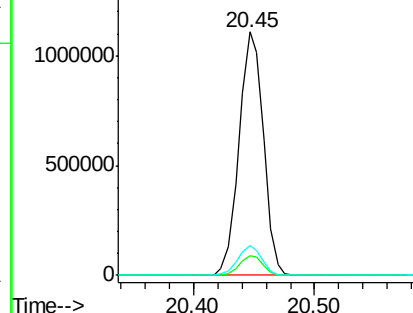

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.92 min Scan# 3784

Delta R.T. -0.10 min

Lab File: BG027384.D

Acq: 12 Jun 2017 20:49


Tgt Ion:264 Resp: 272590

Ion Ratio Lower Upper

264 100

260 24.8 21.8 32.8

265 22.2 18.2 27.4



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

