


Data Path : Z:\HPCHEM1\BNA_G\Data\BG061217\
 Data File : BG027377.D
 Acq On : 12 Jun 2017 16:11
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 05 16:00:35 2017

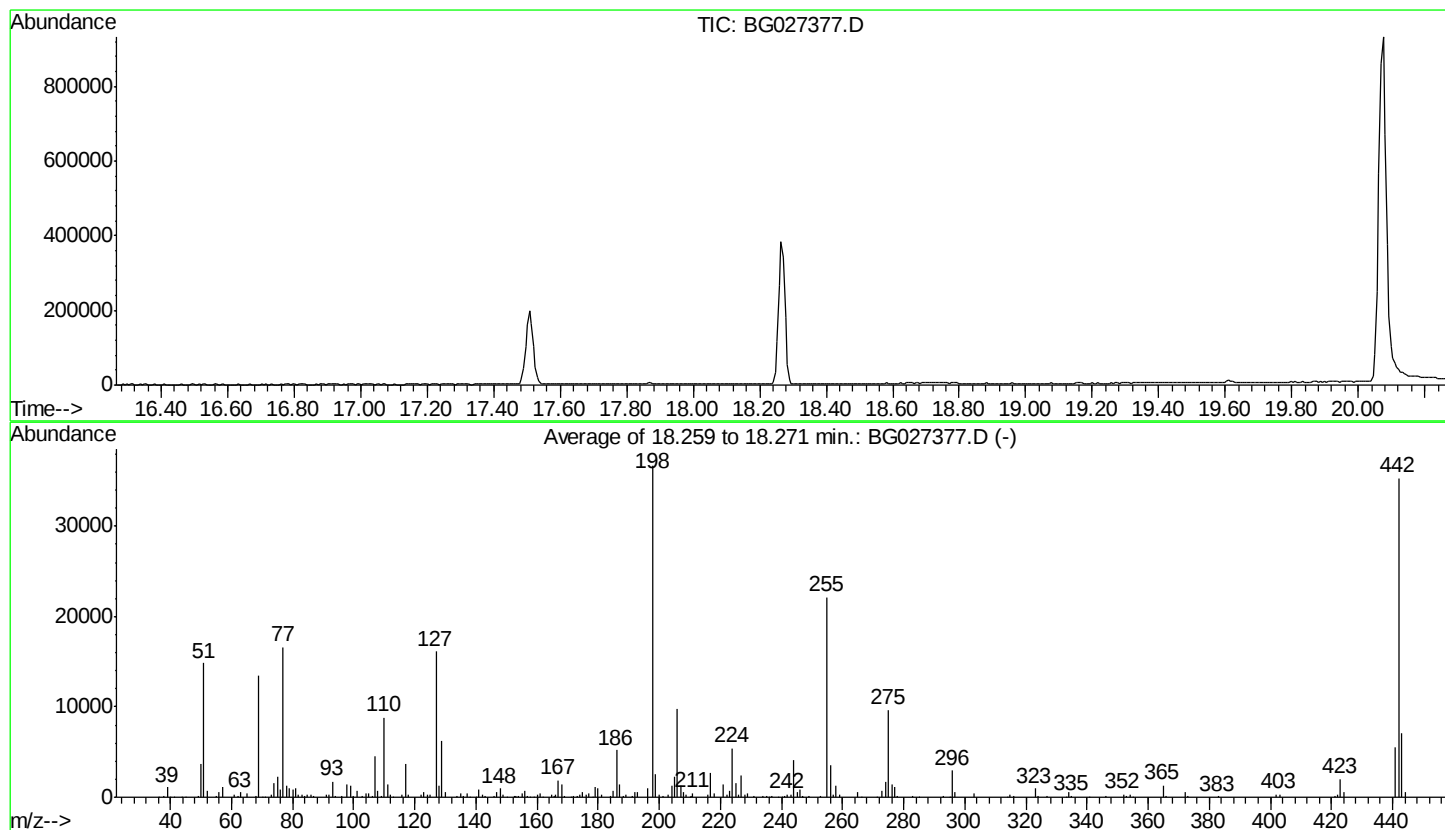

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	14840	PASS
68	69	0.00	2	0.6	85	PASS
69	198	0.00	100	36.8	13514	PASS
70	69	0.00	2	0.4	52	PASS
127	198	10	80	43.8	16092	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	36717	PASS
199	198	5	9	6.9	2533	PASS
275	198	10	60	26.4	9696	PASS
365	198	1	100	3.6	1330	PASS
441	442	0.01	24	15.6	5494	PASS
442	198	50	100	96.1	35296	PASS
443	442	15	24	20.0	7076	PASS