
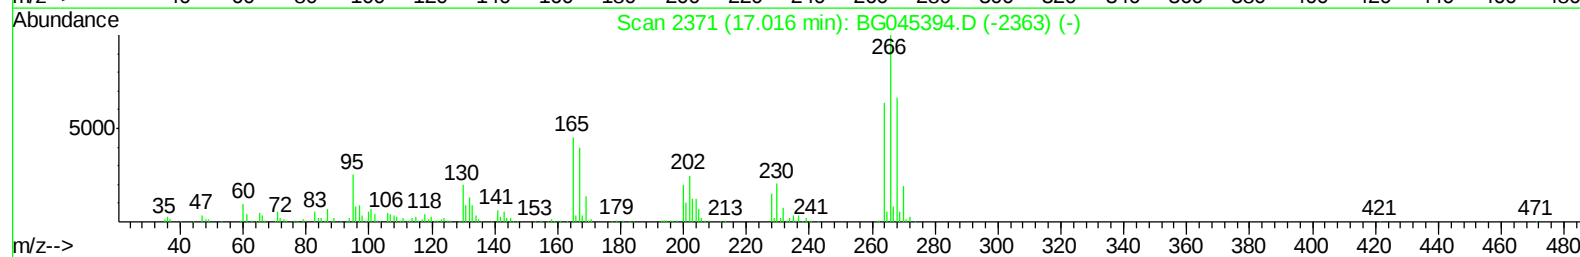
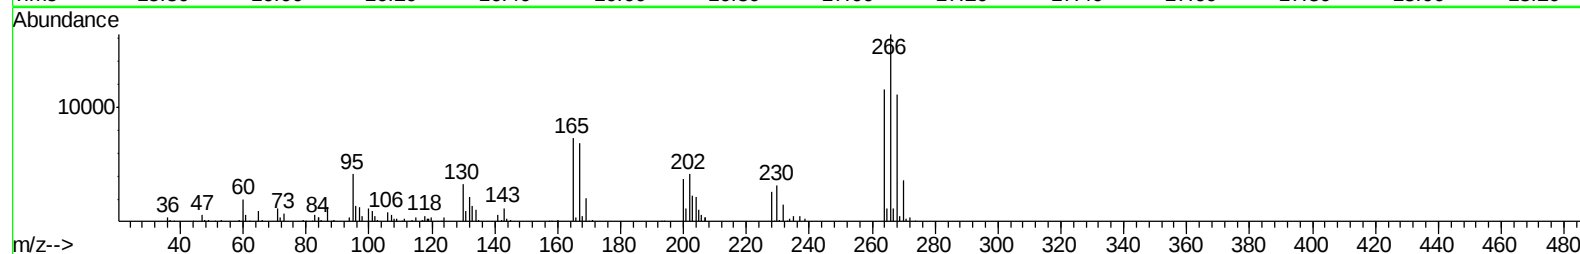


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061220\
Data File : BG045739.D
Acq On : 12 Jun 2020 14:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 02:15:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 01 15:07:00 2020
Response via : Initial Calibration

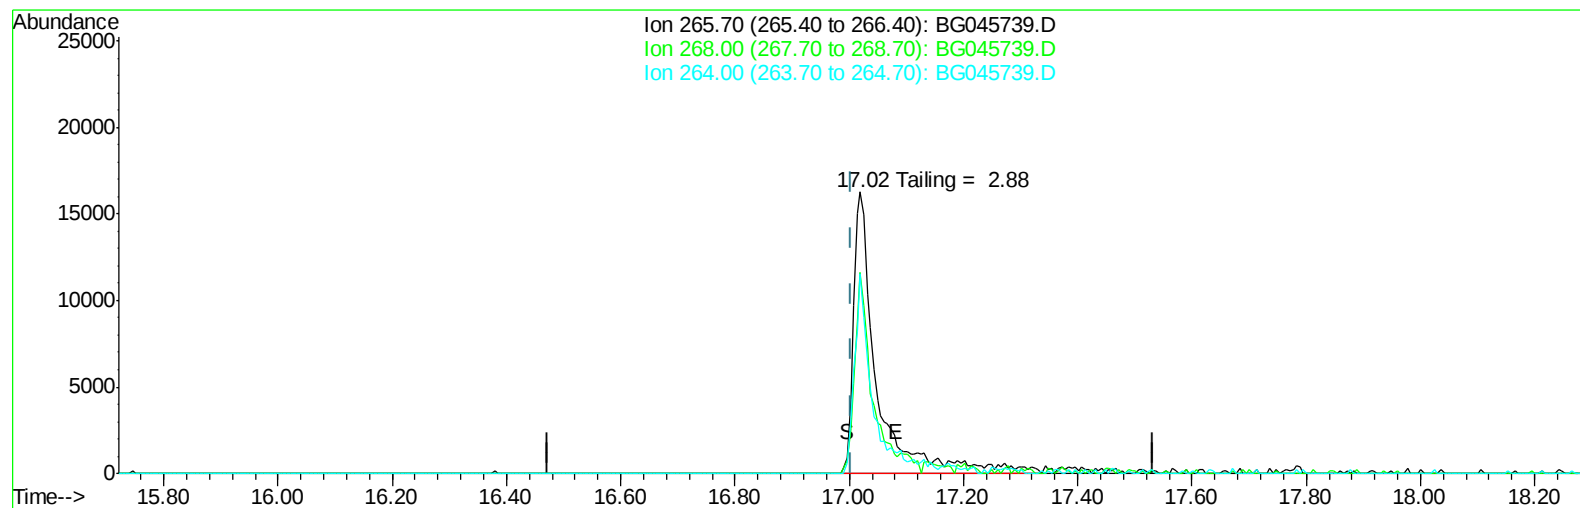

TIC: BG045739.D

(70) Pentachlorophenol (C)




17.020min (+0.016) 108364.53ng

response 39510

Ion	Exp%	Act%
265.70	100	100
268.00	66.50	71.46
264.00	63.70	70.93
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061220\
Data File : BG045739.D
Acq On : 12 Jun 2020 14:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 02:15:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 01 15:07:00 2020
Response via : Initial Calibration

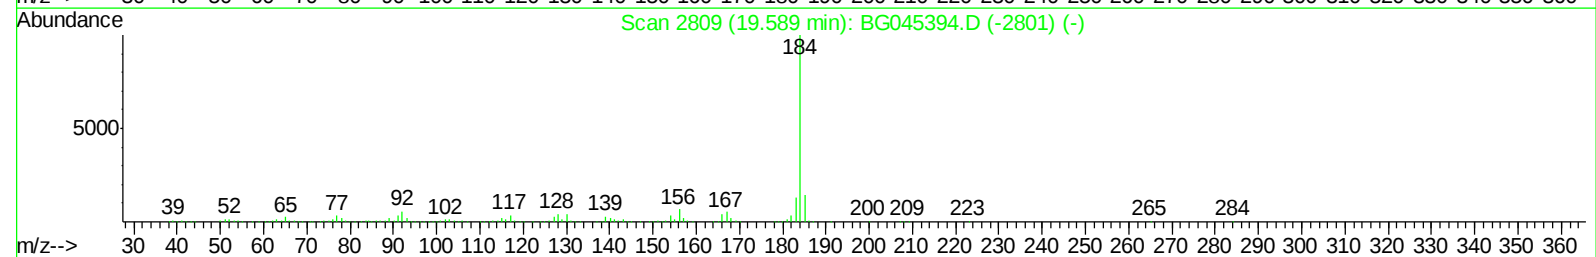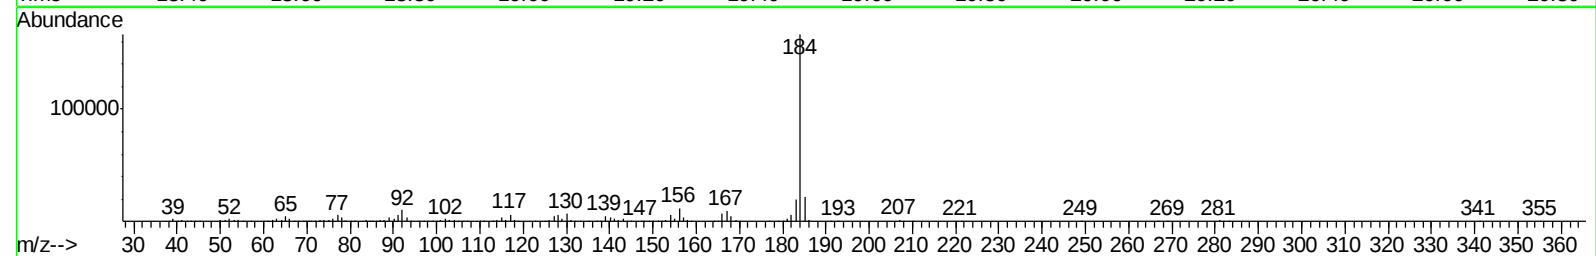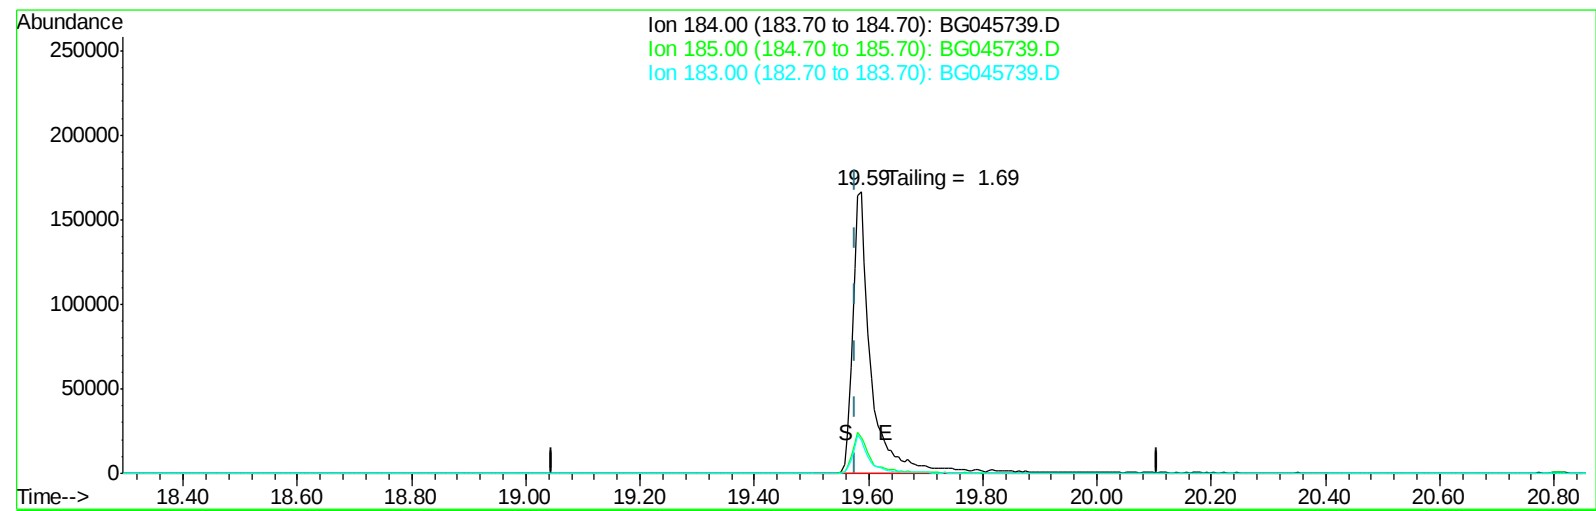

TIC: BG045739.D

(77) Benzidine

19.587min (+0.010) 237379.09ng

response 360013

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	12.92
183.00	12.80	11.99
0.00	0.00	0.00