

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061220\
 Data File : BG045752.D
 Acq On : 12 Jun 2020 22:45
 Operator : CG/JU
 Sample : L2986-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 16-20-COMP

Quant Time: Jun 13 03:04:45 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 01 15:07:00 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.94	152	53907	20.00	ng	0.00
21) Naphthalene-d8	10.75	136	205221	20.00	ng	0.00
39) Acenaphthene-d10	14.59	164	128523	20.00	ng	0.00
64) Phenanthrene-d10	17.34	188	263944	20.00	ng	0.00
76) Chrysene-d12	21.61	240	257717	20.00	ng	0.00
87) Perylene-d12	24.75	264	282969	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	24016	8.71	ng	0.03
7) Phenol-d6	7.18	99	22635	5.77	ng	0.03
23) Nitrobenzene-d5	9.11	82	52535	13.96	ng	0.00
42) 2,4,6-Tribromophenol	16.09	330	25687	15.63	ng	0.00
45) 2-Fluorobiphenyl	13.21	172	117680	15.53	ng	0.00
79) Terphenyl-d14	19.96	244	178422	16.15	ng	0.00
Target Compounds						
10) Phenol	7.20	94	20435	5.050	ng	95
20) 3+4-Methylphenols	8.77	107	37138	9.005	ng	91
50) Dimethylphthalate	14.04	163	142085	16.116	ng	98
84) Bis(2-ethylhexyl)phthalate	21.50	149	597241	68.517	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061220\
Data File : BG045752.D
Acq On : 12 Jun 2020 22:45
Operator : CG/JU
Sample : L2986-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
16-20-COMP

Quant Time: Jun 13 03:04:45 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 01 15:07:00 2020
Response via : Initial Calibration

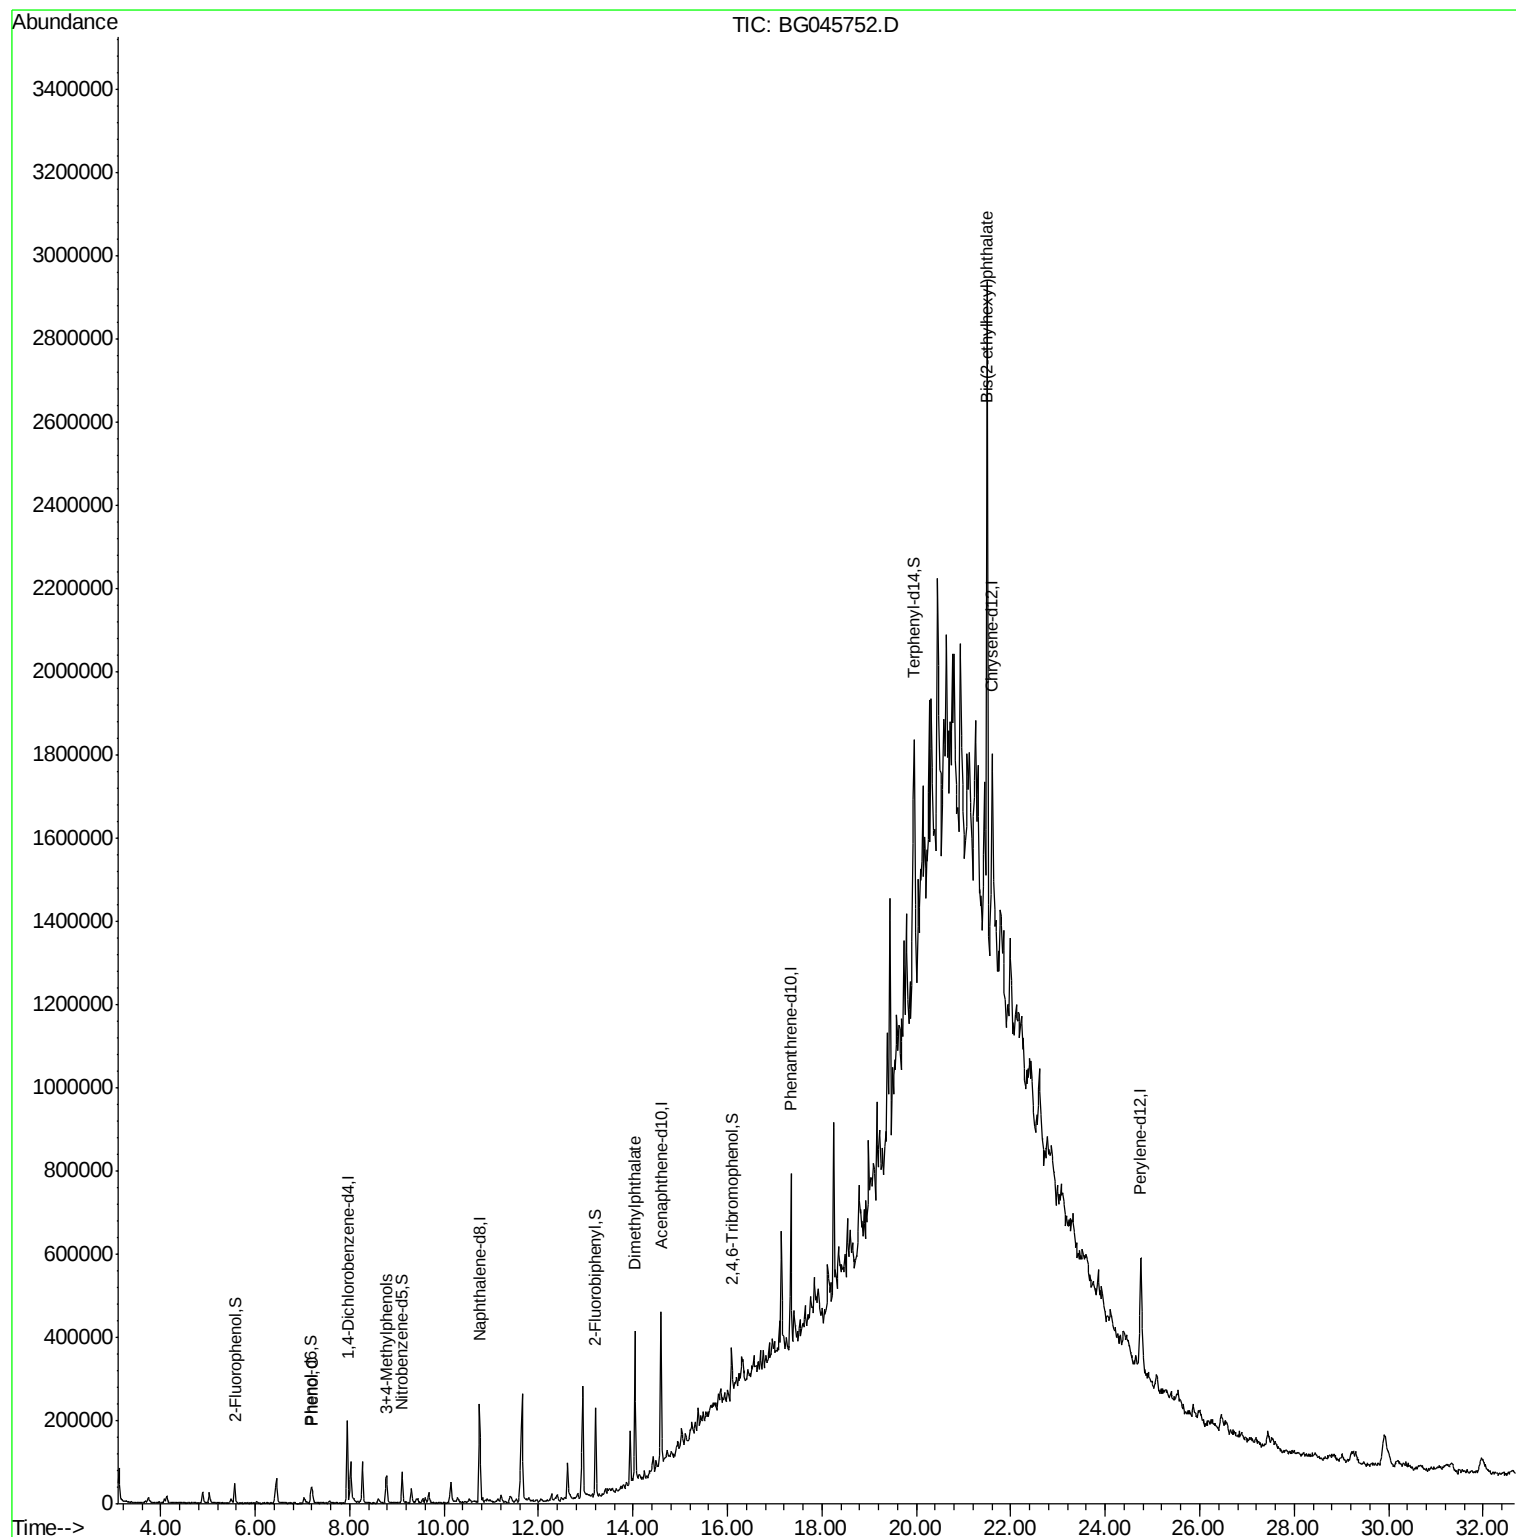

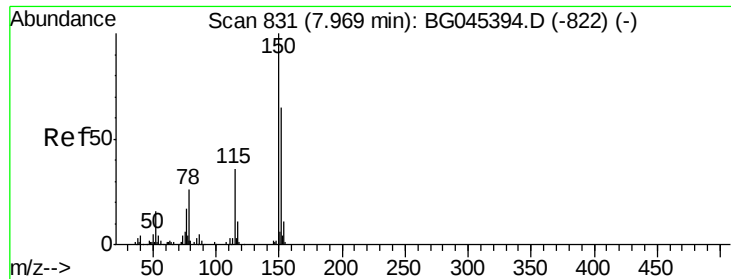


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.94 min Scan# 826
Delta R.T. -0.01 min
Lab File: BG045752.D
Acq: 12 Jun 2020 22:45

Instrument :
BNA_G
ClientSampleId :
16-20-COMP

Tot Ion	Ratio	Lower	Upper
152	100		
150	143.6	122.4	183.6
115	55.6	44.2	66.4

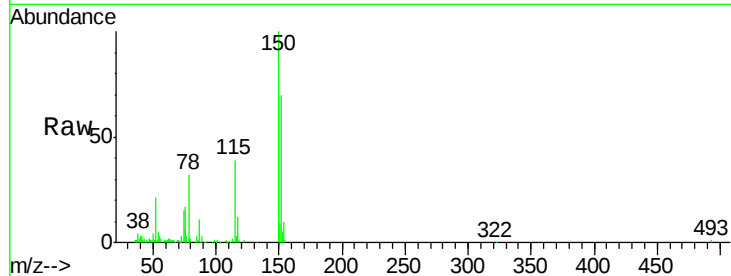


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

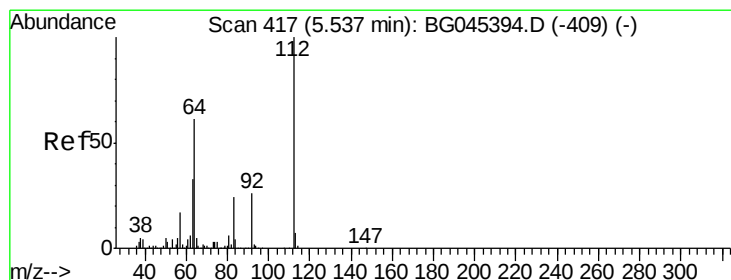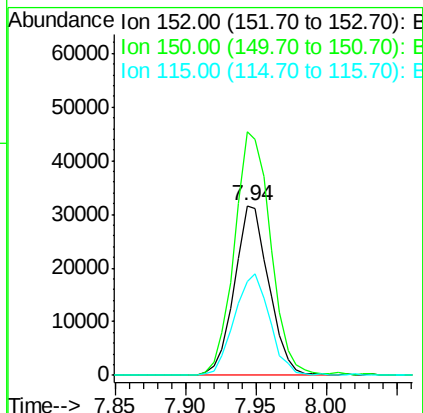



#5




2-Fluorophenol
Concen: 8.707 ng
RT: 5.56 min Scan# 421
Delta R.T. 0.03 min
Lab File: BG045752.D
Acq: 12 Jun 2020 22:45

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.8	48.6	72.8
63	31.7	26.5	39.7

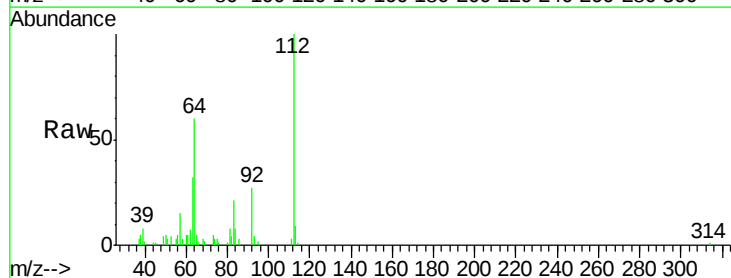

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

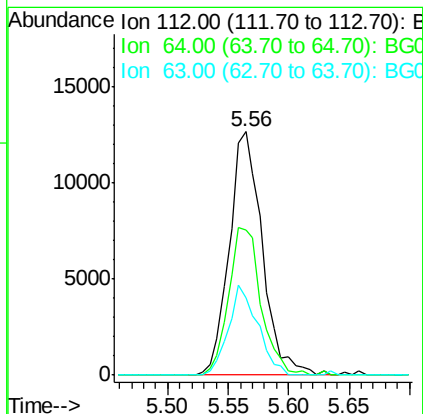

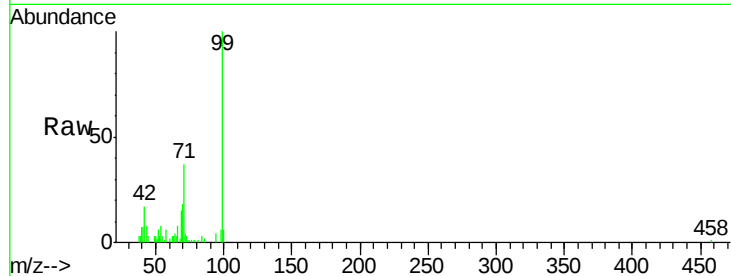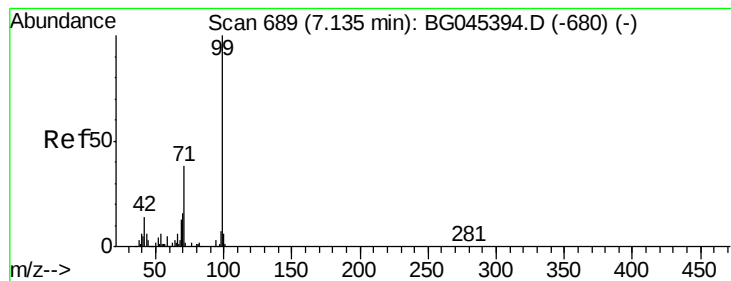

#7

Phenol-d6

Concen: 5.765 ng

RT: 7.18 min Scan# 696

Delta R.T. 0.03 min

Lab File: BG045752.D

Acq: 12 Jun 2020 22:45

Instrument :

BNA_G

ClientSampleId :

16-20-COMP





Tot Ion: 99 Resp: 22635

Ion Ratio Lower Upper

99 100

42 17.2 11.3 16.9#

71 37.1 30.8 46.2

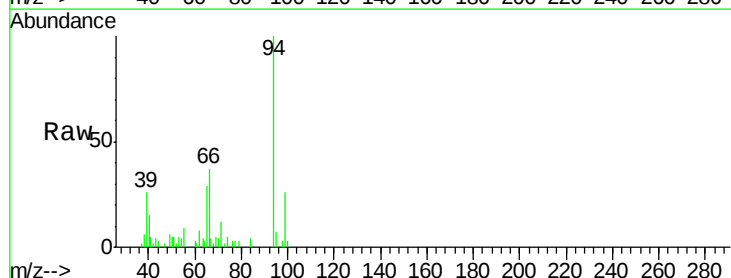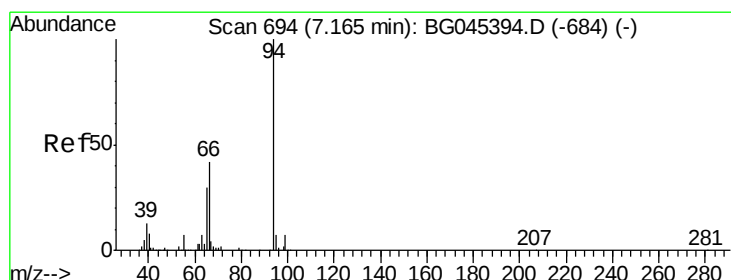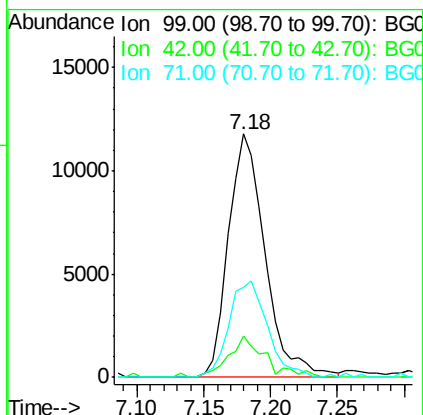

#10

Phenol

Concen: 5.050 ng

RT: 7.20 min Scan# 700

Delta R.T. 0.03 min

Lab File: BG045752.D

Acq: 12 Jun 2020 22:45


Tgt Ion: 94 Resp: 20435


Ion Ratio Lower Upper

94 100

65 28.6 9.8 49.8

66 37.4 22.0 62.0

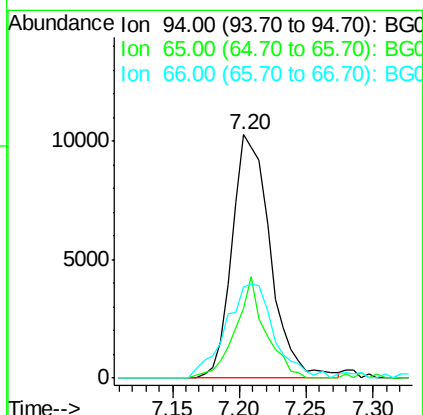



#20

3+4-Methylphenols

Concen: 9.005 ng

RT: 8.77 min Scan# 967

Delta R.T. 0.02 min

Lab File: BG045752.D

Acq: 12 Jun 2020 22:45

Instrument :

BNA_G

ClientSampleId :

16-20-COMP

Tot Ion:107 Resp: 37138


Ion Ratio Lower Upper

107 100

108 82.4 70.3 110.3

77 41.3 15.4 55.4

79 26.9 12.6 52.6



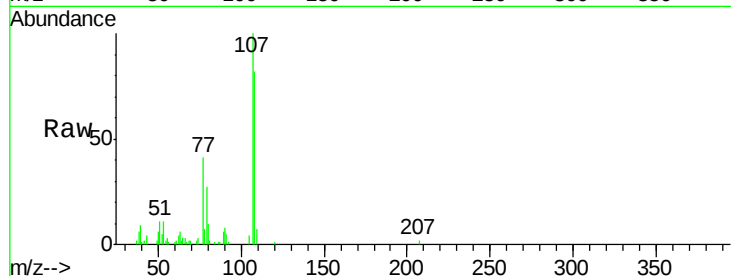


Abundance Ion 107.00 (106.70 to 107.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 77.00 (76.70 to 77.70): BGC

Ion 79.00 (78.70 to 79.70): BGC

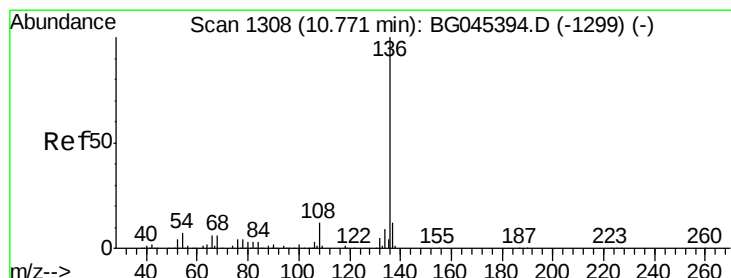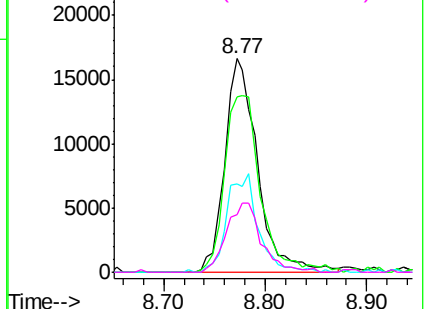

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.75 min Scan# 1304

Delta R.T. -0.01 min

Lab File: BG045752.D

Acq: 12 Jun 2020 22:45

Tgt Ion:136 Resp: 205221


Ion Ratio Lower Upper

136 100

137 10.5 9.4 14.2

54 5.8 5.8 8.6

68 4.6 4.5 6.7


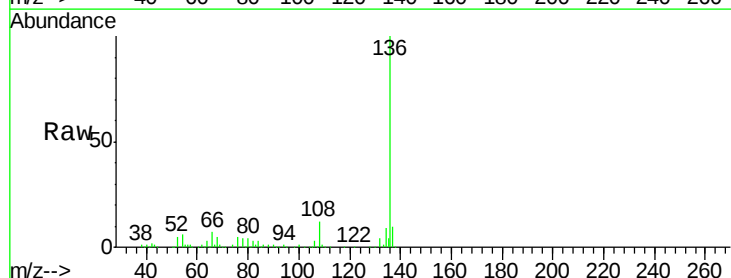



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC

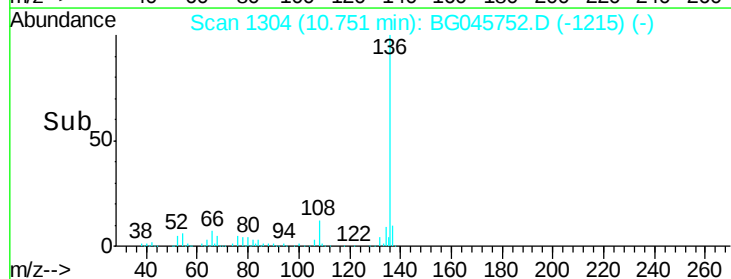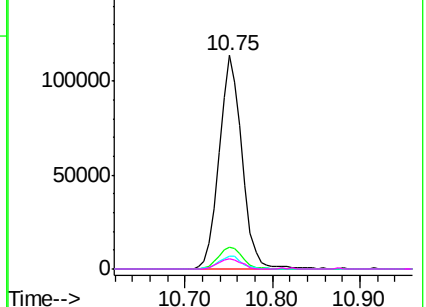


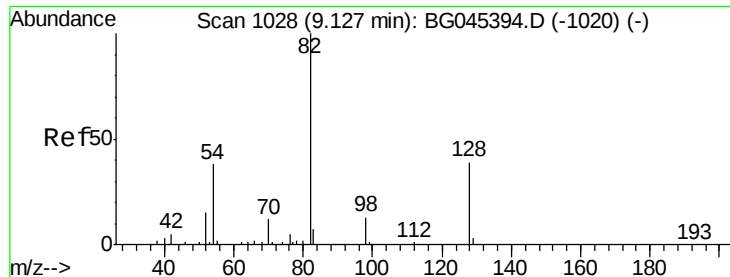




#23
 Nitrobenzene-d5
 Concen: 13.960 ng
 RT: 9.11 min Scan# 1025
 Delta R.T. -0.00 min
 Lab File: BG045752.D
 Acq: 12 Jun 2020 22:45

Instrument :
 BNA_G
 ClientSampleId :
 16-20-COMP

Tot Ion	82	Resp	52535
Ion Ratio	Lower	Upper	
82	100		
128	42.2	30.9	46.3
54	41.6	30.3	45.5

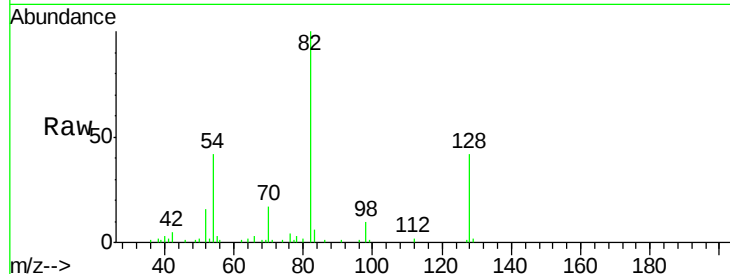


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

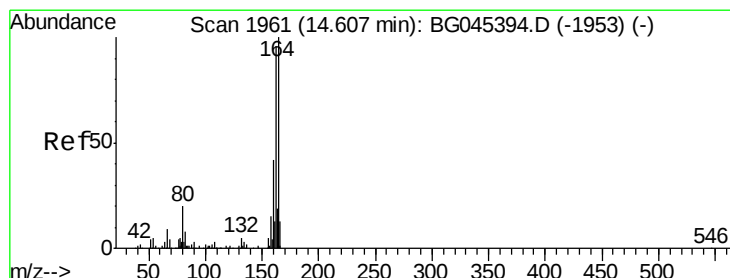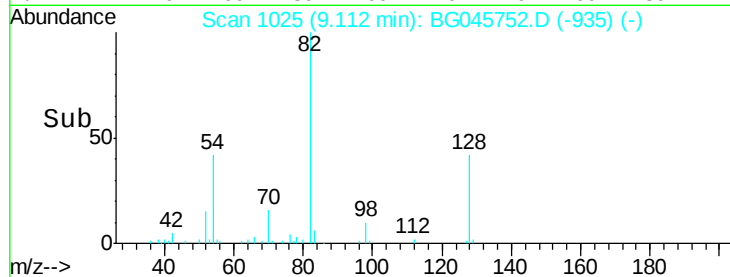
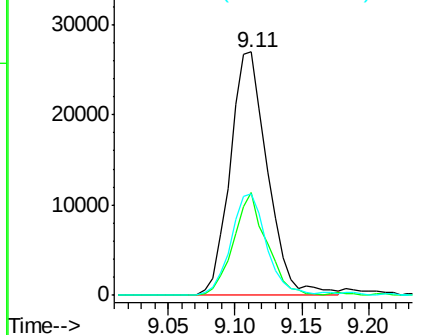



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.59 min Scan# 1958
 Delta R.T. -0.00 min
 Lab File: BG045752.D
 Acq: 12 Jun 2020 22:45

Tgt Ion	164	Resp	128523
Ion Ratio	Lower	Upper	
164	100		
162	94.0	76.9	115.3
160	41.9	33.8	50.8

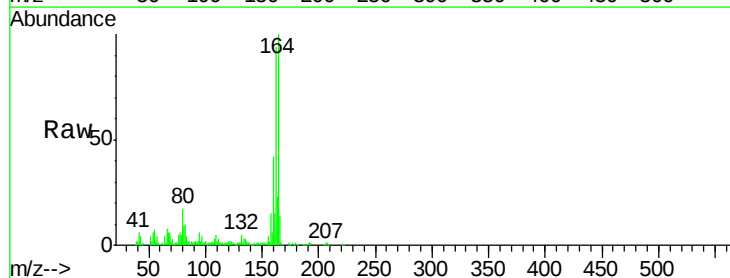

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC



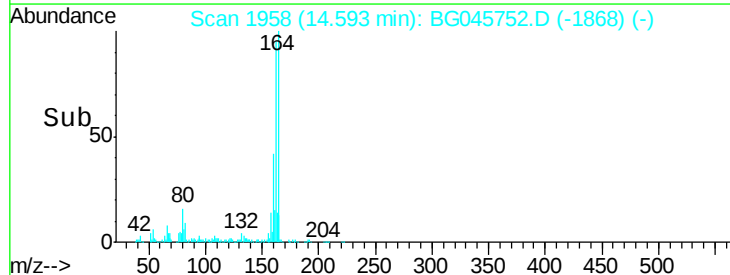
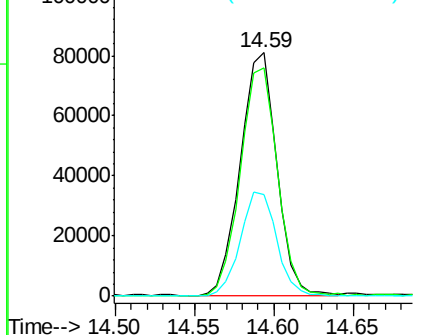


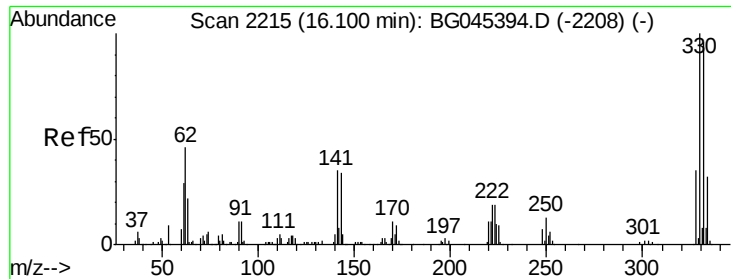

#42
 2,4,6-Tribromophenol
 Concen: 15.628 ng
 RT: 16.09 min Scan# 2213
 Delta R.T. -0.00 min
 Lab File: BG045752.D
 Acq: 12 Jun 2020 22:45




Instrument :
 BNA_G
 ClientSampleId :
 16-20-COMP


Tot Ion:330 Resp: 25687
 Ion Ratio Lower Upper
 330 100
 332 99.6 78.2 117.4
 141 38.4 28.2 42.4

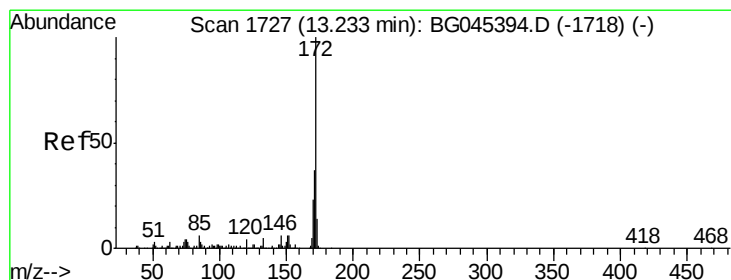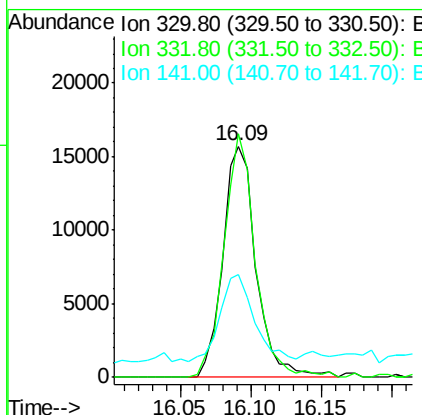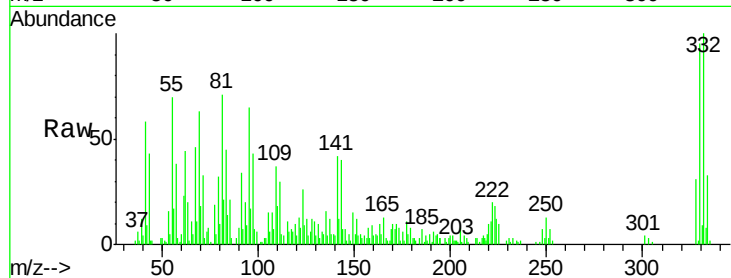

#45
 2-Fluorobiphenyl
 Concen: 15.531 ng
 RT: 13.21 min Scan# 1723
 Delta R.T. -0.00 min
 Lab File: BG045752.D
 Acq: 12 Jun 2020 22:45

Tgt Ion:172 Resp: 117680
 Ion Ratio Lower Upper
 172 100
 171 35.1 29.5 44.3
 170 23.1 18.5 27.7

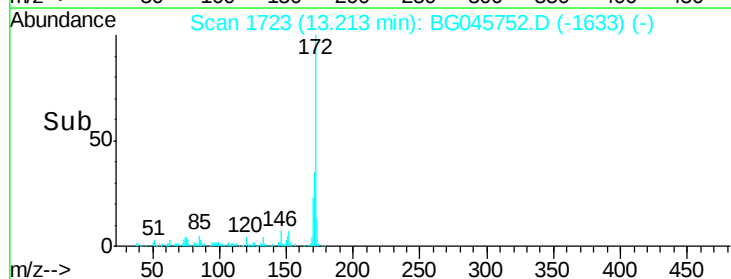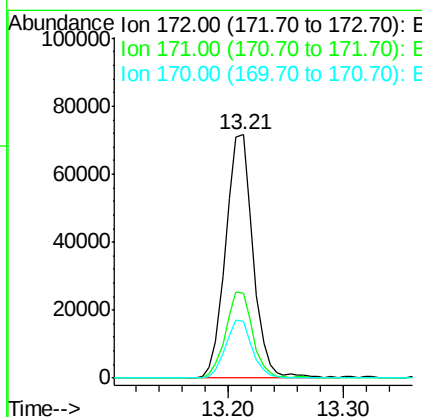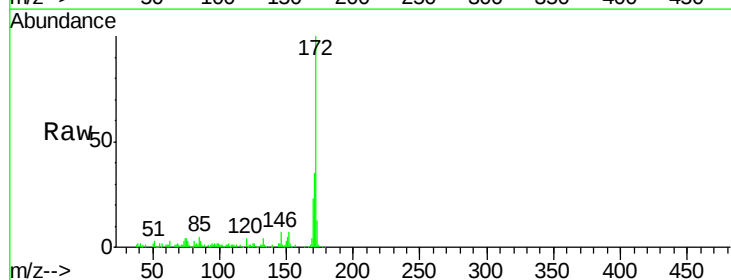



#50

Dimethylphthalate

Concen: 16.116 ng

RT: 14.04 min Scan# 1864

Delta R.T. -0.01 min

Lab File: BG045752.D

Acq: 12 Jun 2020 22:45

Instrument :

BNA_G

ClientSampleId :

16-20-COMP


Tot Ion:163 Resp: 142085

Ion Ratio Lower Upper

163 100

194 4.1 3.2 4.8




164 11.2 8.3 12.5

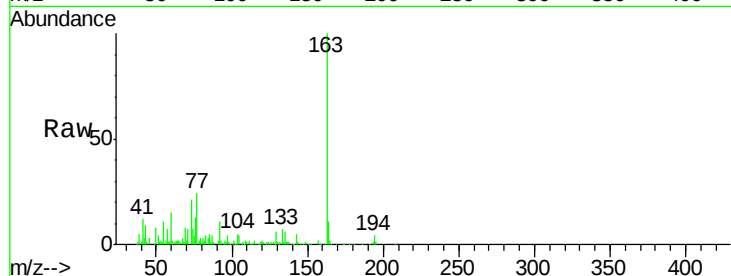

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

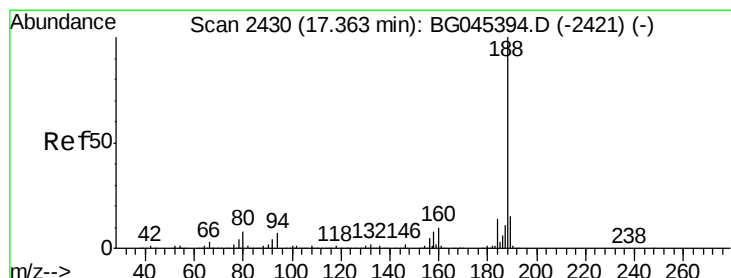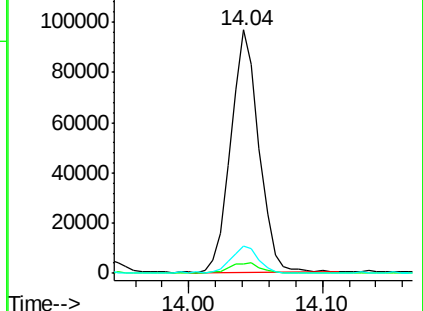

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.34 min Scan# 2426

Delta R.T. -0.00 min

Lab File: BG045752.D

Acq: 12 Jun 2020 22:45


Tgt Ion:188 Resp: 263944

Ion Ratio Lower Upper

188 100

94 7.6 5.5 8.3



80 8.2 6.6 10.0

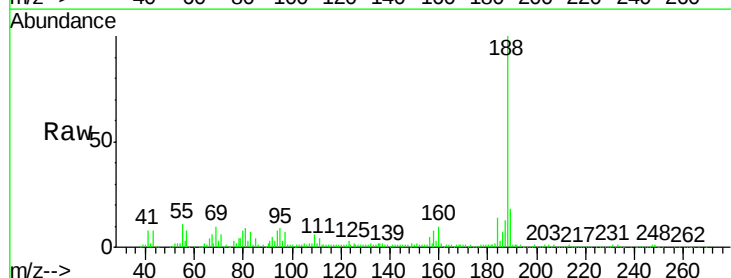


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC



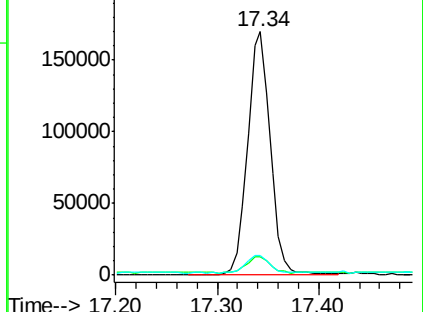



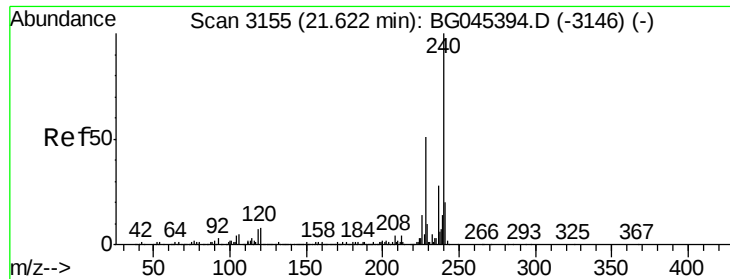

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.61 min Scan# 3152
Delta R.T. 0.00 min
Lab File: BG045752.D
Acq: 12 Jun 2020 22:45




Instrument :
BNA_G
ClientSampleId :
16-20-COMP


Tot Ion:240 Resp: 257717
Ion Ratio Lower Upper
240 100
120 6.1 6.1 9.1
236 25.8 22.3 33.5

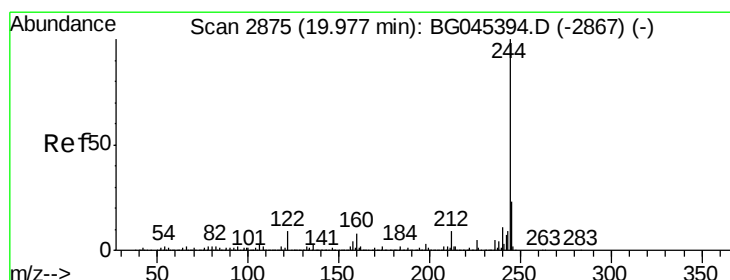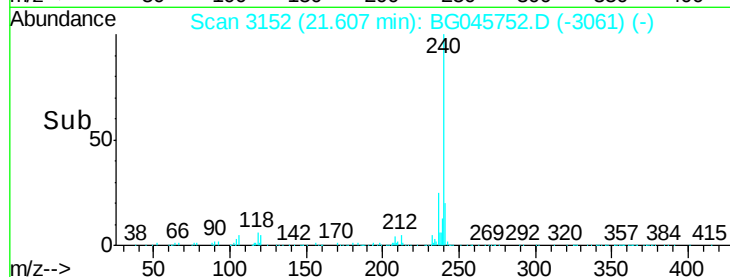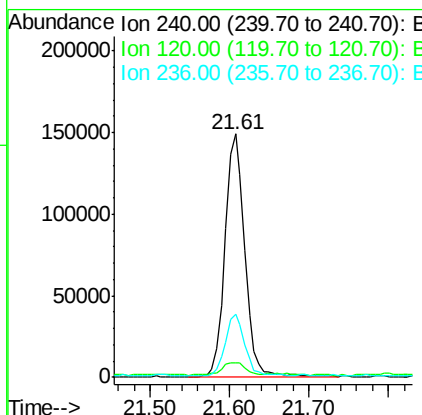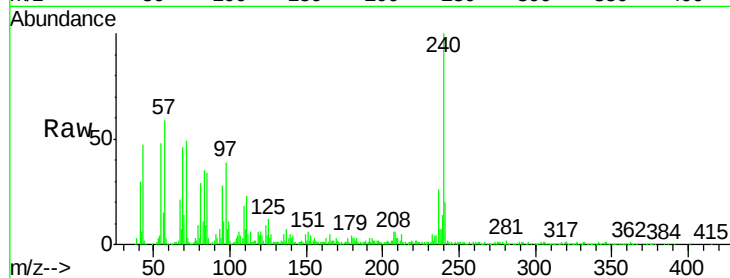

#79
Terphenyl-d14
Concen: 16.147 ng
RT: 19.96 min Scan# 2871
Delta R.T. -0.00 min
Lab File: BG045752.D
Acq: 12 Jun 2020 22:45

Tgt Ion:244 Resp: 178422
Ion Ratio Lower Upper
244 100
212 8.7 7.4 11.0
122 8.5 6.8 10.2


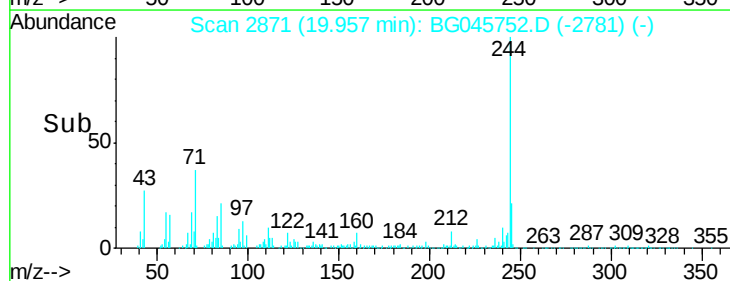
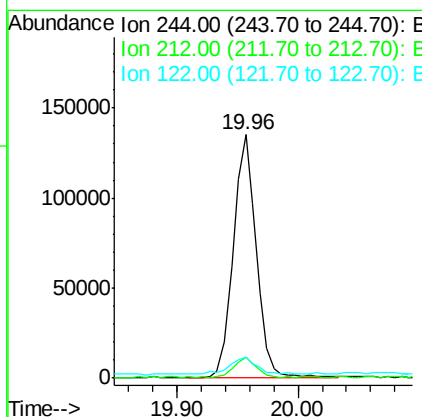
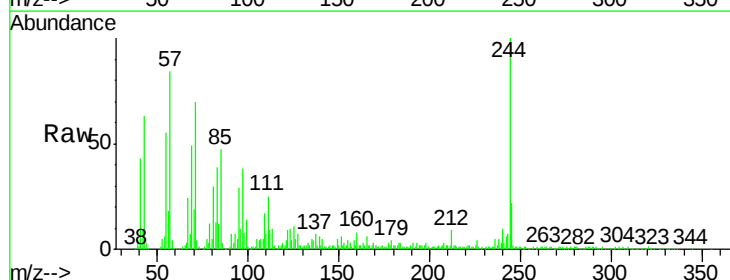


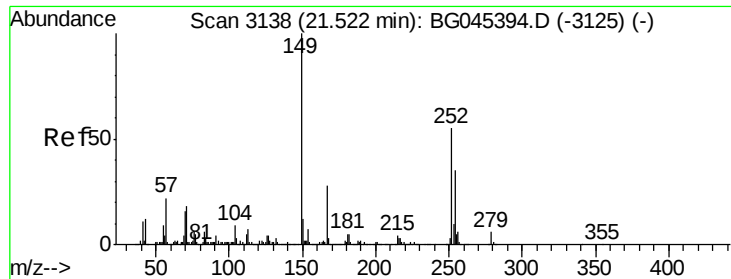

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 68.517 ng
 RT: 21.50 min Scan# 3133
 Delta R.T. -0.00 min
 Lab File: BG045752.D
 Acq: 12 Jun 2020 22:45

Instrument :
 BNA_G
 ClientSampleId :
 16-20-COMP

Tot Ion:149 Resp: 597241
 Ion Ratio Lower Upper
 149 100
 167 29.2 22.2 33.2
 279 5.8 4.7 7.1

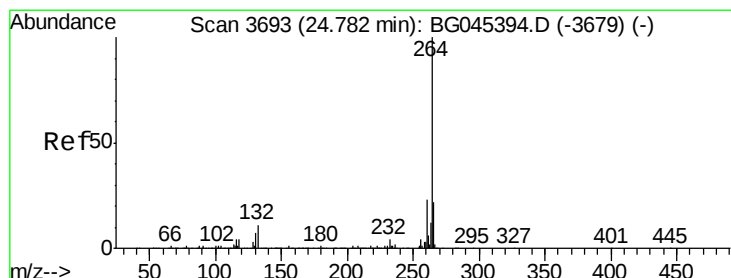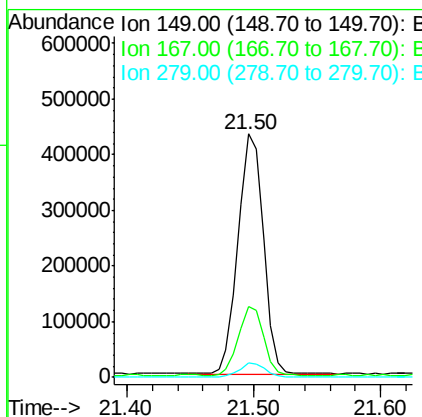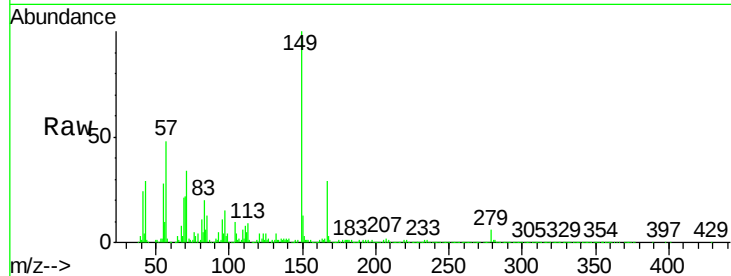

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.75 min Scan# 3687
 Delta R.T. -0.00 min
 Lab File: BG045752.D
 Acq: 12 Jun 2020 22:45

Tgt Ion:264 Resp: 282969
 Ion Ratio Lower Upper
 264 100
 260 22.3 18.2 27.4
 265 22.7 17.6 26.4

