


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061220\
 Data File : BG045739.D
 Acq On : 12 Jun 2020 14:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG051520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 01 15:07:00 2020

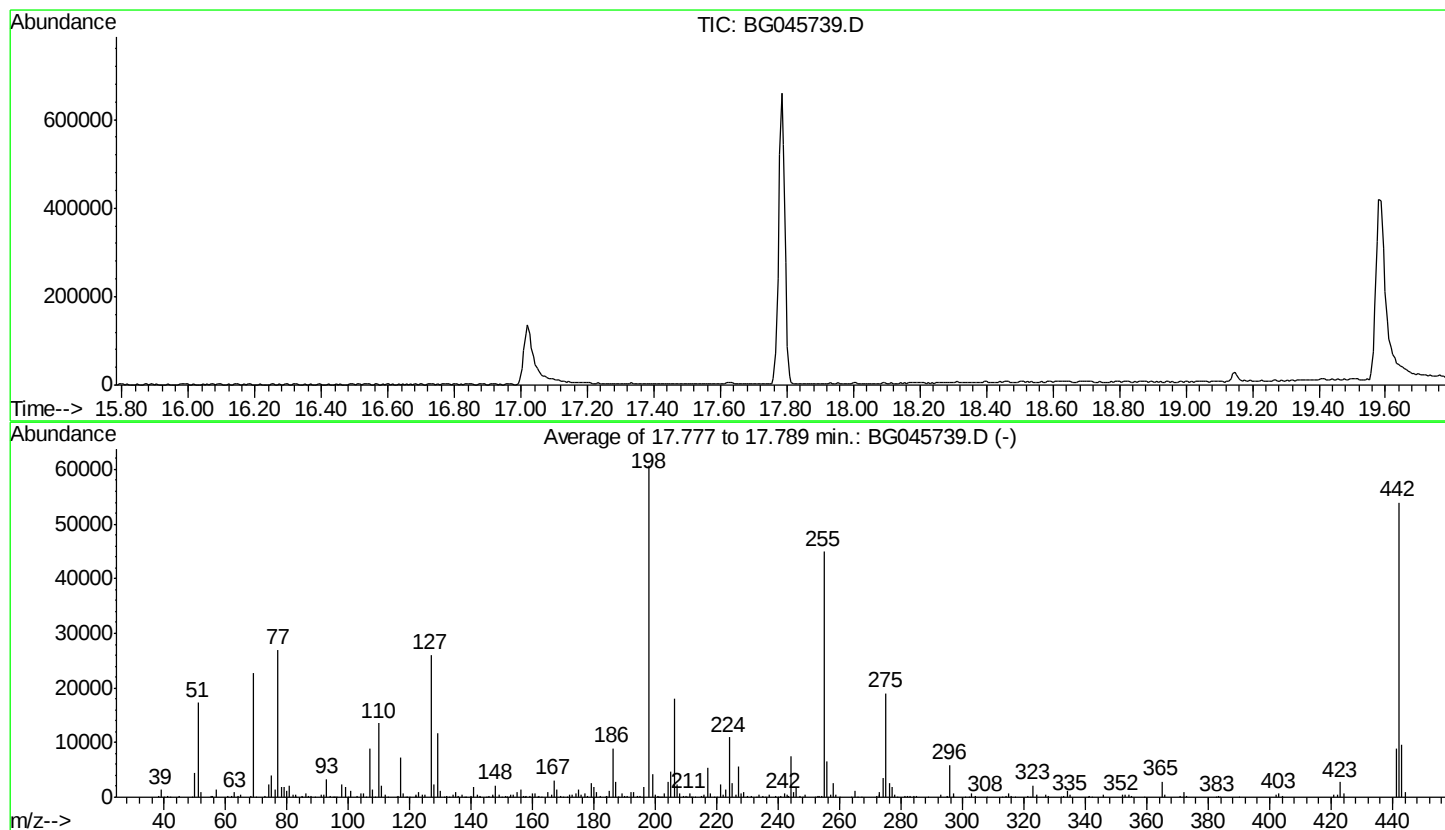

AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.5	17274	PASS
68	69	0.00	2	1.0	219	PASS
69	198	0.00	100	37.6	22818	PASS
70	69	0.00	2	0.3	71	PASS
127	198	10	80	42.9	26061	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	60693	PASS
199	198	5	9	6.9	4210	PASS
275	198	10	60	31.3	19017	PASS
365	198	1	100	4.7	2824	PASS
441	198	0.01	100	14.6	8861	PASS
442	198	50	100	88.9	53936	PASS
443	442	15	24	17.7	9550	PASS