


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061220\
 Data File : BG045757.D
 Acq On : 13 Jun 2020 3:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG051520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 01 15:07:00 2020

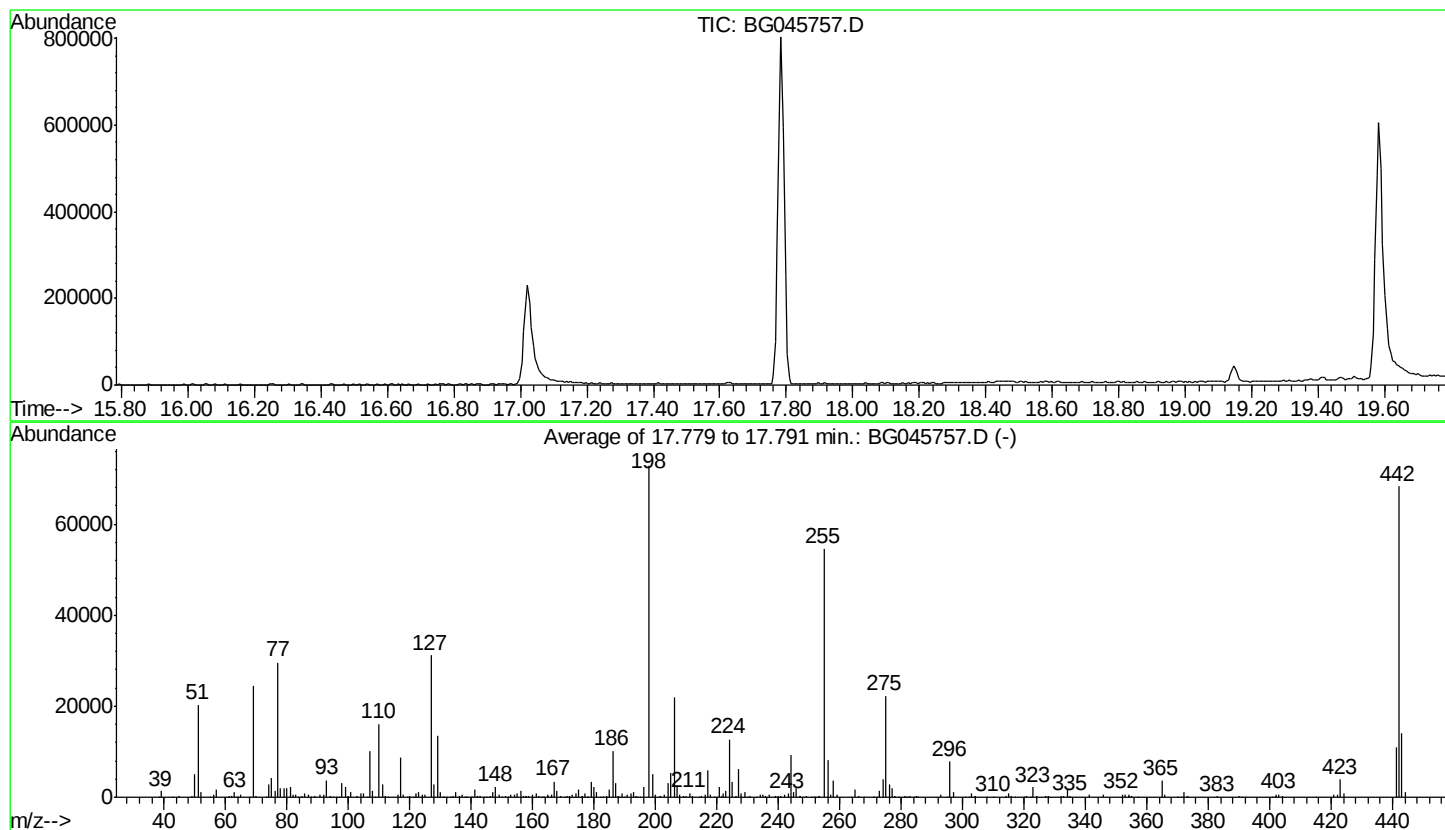

AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.9	20341	PASS
68	69	0.00	2	0.3	79	PASS
69	198	0.00	100	33.5	24434	PASS
70	69	0.00	2	0.8	187	PASS
127	198	10	80	42.7	31096	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	72848	PASS
199	198	5	9	6.8	4948	PASS
275	198	10	60	30.6	22317	PASS
365	198	1	100	4.9	3541	PASS
441	198	0.01	100	15.1	11035	PASS
442	198	50	100	93.8	68333	PASS
443	442	15	24	20.4	13940	PASS