
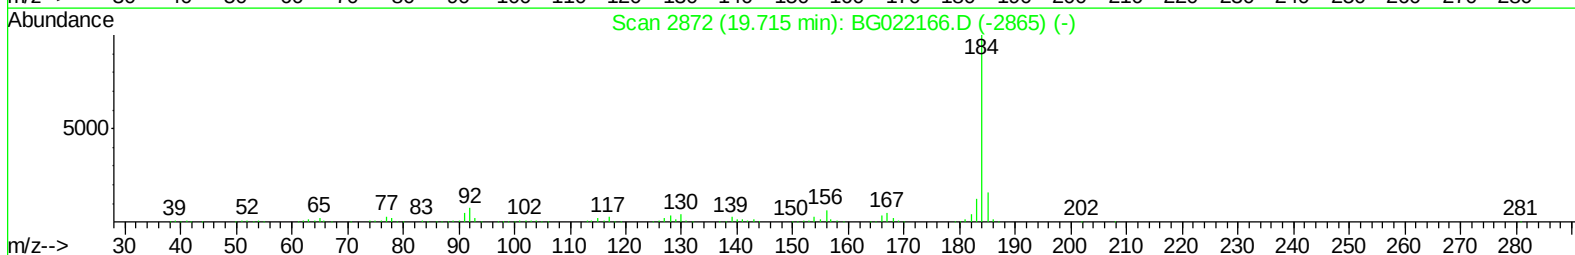
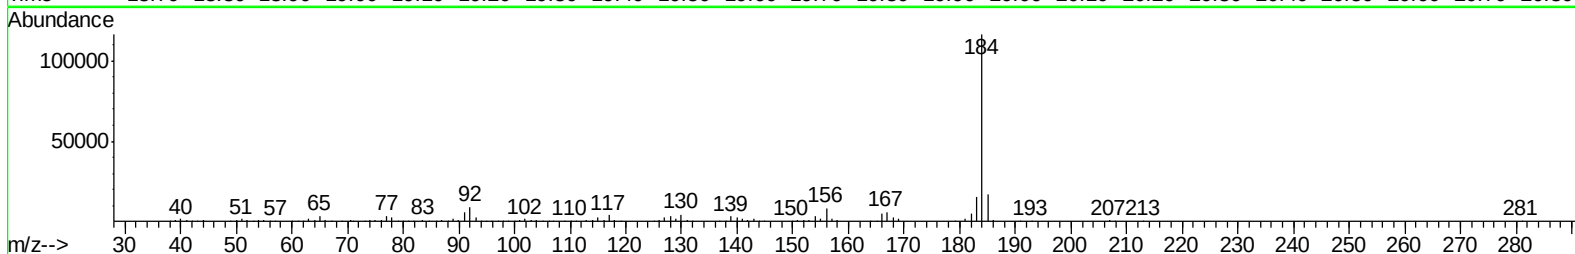


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061316\
Data File : BG022320.D
Acq On : 13 Jun 2016 10:08
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 03:57:10 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 17:40:23 2016
Response via : Initial Calibration

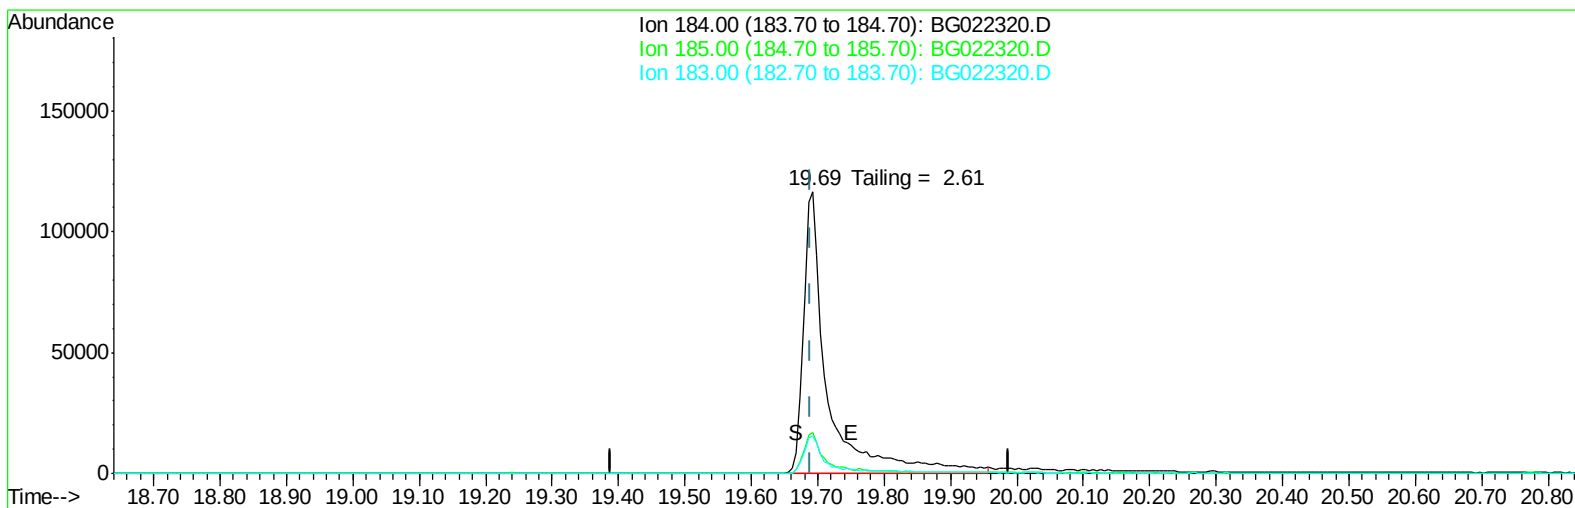

TIC: BG022320.D

(76) Benzidine




19.692min (+0.003) 0.00ng

response 269617

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.66
183.00	12.80	13.25
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061316\
Data File : BG022320.D
Acq On : 13 Jun 2016 10:08
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 03:57:10 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 17:40:23 2016
Response via : Initial Calibration

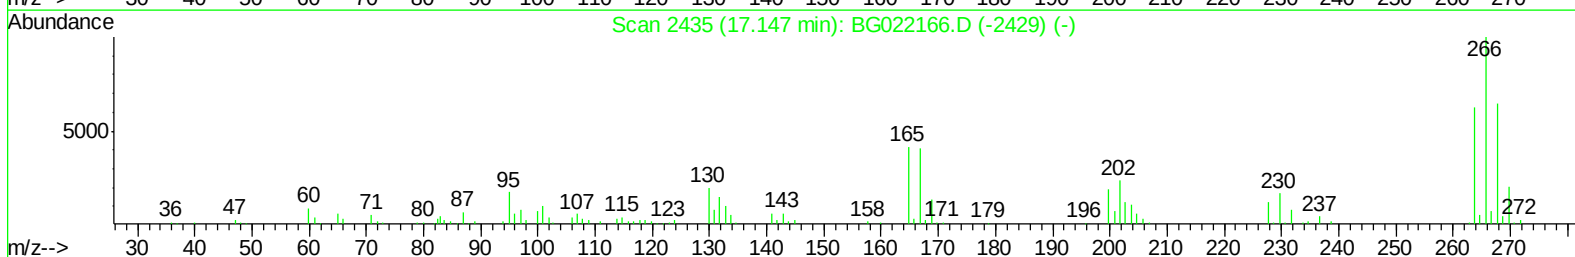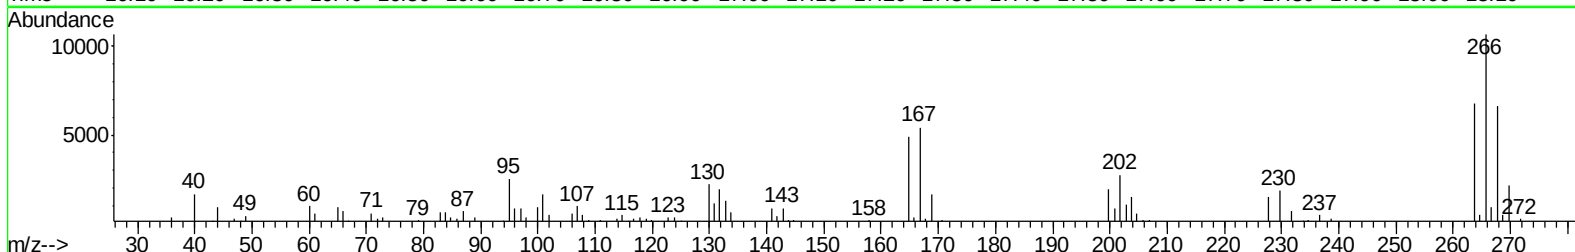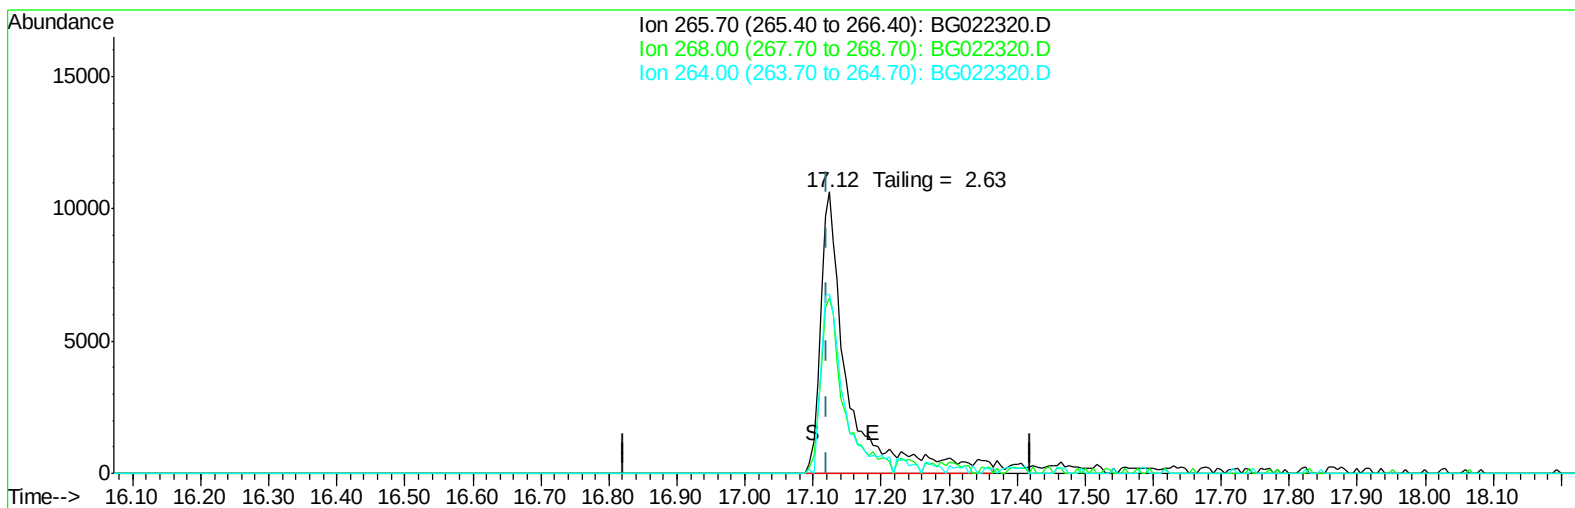

TIC: BG022320.D

(69) Pentachlorophenol (C)

17.124min (+0.003) 0.00ng

response 25711

Ion	Exp%	Act%
265.70	100	100
268.00	68.10	67.18
264.00	67.20	68.61
0.00	0.00	0.00