


Data Path : Z:\HPCHEM1\BNA G\DATA\BG061316\
 Data File : BG022320.D
 Acq On : 13 Jun 2016 10:08
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 13 17:40:23 2016

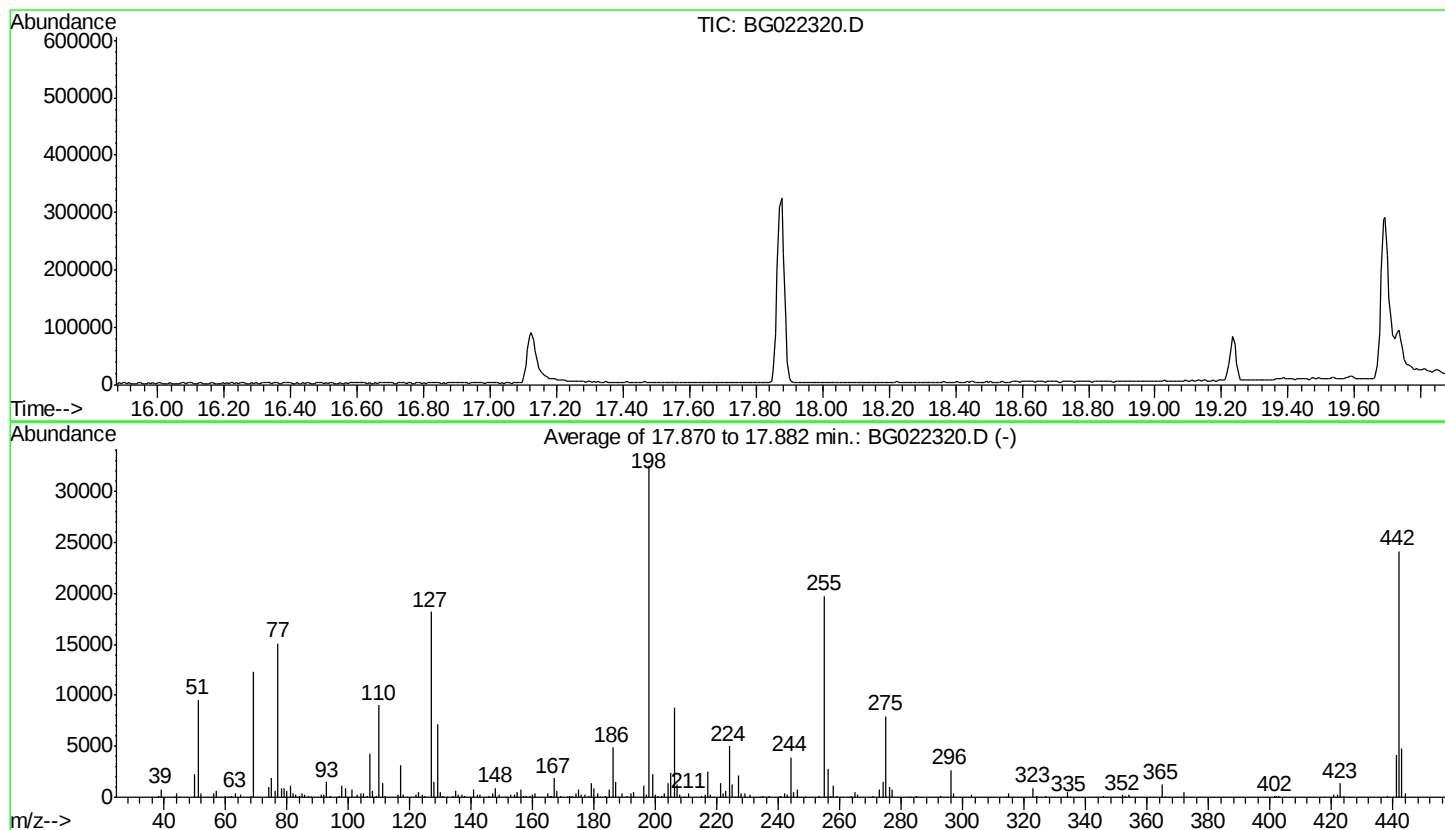

AutoFind: Scans 2558, 2559, 2560; Background Corrected with Scan 2551

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	9551	PASS
68	69	0.00	2	0.8	96	PASS
69	198	0.00	100	37.9	12338	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.9	18176	PASS
197	198	0.00	2	0.8	261	PASS
198	198	100	100	100.0	32541	PASS
199	198	5	9	7.0	2271	PASS
275	198	10	60	24.5	7965	PASS
365	198	1	100	3.7	1220	PASS
441	442	0.01	24	17.3	4168	PASS
442	198	50	100	74.2	24152	PASS
443	442	15	24	19.5	4716	PASS