

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061317\
 Data File : BG027410.D
 Acq On : 14 Jun 2017 7:36
 Operator : SJ/MA
 Sample : I3640-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 NF-DRUMS-DEBRIS-COMP

Quant Time: Jun 14 11:39:54 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 05 16:00:35 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.54	152	54472	20.00	ng	-0.04
21) Naphthalene-d8	11.36	136	238448	20.00	ng	-0.04
38) Acenaphthene-d10	15.12	164	141353	20.00	ng	-0.04
63) Phenanthrene-d10	17.87	188	338815	20.00	ng	-0.05
75) Chrysene-d12	22.25	240	408255	20.00	ng	-0.06
86) Perylene-d12	25.91	264	390090	20.00	ng	-0.11
System Monitoring Compounds						
5) 2-Fluorophenol	6.13	112	426439	119.46	ng	-0.02
7) Phenol-d6	7.68	99	521787	99.58	ng	-0.02
23) Nitrobenzene-d5	9.70	82	385273	101.61	ng	-0.04
41) 2,4,6-Tribromophenol	16.60	330	266215	143.02	ng	-0.04
44) 2-Fluorobiphenyl	13.74	172	821659	81.32	ng	-0.05
78) Terphenyl-d14	20.45	244	1455388	90.94	ng	-0.05
Target Compounds						Qvalue
31) Naphthalene	11.40	128	187768	14.41	ng	98
37) 2-Methylnaphthalene	12.97	142	117381	12.35	ng	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061317\
Data File : BG027410.D
Acq On : 14 Jun 2017 7:36
Operator : SJ/MA
Sample : I3640-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
NF-DRUMS-DEBRIS-COMP

Quant Time: Jun 14 11:39:54 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:00:35 2017
Response via : Initial Calibration

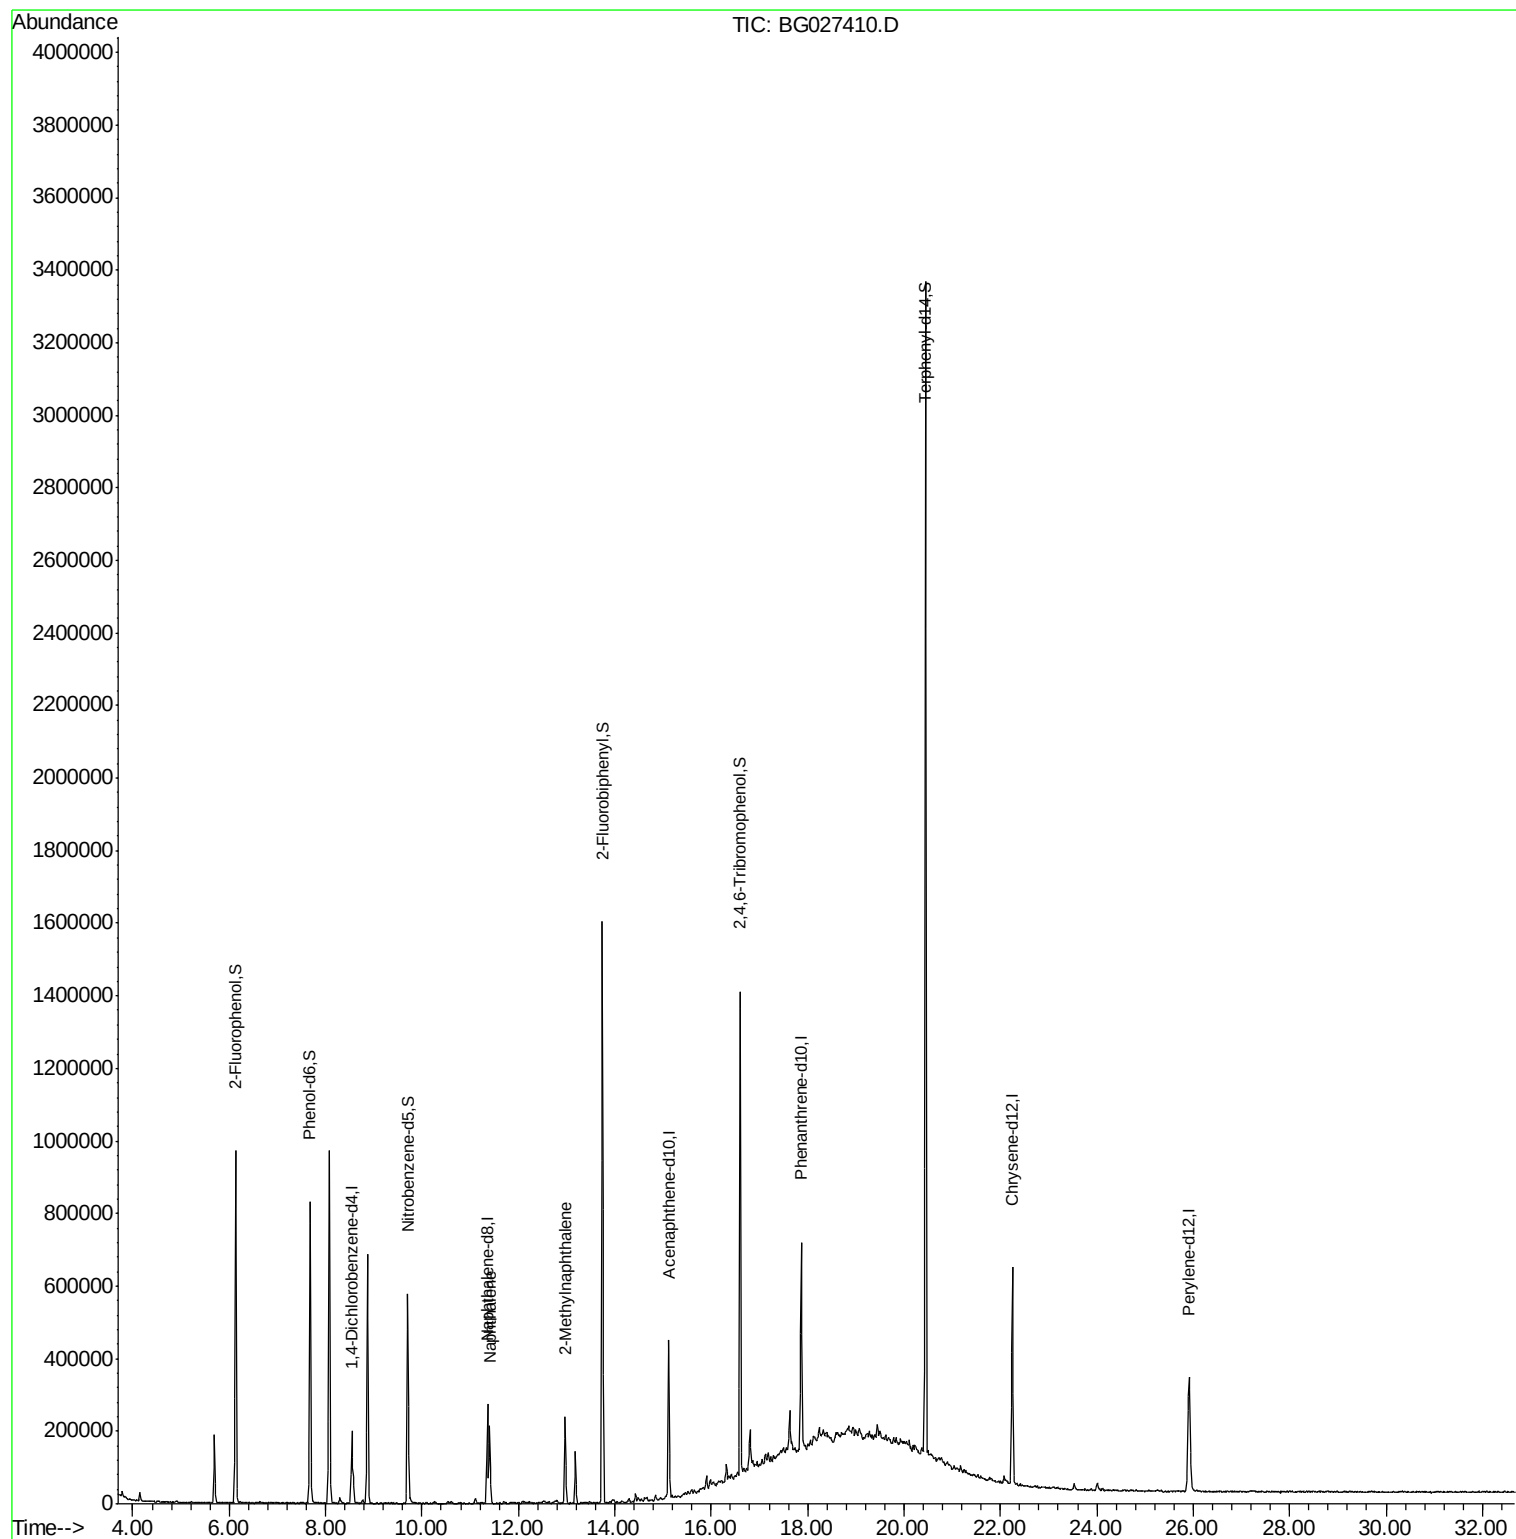



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.54 min Scan# 826

Delta R.T. -0.04 min

Lab File: BG027410.D

Acq: 14 Jun 2017 7:36

Instrument :

BNA_G

ClientSampleId :

NF-DRUMS-DEBRIS-COMP


Tot Ion:152 Resp: 54472

Ion Ratio Lower Upper

152 100

150 160.8 114.0 171.0




115 68.6 48.1 72.1

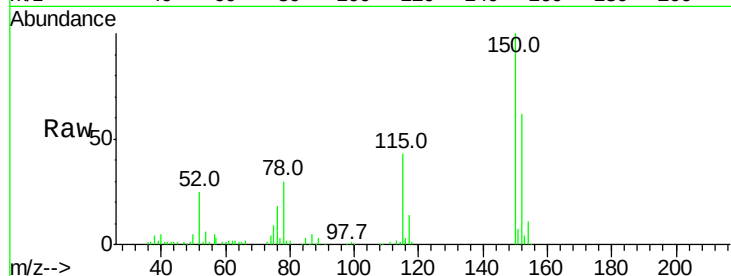

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

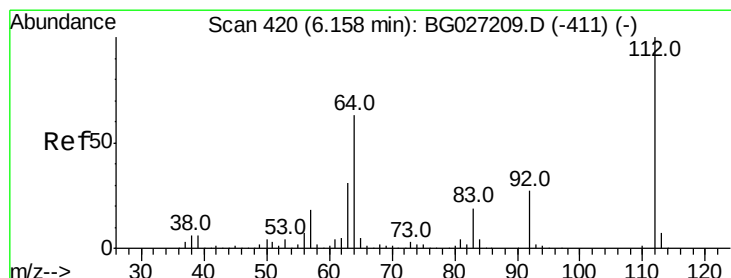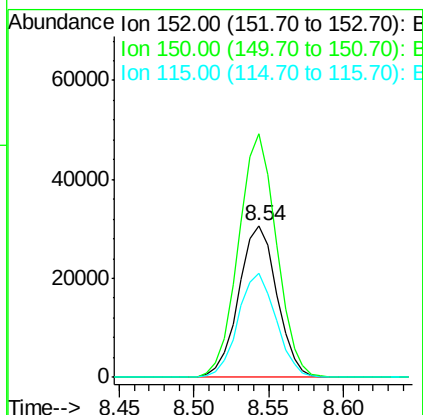

#5

2-Fluorophenol

Concen: 119.46 ng

RT: 6.13 min Scan# 416

Delta R.T. -0.02 min

Lab File: BG027410.D

Acq: 14 Jun 2017 7:36


Tgt Ion:112 Resp: 426439

Ion Ratio Lower Upper

112 100

64 73.1 61.8 92.6



63 36.5 37.2 55.8#

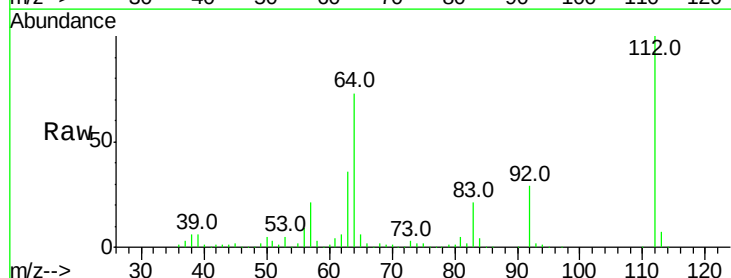


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

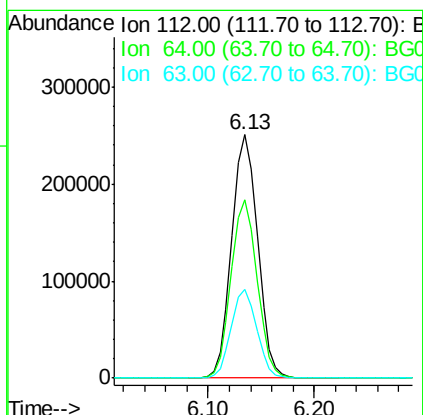

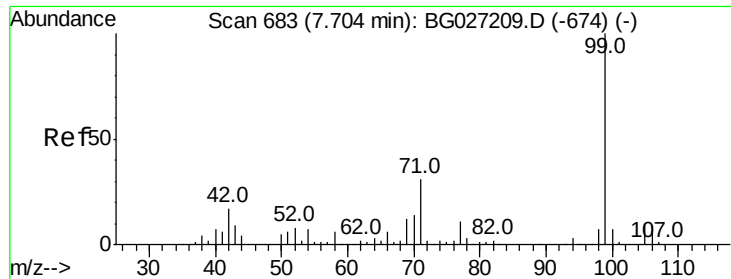

#7

Phenol-d6

Concen: 99.58 ng

RT: 7.68 min Scan# 679

Delta R.T. -0.02 min

Lab File: BG027410.D

Acq: 14 Jun 2017 7:36

Instrument :

BNA_G

ClientSampleId :

NF-DRUMS-DEBRIS-COMP


Tot Ion: 99 Resp: 521787

Ion Ratio Lower Upper




99 100

42 17.8 20.5 30.7#

71 33.1 37.6 56.4#

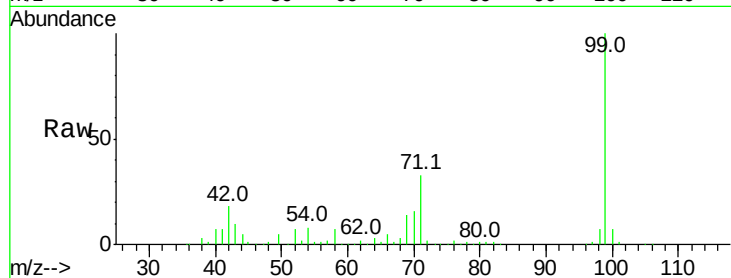

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

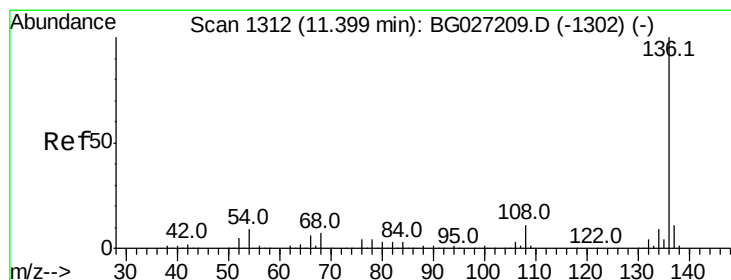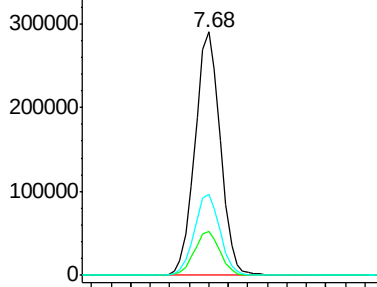

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 11.36 min Scan# 1305

Delta R.T. -0.04 min

Lab File: BG027410.D

Acq: 14 Jun 2017 7:36

Tgt Ion: 136 Resp: 238448


Ion Ratio Lower Upper

136 100



137 11.3 8.9 13.3


54 11.2 9.3 13.9

68 8.5 5.1 7.7#

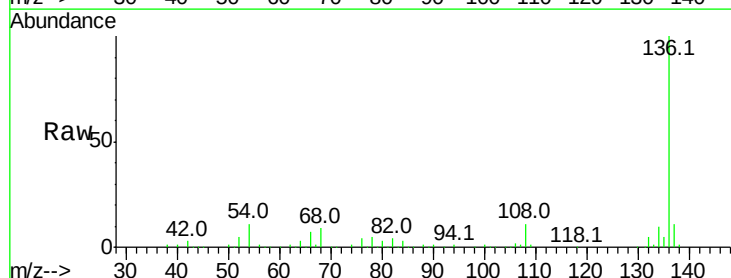

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




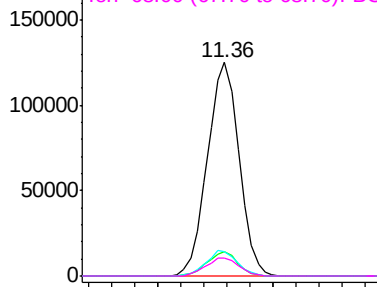


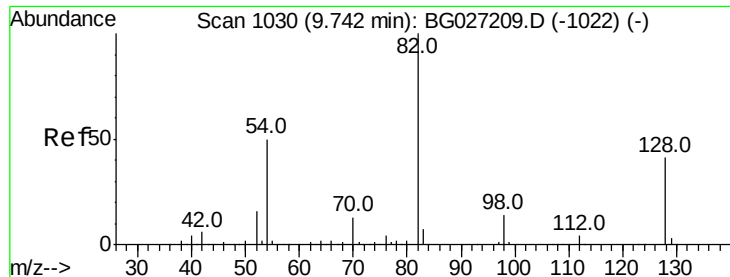

#23
 Nitrobenzene-d5
 Concen: 101.61 ng
 RT: 9.70 min Scan# 1023
 Delta R.T. -0.04 min
 Lab File: BG027410.D
 Acq: 14 Jun 2017 7:36




Instrument :
 BNA_G
 ClientSampleId :
 NF-DRUMS-DEBRIS-COMP


Tot Ion: 82 Resp: 385273
 Ion Ratio Lower Upper
 82 100
 128 38.9 26.4 39.6
 54 54.7 49.4 74.2

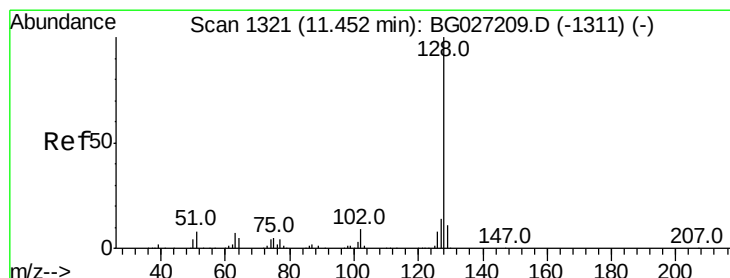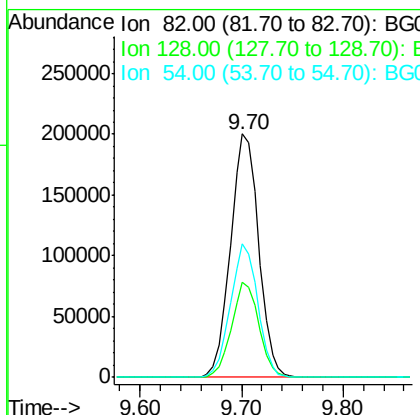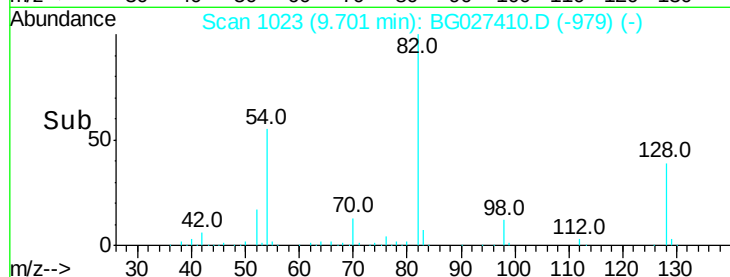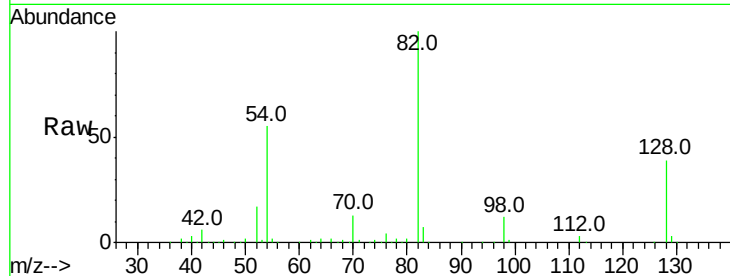

#31
 Naphthalene
 Concen: 14.41 ng
 RT: 11.40 min Scan# 1313
 Delta R.T. -0.05 min
 Lab File: BG027410.D
 Acq: 14 Jun 2017 7:36

Tgt Ion: 128 Resp: 187768
 Ion Ratio Lower Upper
 128 100
 129 10.9 9.3 13.9
 127 13.4 11.4 17.0


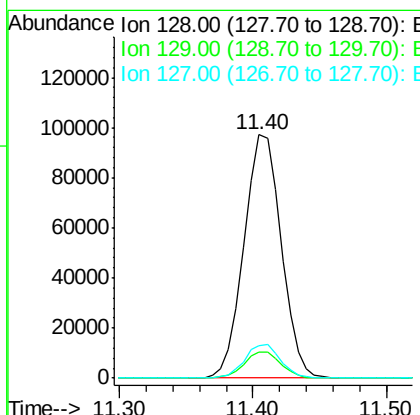
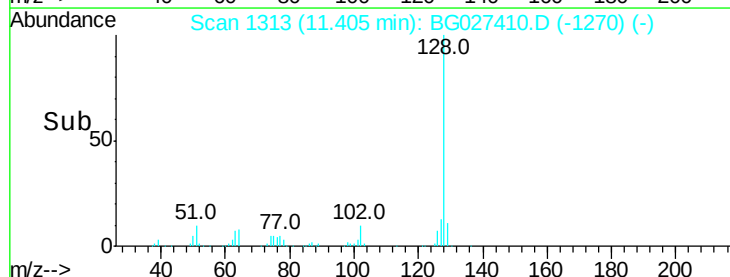
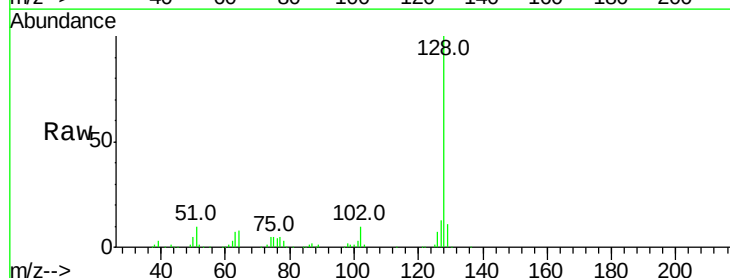


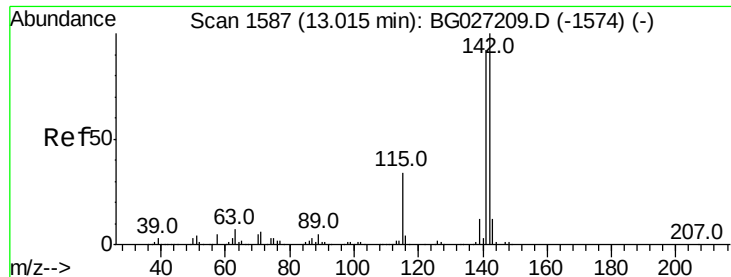

#37
2-Methylnaphthalene
Concen: 12.35 ng
RT: 12.97 min Scan# 1580
Delta R.T. -0.04 min
Lab File: BG027410.D
Acq: 14 Jun 2017 7:36




Instrument :
BNA_G
ClientSampleId :
NF-DRUMS-DEBRIS-COMP


Tot Ion	Ratio	Lower	Upper
142	100		
141	92.4	70.4	105.6
115	37.4	35.5	53.3

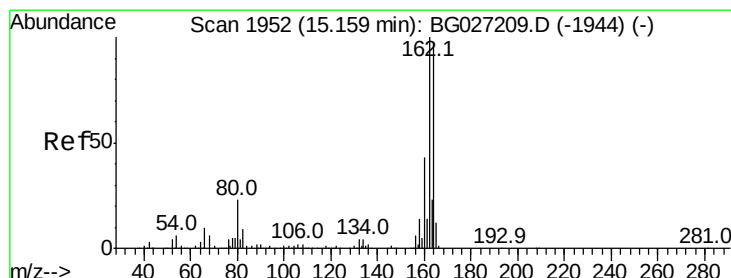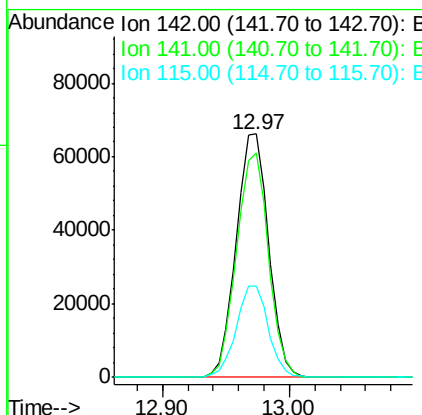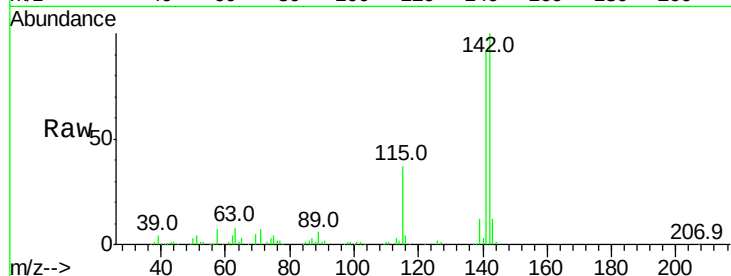

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 15.12 min Scan# 1945
Delta R.T. -0.04 min
Lab File: BG027410.D
Acq: 14 Jun 2017 7:36

Tgt Ion	Ratio	Lower	Upper
164	100		
162	104.6	85.1	127.7
160	45.5	34.7	52.1

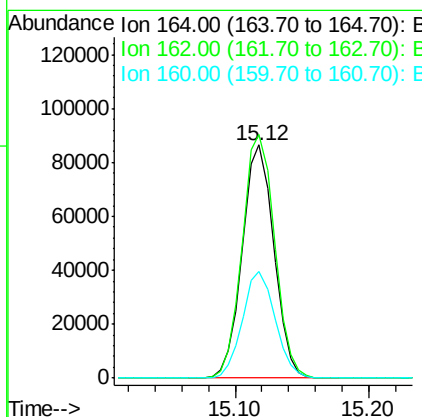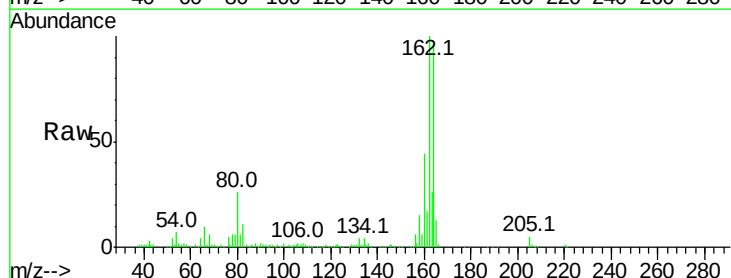


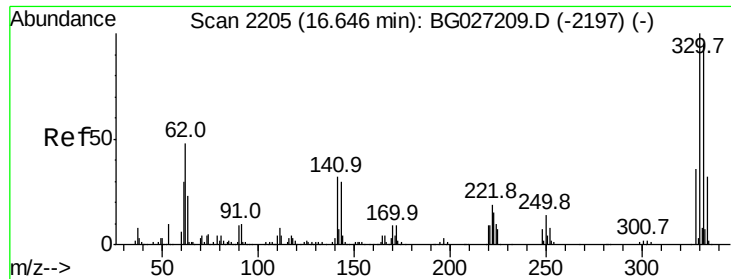




#41
 2,4,6-Tribromophenol
 Concen: 143.02 ng
 RT: 16.60 min Scan# 2198
 Delta R.T. -0.04 min
 Lab File: BG027410.D
 Acq: 14 Jun 2017 7:36

Instrument :
 BNA_G
 ClientSampleId :
 NF-DRUMS-DEBRIS-COMP

Tot Ion:330 Resp: 266215
 Ion Ratio Lower Upper
 330 100
 332 97.2 77.3 115.9
 141 33.8 32.1 48.1

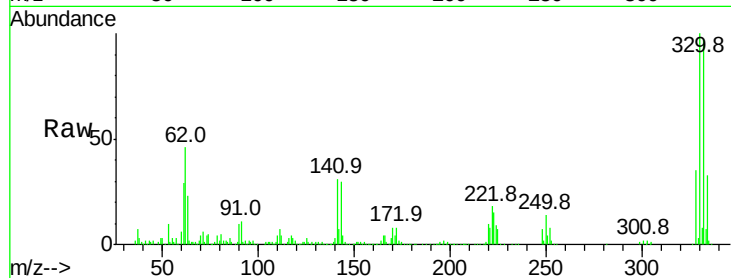


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

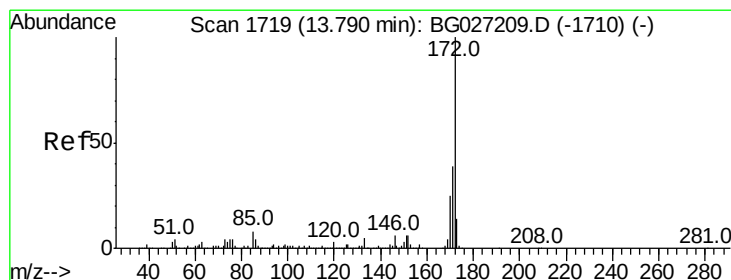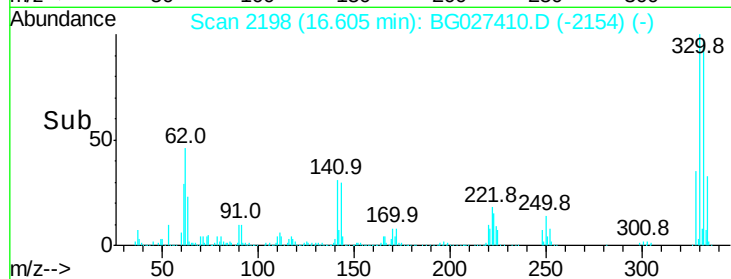
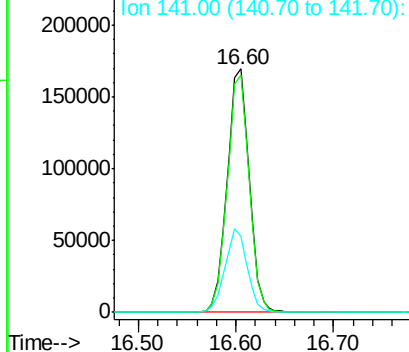



#44
 2-Fluorobiphenyl
 Concen: 81.32 ng
 RT: 13.74 min Scan# 1711
 Delta R.T. -0.05 min
 Lab File: BG027410.D
 Acq: 14 Jun 2017 7:36

Tgt Ion:172 Resp: 821659
 Ion Ratio Lower Upper
 172 100
 171 37.5 32.2 48.2
 170 24.7 21.8 32.6

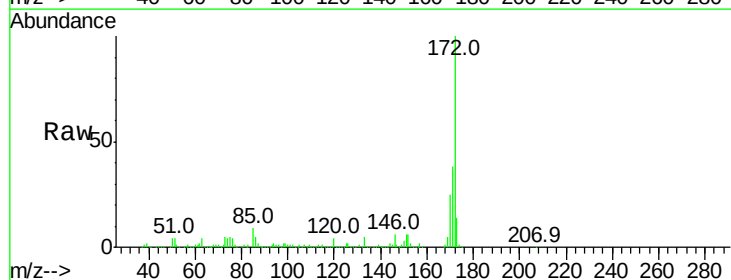

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

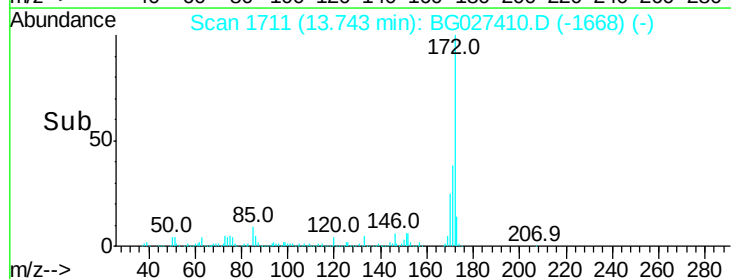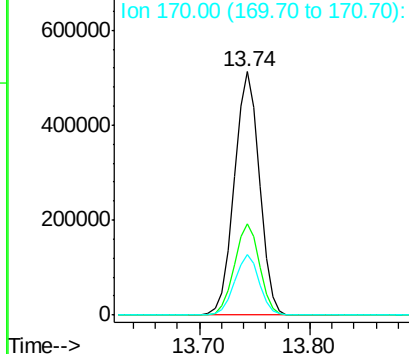


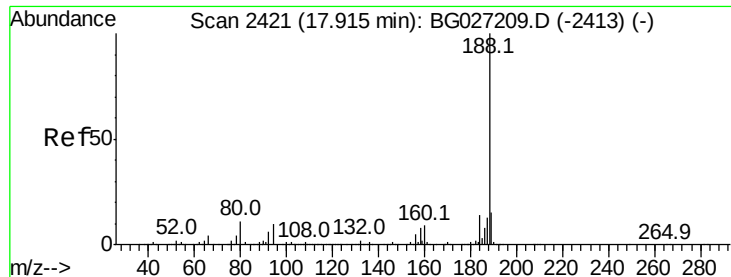




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.87 min Scan# 2413
Delta R.T. -0.05 min
Lab File: BG027410.D
Acq: 14 Jun 2017 7:36

Instrument :
BNA_G
ClientSampleId :
NF-DRUMS-DEBRIS-COMP

Tot Ion:188 Resp: 338815
Ion Ratio Lower Upper
188 100
94 11.3 5.8 8.8#
80 13.4 7.5 11.3#

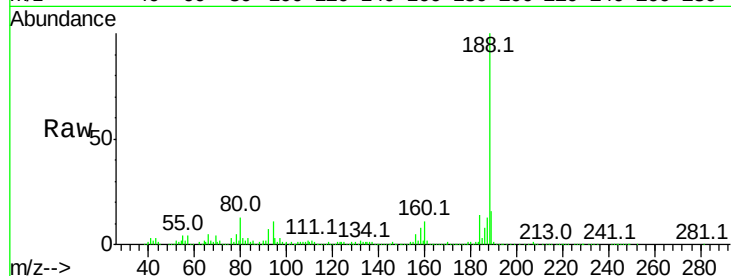


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

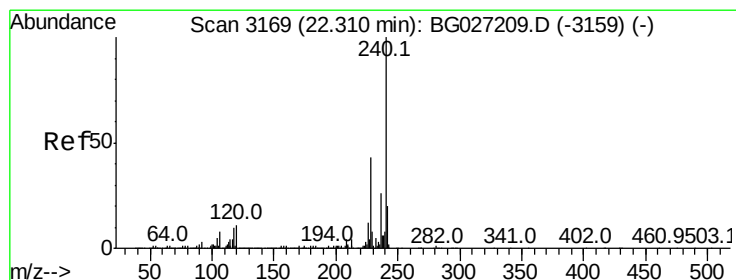
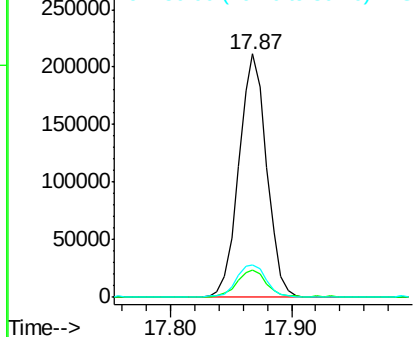



#75
Chrysene-d12
Concen: 20.00 ng
RT: 22.25 min Scan# 3158
Delta R.T. -0.06 min
Lab File: BG027410.D
Acq: 14 Jun 2017 7:36

Tgt Ion:240 Resp: 408255
Ion Ratio Lower Upper
240 100
120 11.8 5.7 8.5#
236 26.1 22.2 33.4

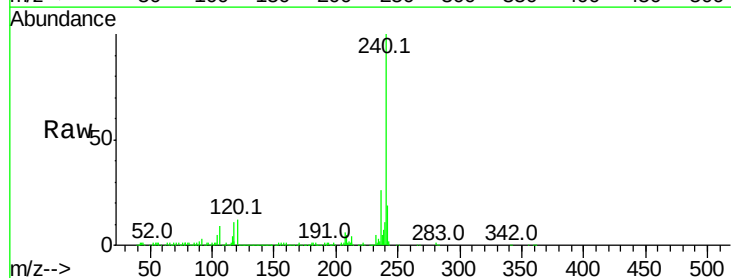

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

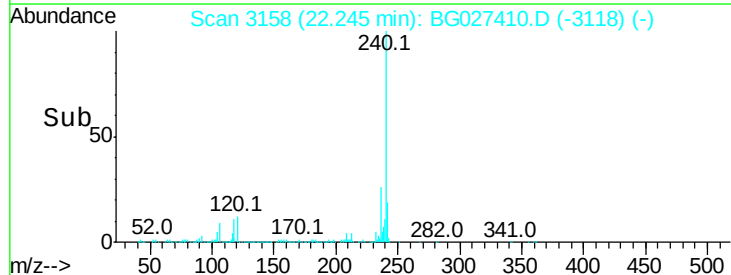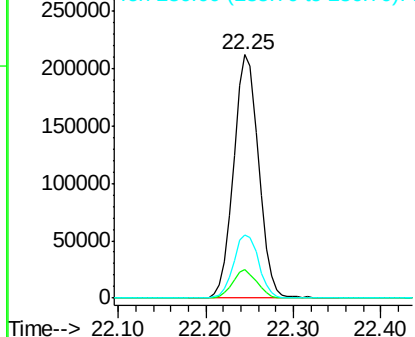

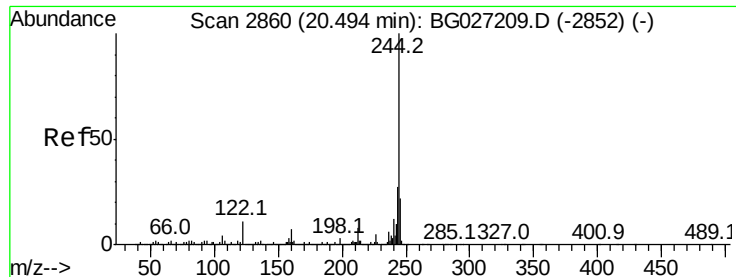

#78

Terphenyl-d14

Concen: 90.94 ng

RT: 20.45 min Scan# 2852

Delta R.T. -0.05 min

Lab File: BG027410.D

Acq: 14 Jun 2017 7:36

Instrument :

BNA_G

ClientSampleId :

NF-DRUMS-DEBRIS-COMP


Tot Ion:244 Resp: 1455388

Ion Ratio Lower Upper

244 100

212 7.8 10.0 15.0#




122 11.8 8.6 12.8

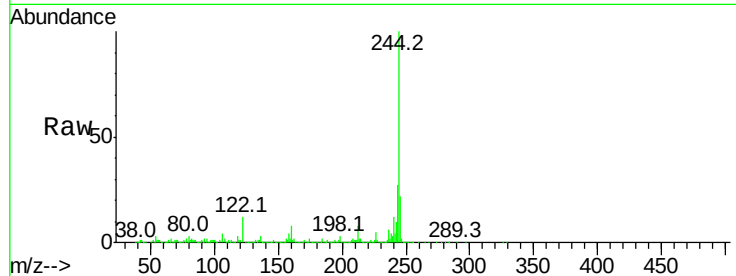

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

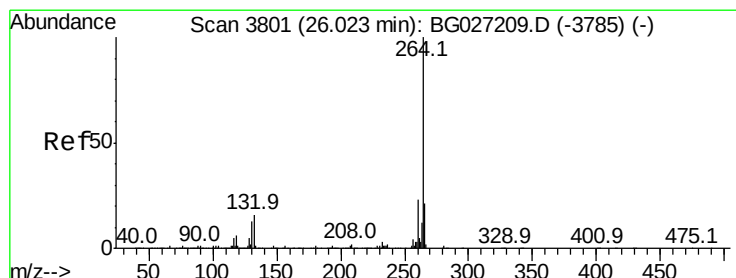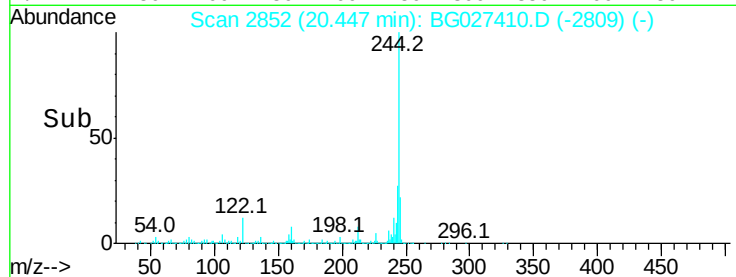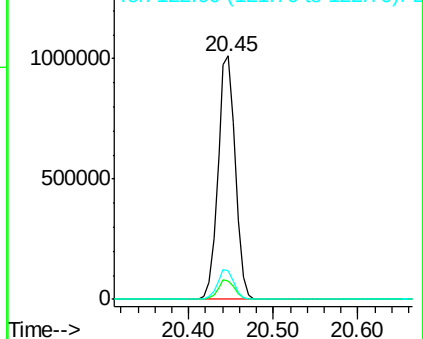

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.91 min Scan# 3782

Delta R.T. -0.11 min

Lab File: BG027410.D

Acq: 14 Jun 2017 7:36


Tgt Ion:264 Resp: 390090

Ion Ratio Lower Upper

264 100

260 23.3 21.8 32.8

265 21.2 18.2 27.4

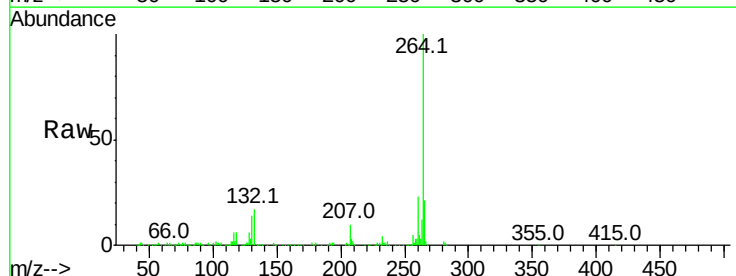

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

