


Data Path : Z:\HPCHEM1\BNA G\Data\BG061317\
 Data File : BG027407.D
 Acq On : 14 Jun 2017 4:55
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 05 16:00:35 2017

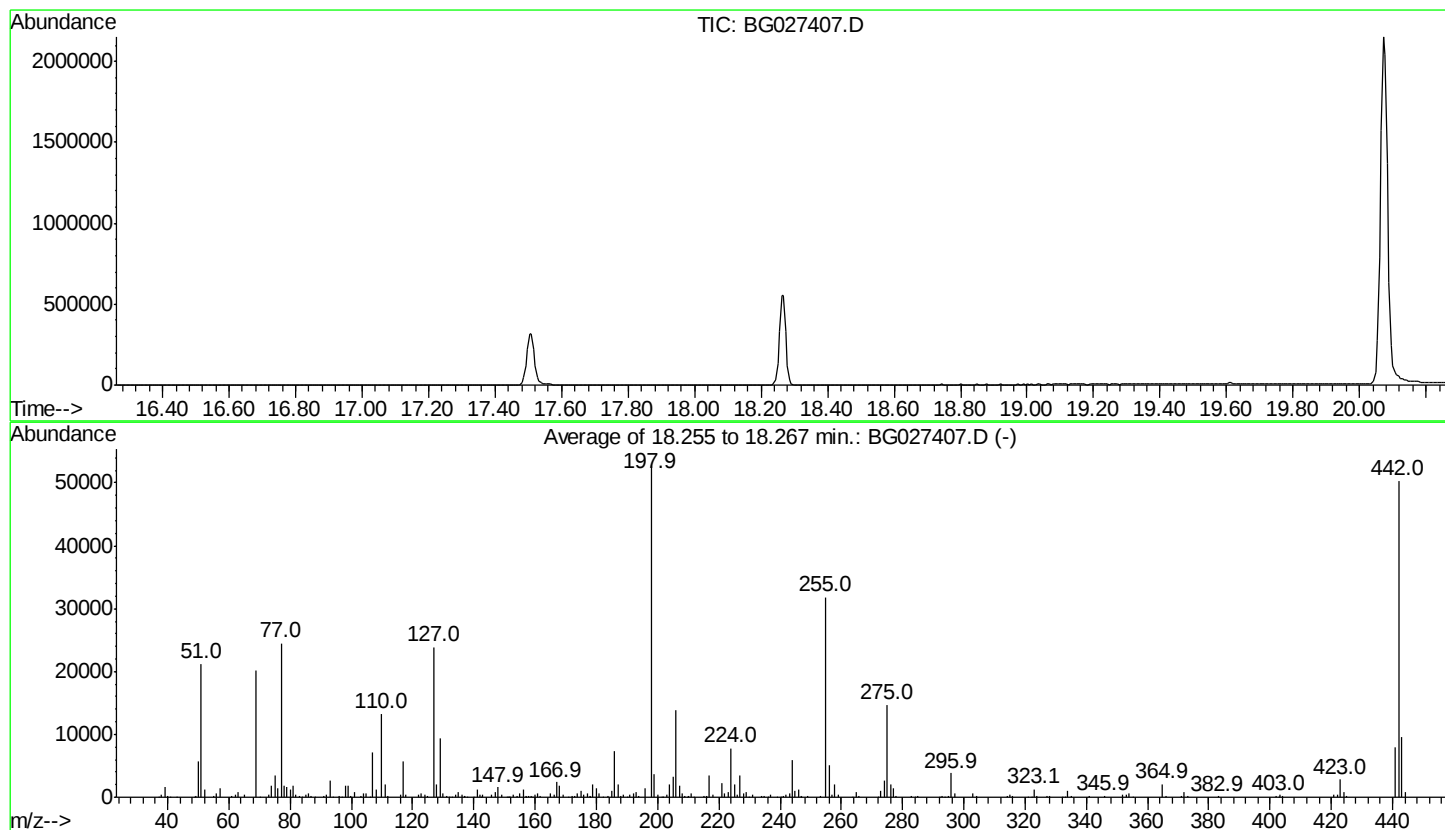

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	21205	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.3	20198	PASS
70	69	0.00	2	0.3	56	PASS
127	198	10	80	45.3	23901	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52741	PASS
199	198	5	9	6.8	3588	PASS
275	198	10	60	28.0	14746	PASS
365	198	1	100	4.0	2101	PASS
441	442	0.01	24	16.0	8038	PASS
442	198	50	100	95.4	50322	PASS
443	442	15	24	18.9	9490	PASS