
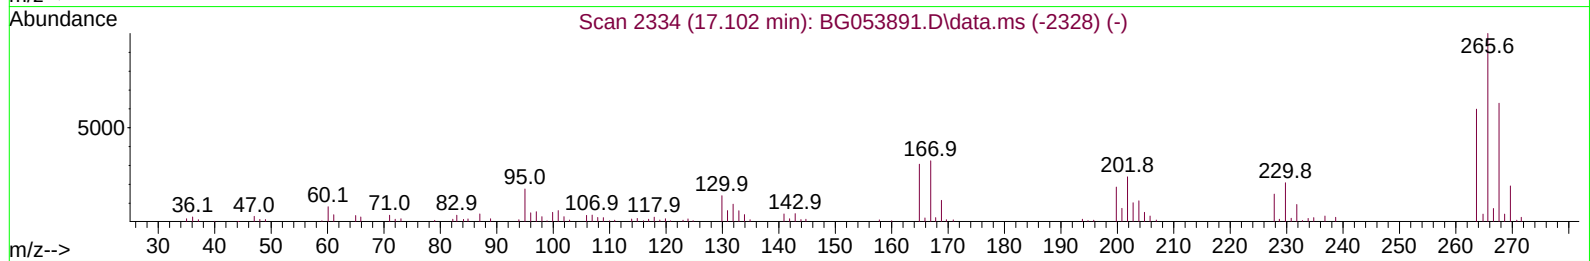
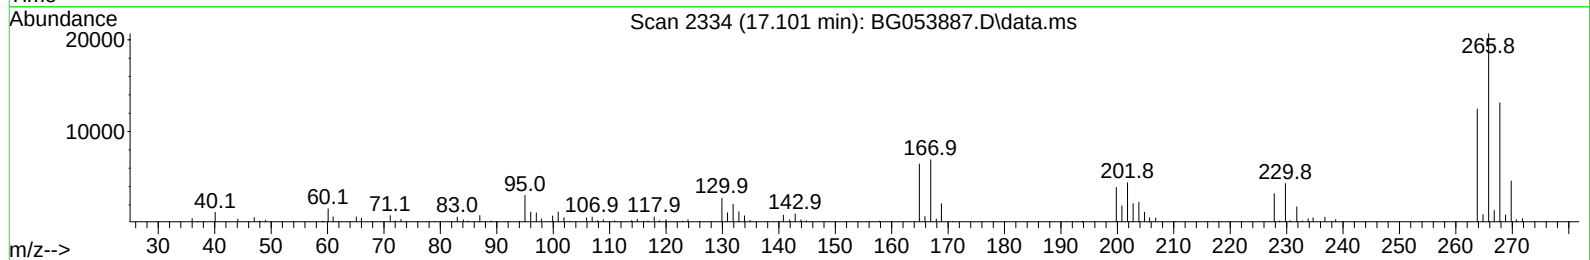


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061322\
Data File : BG053887.D
Acq On : 13 Jun 2022 10:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 14:37:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 14:28:25 2022
Response via : Initial Calibration

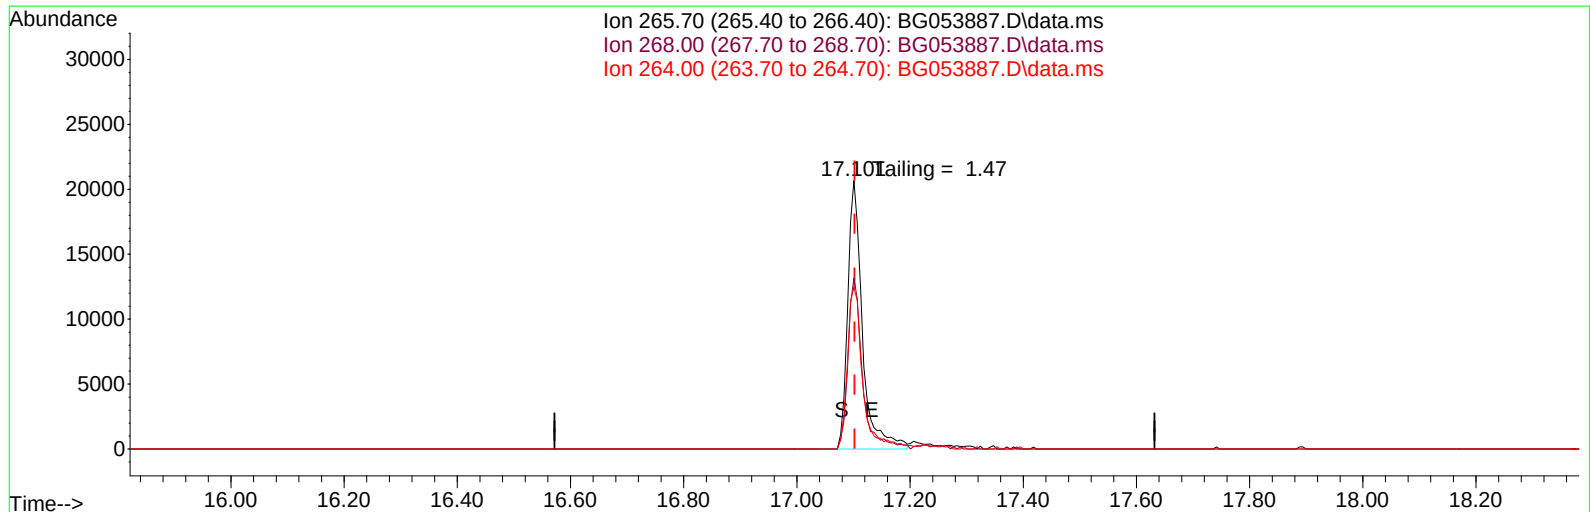

TIC: BG053887.D\data.ms

(70) Pentachlorophenol (C)




17.101min (-0.001) 29510.17 ng

response 37411

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	63.63
264.00	66.20	60.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061322\
Data File : BG053887.D
Acq On : 13 Jun 2022 10:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 14:37:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 14:28:25 2022
Response via : Initial Calibration

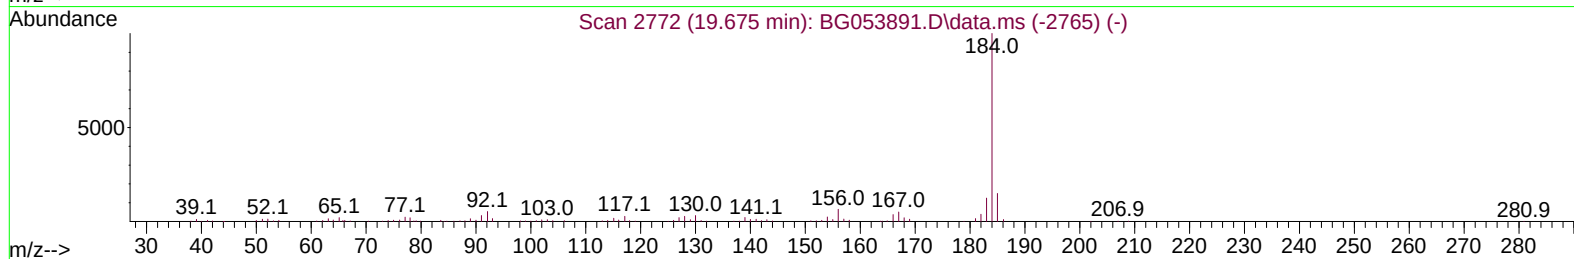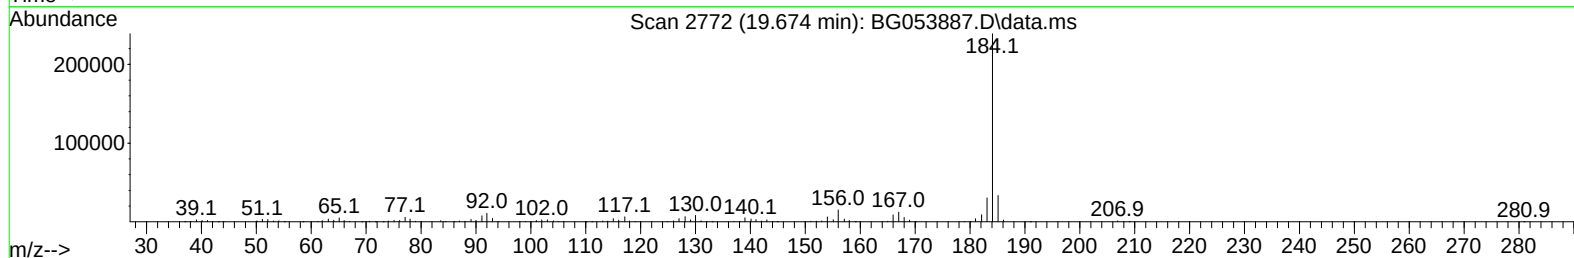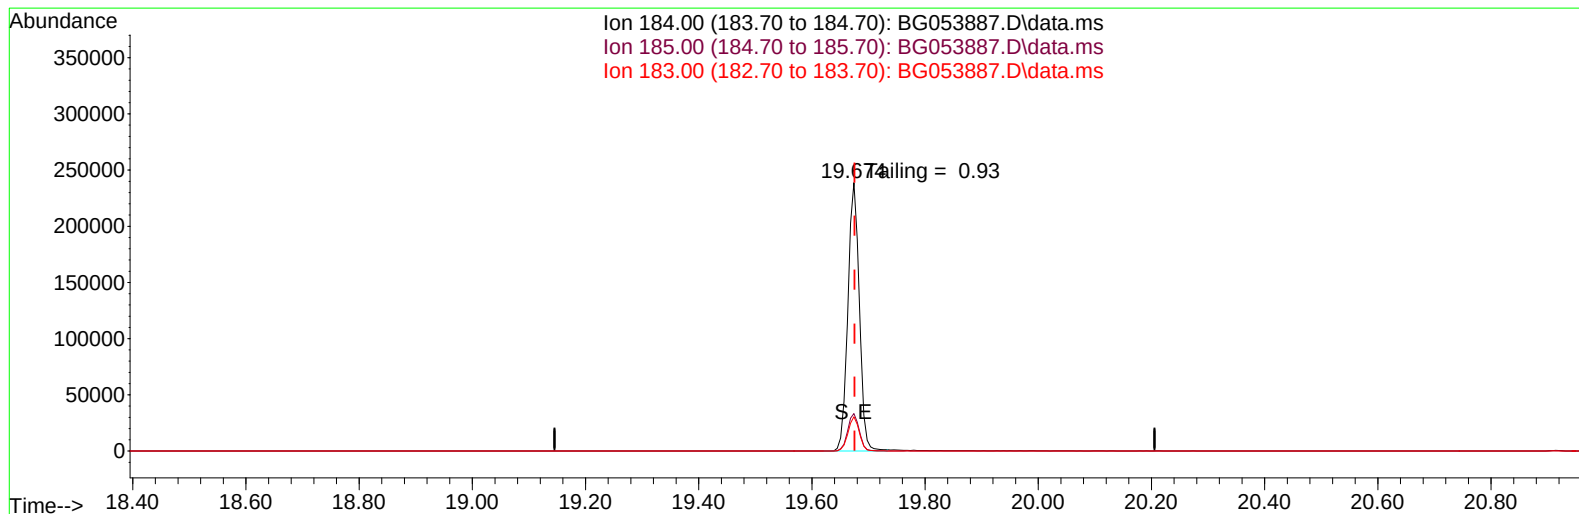

TIC: BG053887.D\data.ms

(77) Benzidine

19.674min (-0.001) 0.00 ng

response 337855

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.98
183.00	11.10	12.78
0.00	0.00	0.00