
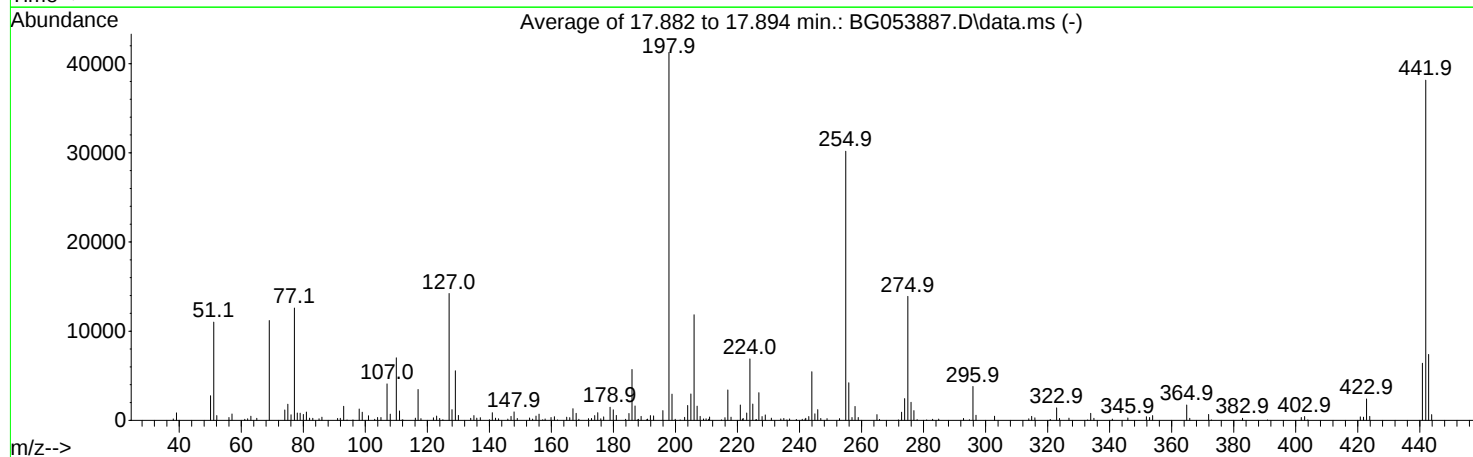


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061322\
 Data File : BG053887.D
 Acq On : 13 Jun 2022 10:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 13 15:49:31 2022

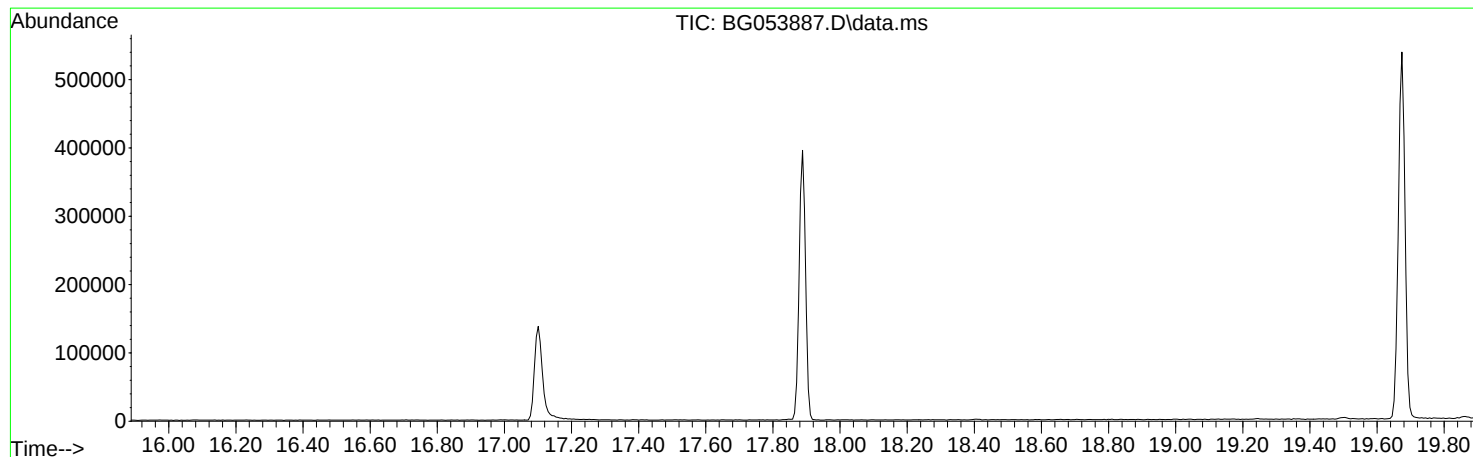




AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.7	11010	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	27.1	11197	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	34.5	14225	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	41248	PASS
199	198	5	9	7.1	2934	PASS
275	198	10	60	33.7	13904	PASS
365	198	1	100	4.2	1724	PASS
441	198	0.01	100	15.5	6413	PASS
442	442	50	100	100.0	38141	PASS
443	442	15	24	19.4	7384	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061322\
Data File : BG053887.D
Acq On : 13 Jun 2022 10:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 13 14:37:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 14:28:25 2022
Response via : Initial Calibration

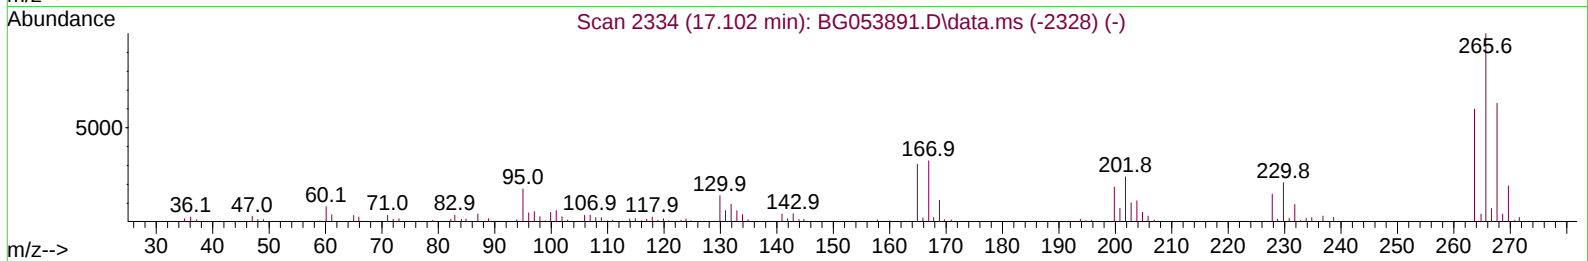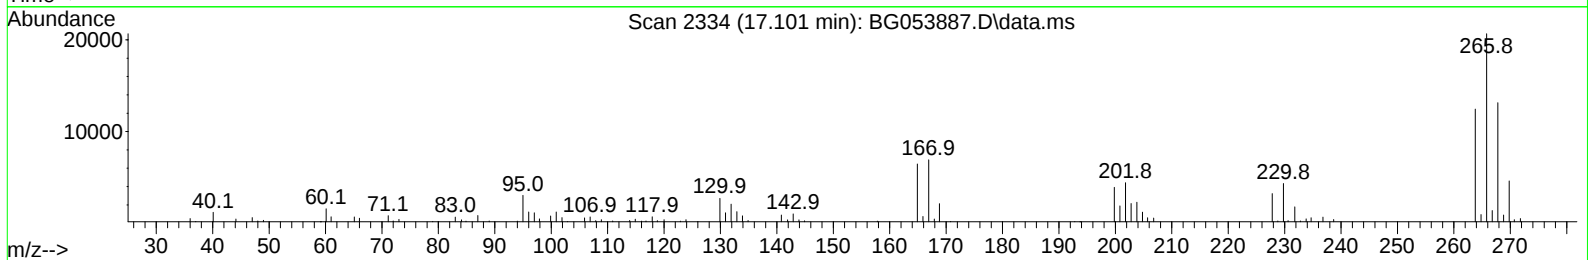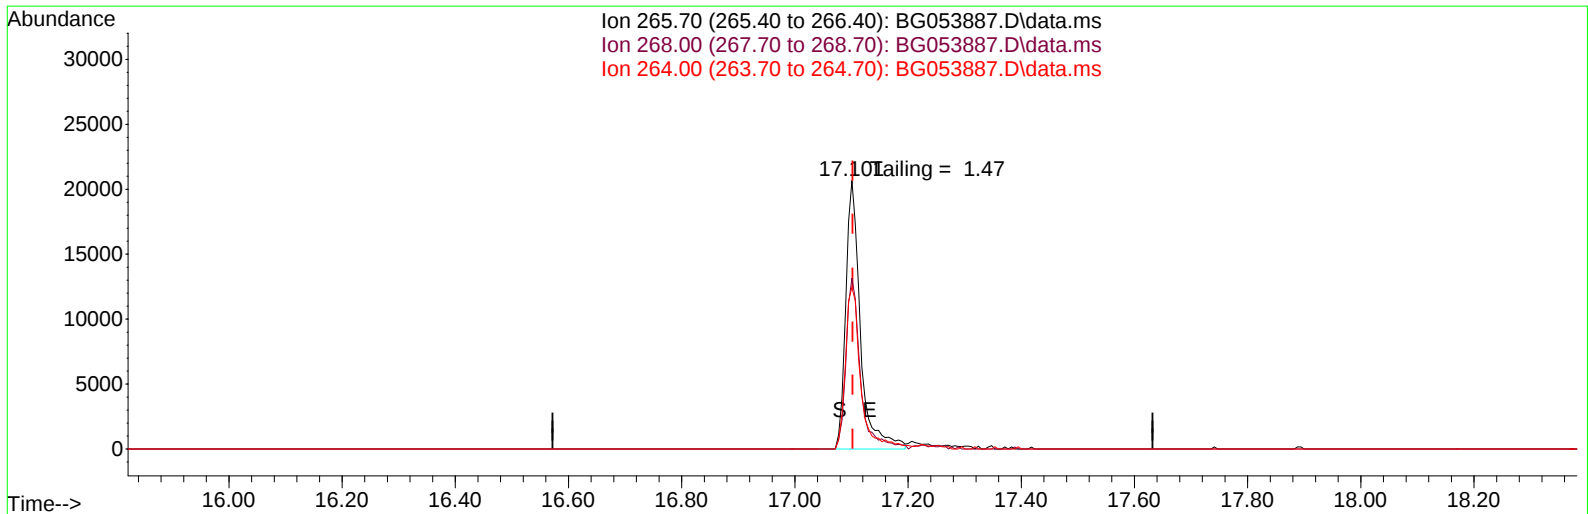

TIC: BG053887.D\data.ms

(70) Pentachlorophenol (C)

17.101min (-0.001) 29510.17 ng




response 37411

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	63.63
264.00	66.20	60.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061322\
Data File : BG053887.D
Acq On : 13 Jun 2022 10:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 13 14:37:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 14:28:25 2022
Response via : Initial Calibration

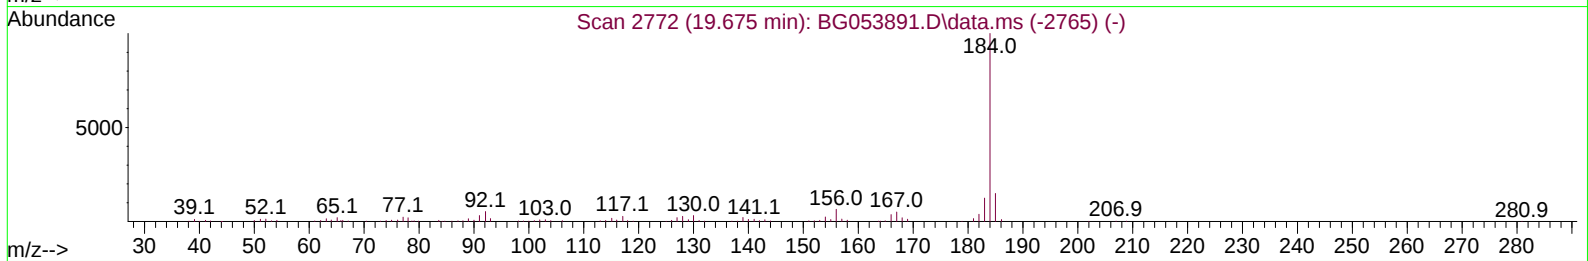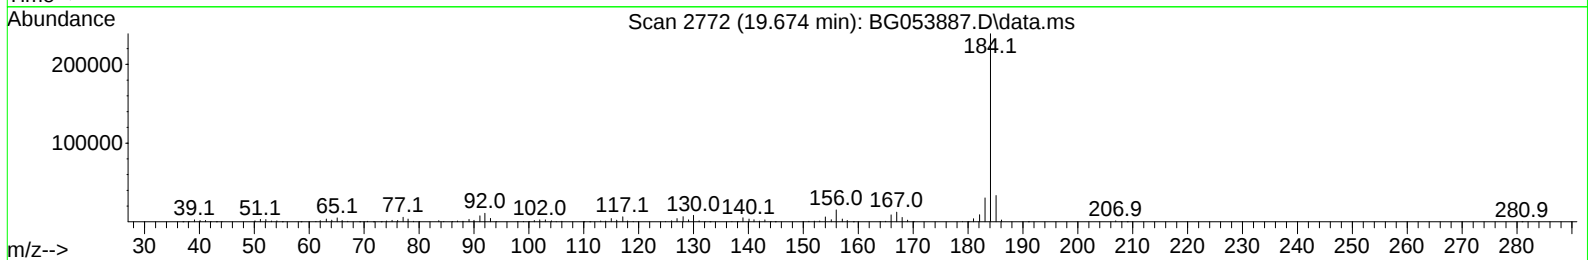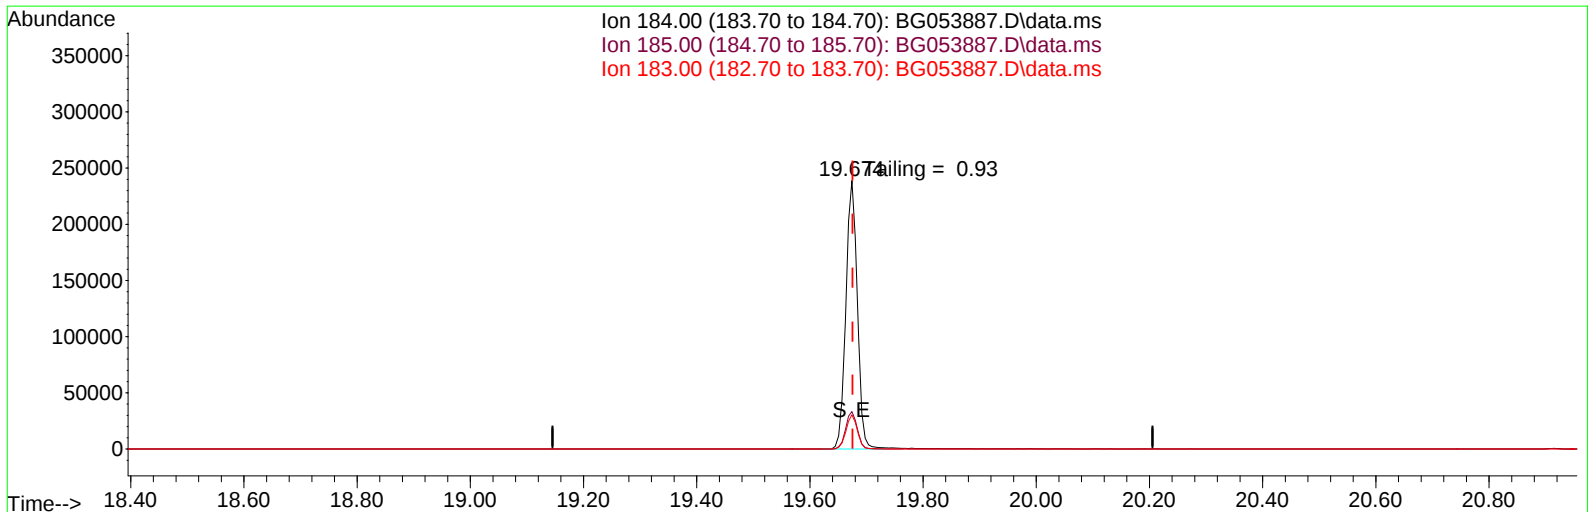

TIC: BG053887.D\data.ms

(77) Benzidine

19.674min (-0.001) 0.00 ng

response 337855

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.98
183.00	11.10	12.78
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/13/2022	BNA_G	<u>BG053887.D</u>
Compound Name	Response	Retention Time
DDT	157790	20.91
DDD	790	20.47
DDE	0	19.97
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
790	158580	0.50