

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061416\
 Data File : BG022341.D
 Acq On : 14 Jun 2016 19:05
 Operator : UM/SJ
 Sample : H3427-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 W-47

Quant Time: Jun 15 02:25:17 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 13 17:40:23 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	20914	20.00	ng	-0.02
21) Naphthalene-d8	10.89	136	101025	20.00	ng	-0.01
38) Acenaphthene-d10	14.71	164	66848	20.00	ng	-0.01
63) Phenanthrene-d10	17.46	188	172157	20.00	ng	-0.01
75) Chrysene-d12	21.73	240	164785	20.00	ng	-0.01
86) Perylene-d12	24.99	264	149886	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.62	112	64934	60.03	ng	-0.02
7) Phenol-d6	7.24	99	57451	33.78	ng	-0.01
23) Nitrobenzene-d5	9.25	82	124861	86.17	ng	-0.01
41) 2,4,6-Tribromophenol	16.20	330	112309	148.68	ng	-0.02
44) 2-Fluorobiphenyl	13.33	172	350701	79.95	ng	-0.01
78) Terphenyl-d14	20.05	244	639366	92.12	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061416\
Data File : BG022341.D
Acq On : 14 Jun 2016 19:05
Operator : UM/SJ
Sample : H3427-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
W-47

Quant Time: Jun 15 02:25:17 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 17:40:23 2016
Response via : Initial Calibration

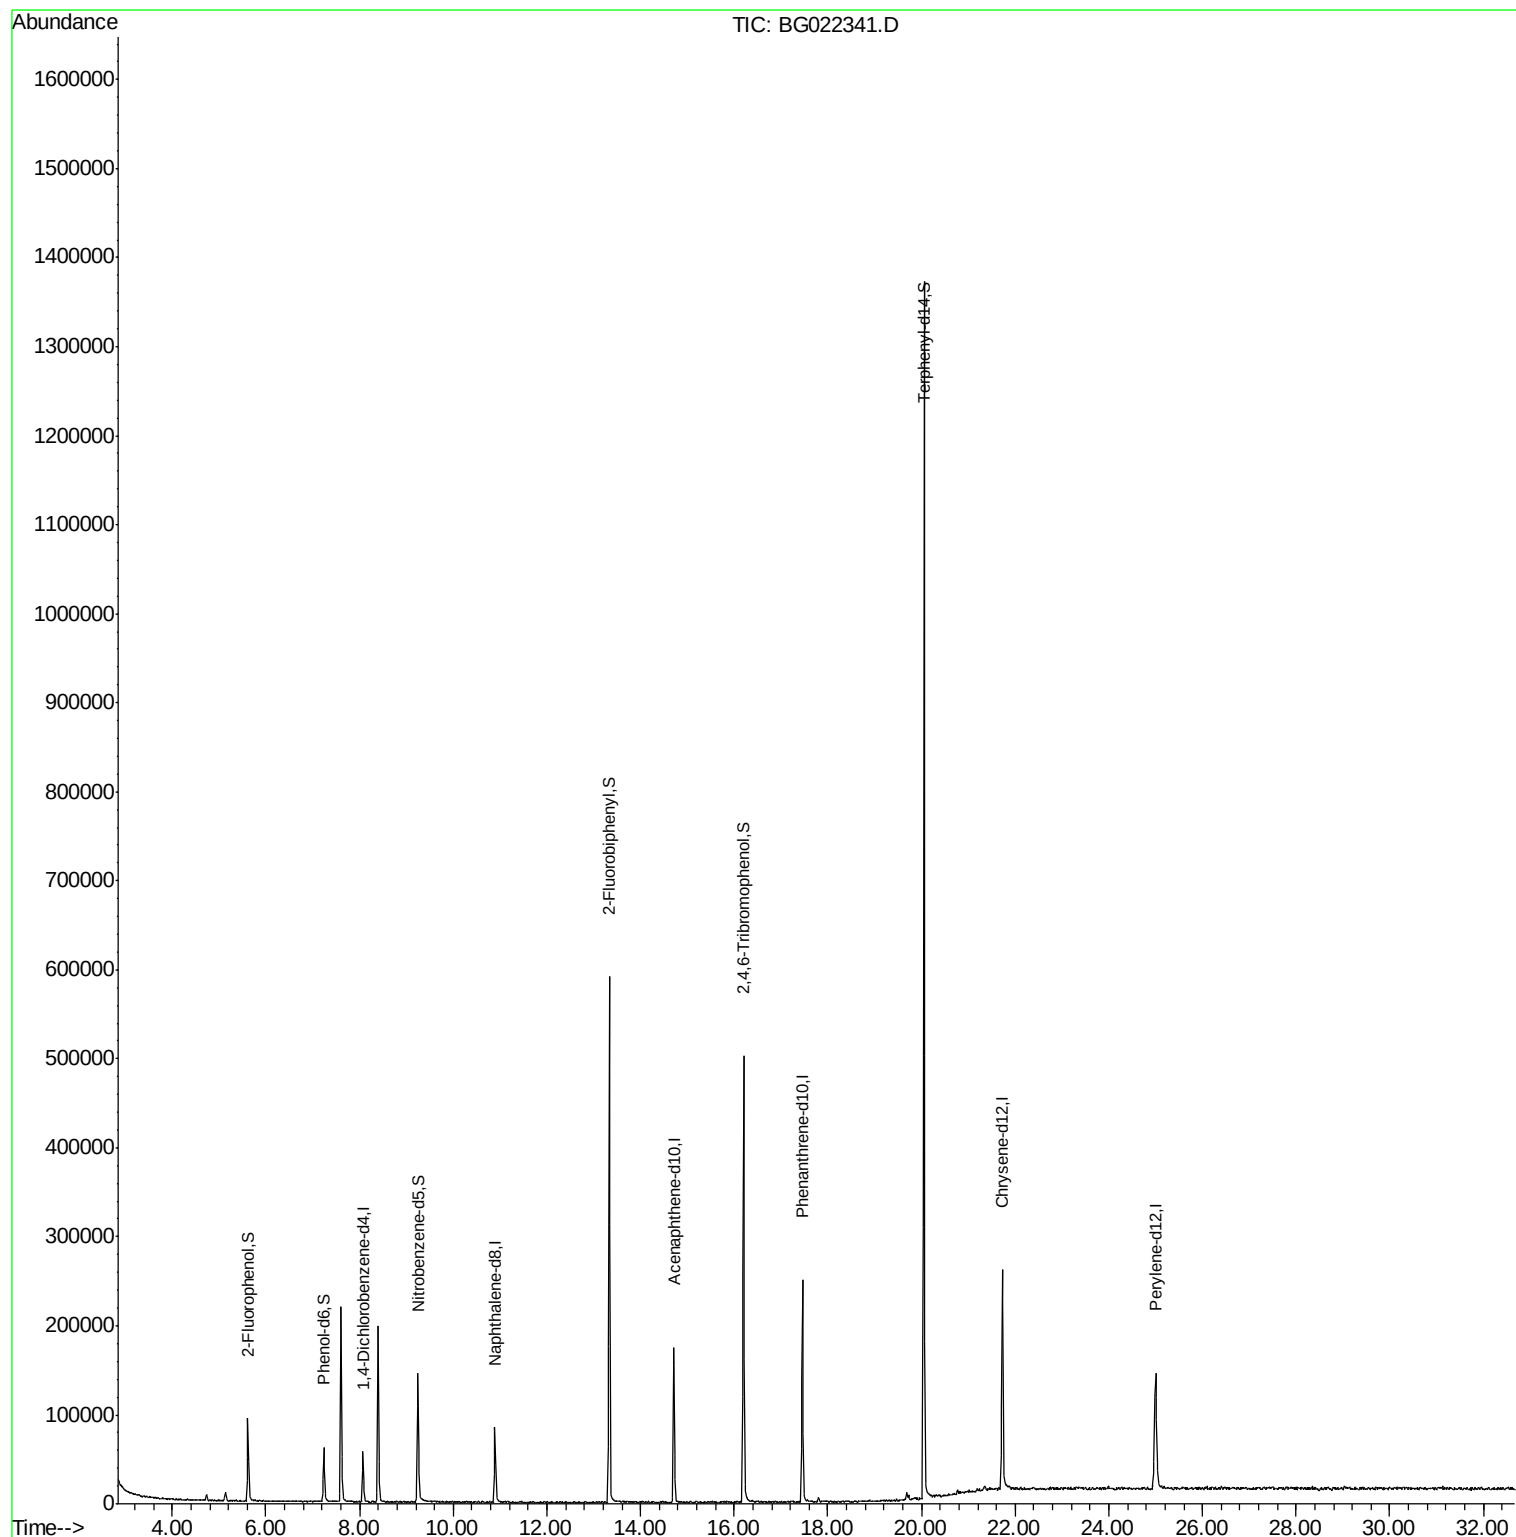


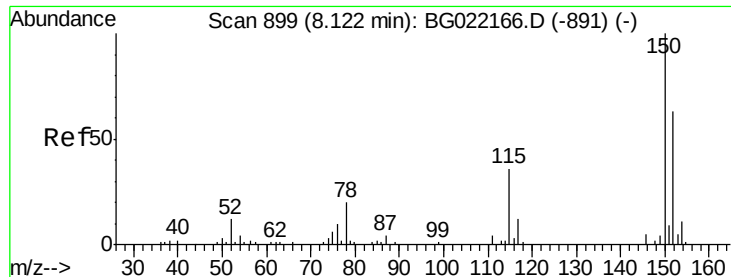




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 8.07 min Scan# 891
 Delta R.T. -0.02 min
 Lab File: BG022341.D
 Acq: 14 Jun 2016 19:05

Instrument :
 BNA_G
 ClientSampleId :
 W-47

Tgt Ion:152 Resp: 20914
 Ion Ratio Lower Upper
 152 100
 150 157.2 130.1 195.1
 115 57.3 62.2 93.2#

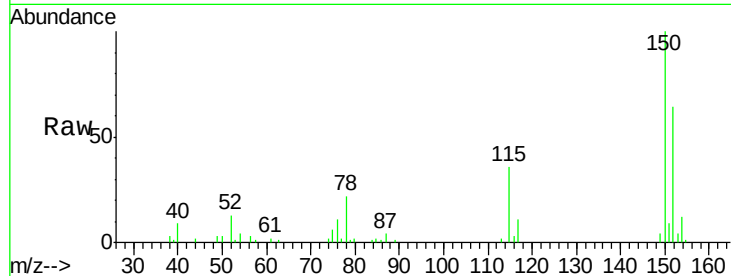


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

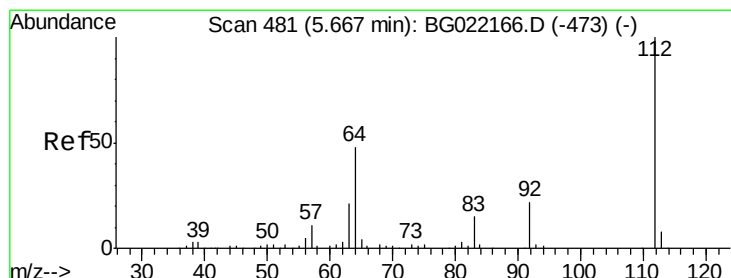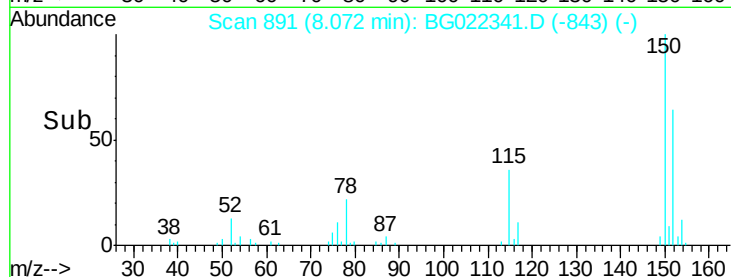
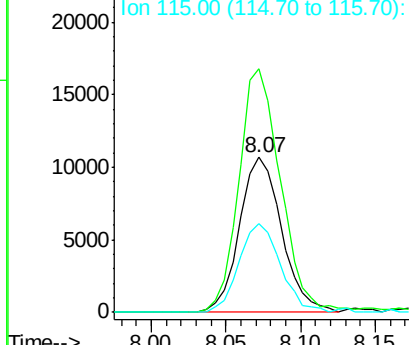



#5
 2-Fluorophenol
 Concen: 60.03 ng
 RT: 5.62 min Scan# 473
 Delta R.T. -0.02 min
 Lab File: BG022341.D
 Acq: 14 Jun 2016 19:05

Tgt Ion:112 Resp: 64934
 Ion Ratio Lower Upper
 112 100
 64 50.8 51.1 76.7#
 63 23.7 24.6 37.0#

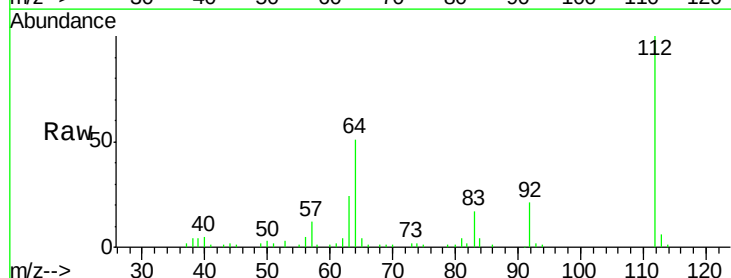

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BGC
 Ion 63.00 (62.70 to 63.70): BGC

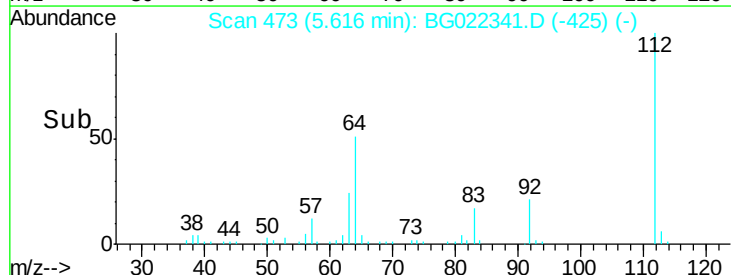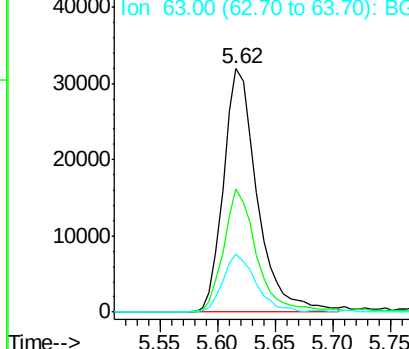

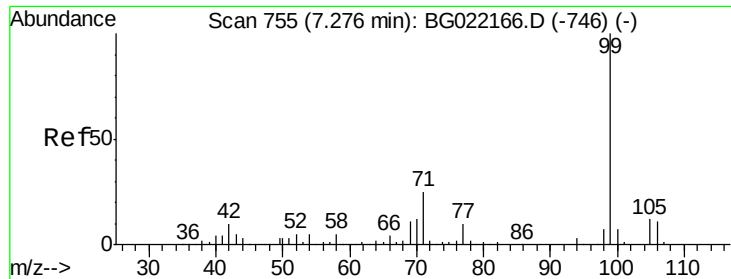

#7

Phenol-d6

Concen: 33.78 ng

RT: 7.24 min Scan# 749

Delta R.T. -0.01 min

Lab File: BG022341.D

Acq: 14 Jun 2016 19:05

Instrument :

BNA_G

ClientSampleId :

W-47


Tgt Ion: 99 Resp: 57451

Ion Ratio Lower Upper




99 100

42 11.3 16.4 24.6#

71 24.6 25.0 37.4#

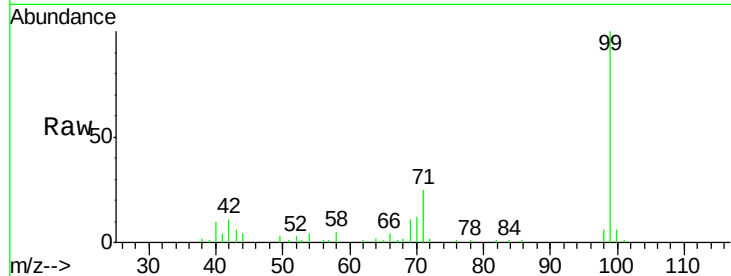

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

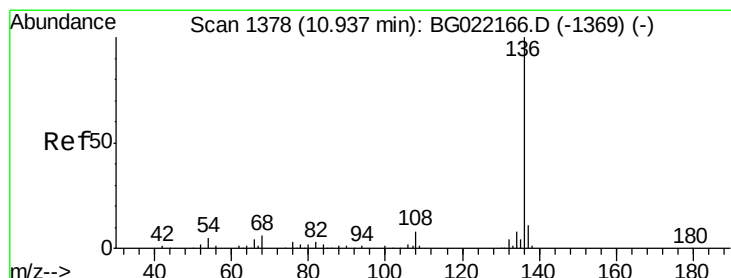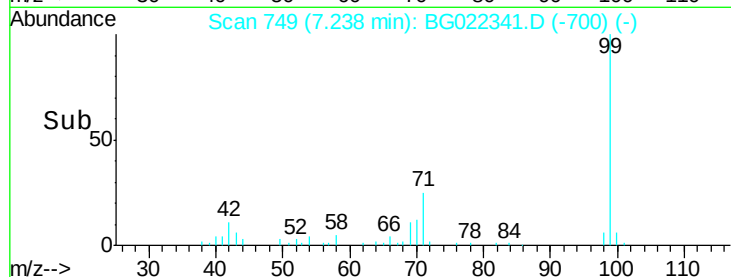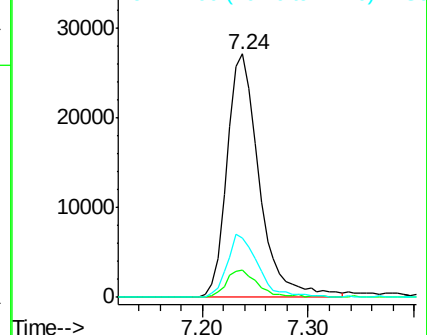

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.89 min Scan# 1371

Delta R.T. -0.01 min

Lab File: BG022341.D

Acq: 14 Jun 2016 19:05

Tgt Ion: 136 Resp: 101025


Ion Ratio Lower Upper

136 100



137 11.2 9.0 13.4


54 5.8 9.6 14.4#

68 5.7 6.4 9.6#

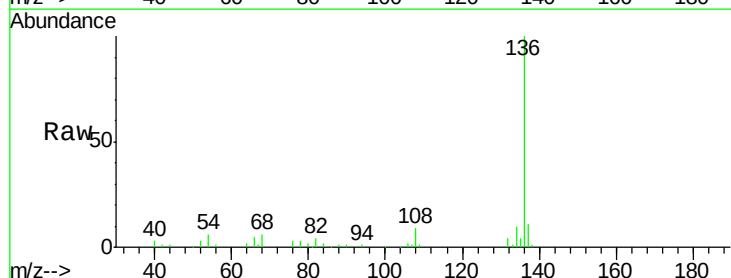

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

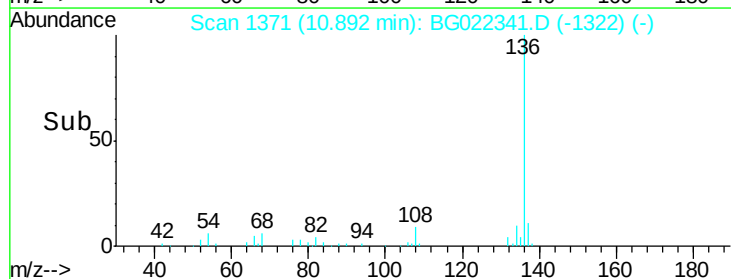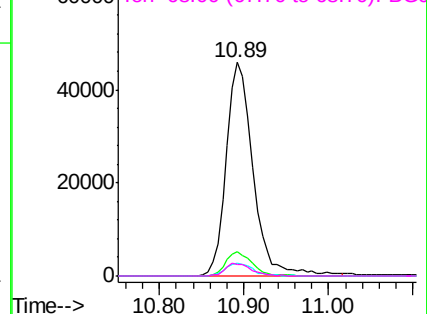


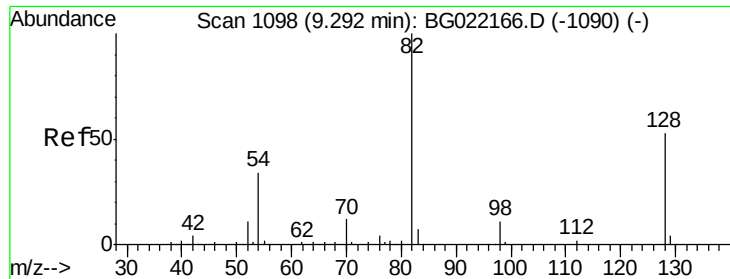




#23
 Nitrobenzene-d5
 Concen: 86.17 ng
 RT: 9.25 min Scan# 1091
 Delta R.T. -0.01 min
 Lab File: BG022341.D
 Acq: 14 Jun 2016 19:05

Instrument :
 BNA_G
 ClientSampled :
 W-47

Tgt Ion: 82 Resp: 124861
 Ion Ratio Lower Upper
 82 100
 128 50.0 33.4 50.0
 54 36.2 46.1 69.1#

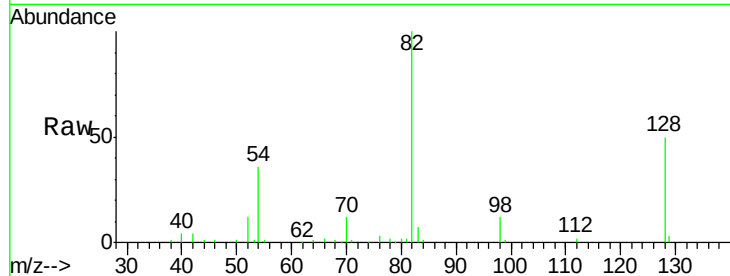


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

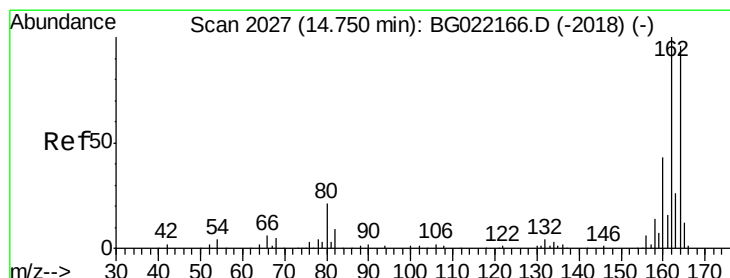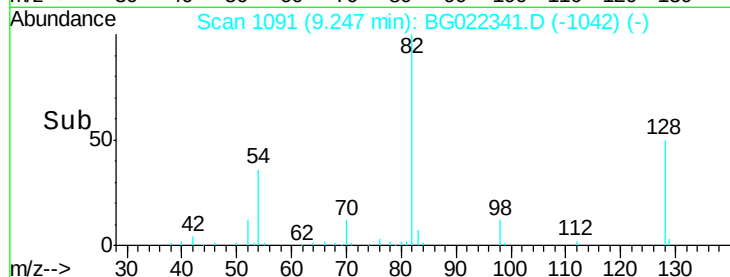
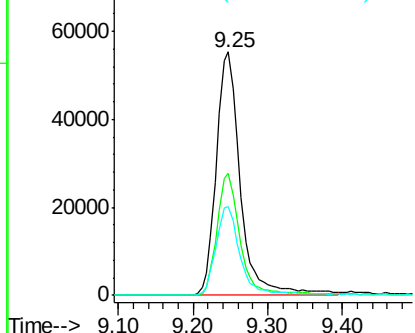



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.71 min Scan# 2021
 Delta R.T. -0.01 min
 Lab File: BG022341.D
 Acq: 14 Jun 2016 19:05

Tgt Ion: 164 Resp: 66848
 Ion Ratio Lower Upper
 164 100
 162 101.4 78.0 117.0
 160 49.2 32.9 49.3

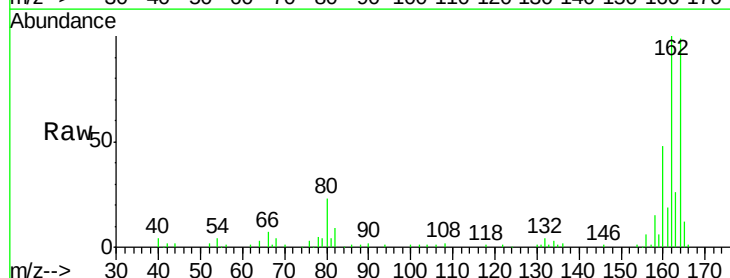

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

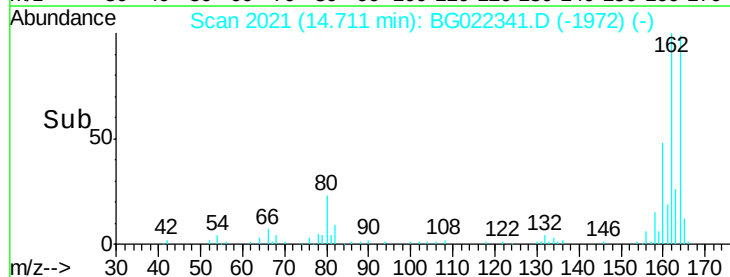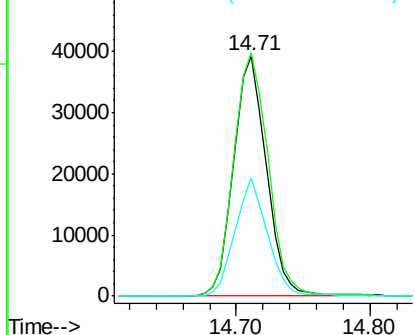


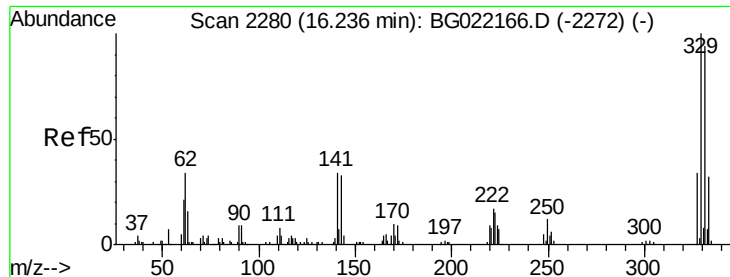




#41
 2,4,6-Tribromophenol
 Concen: 148.68 ng
 RT: 16.20 min Scan# 2274
 Delta R.T. -0.02 min
 Lab File: BG022341.D
 Acq: 14 Jun 2016 19:05

Instrument :
 BNA_G
 ClientSampleId :
 W-47

Tgt Ion	Ratio	Lower	Upper
330	100		
332	95.2	78.0	117.0
141	39.9	33.8	50.8

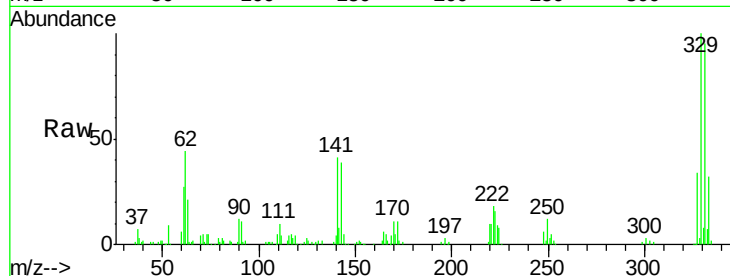


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

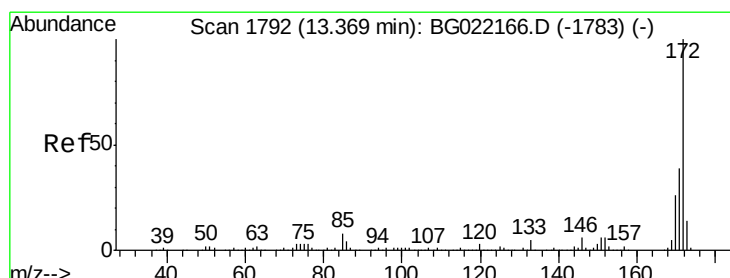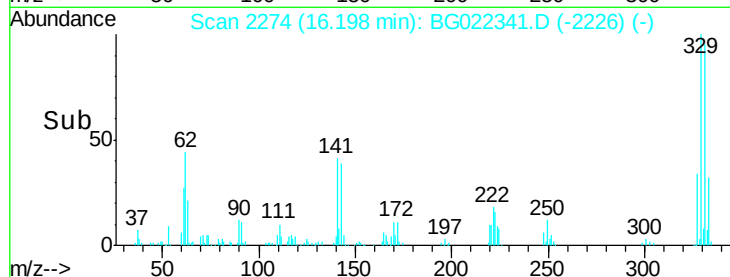
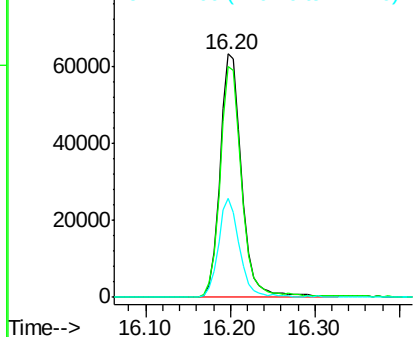



#44
 2-Fluorobiphenyl
 Concen: 79.95 ng
 RT: 13.33 min Scan# 1786
 Delta R.T. -0.01 min
 Lab File: BG022341.D
 Acq: 14 Jun 2016 19:05

Tgt Ion	Ratio	Lower	Upper
172	100		
171	39.0	27.8	41.6
170	25.3	19.6	29.4

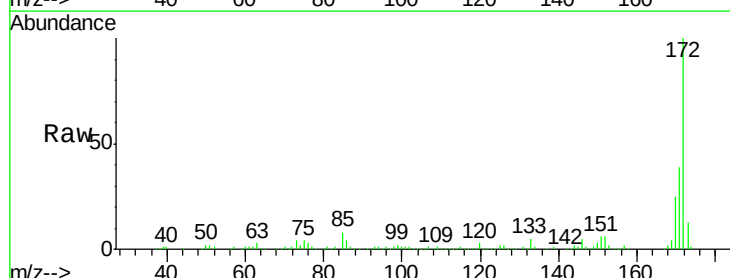

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

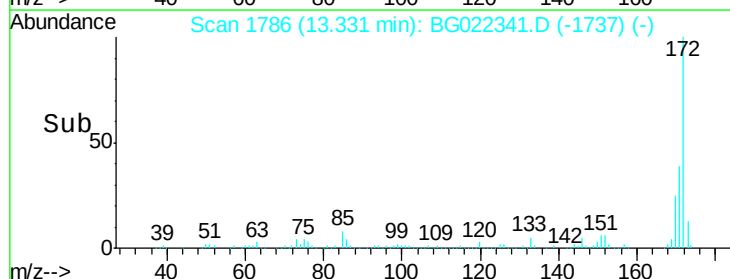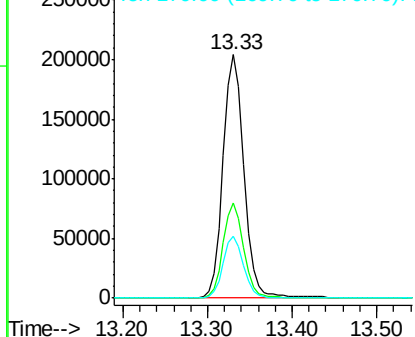

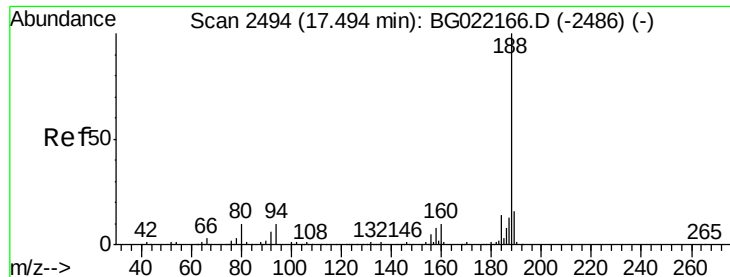

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.46 min Scan# 2488

Delta R.T. -0.01 min

Lab File: BG022341.D

Acq: 14 Jun 2016 19:05

Instrument :

BNA_G

ClientSampleId :

W-47


Tgt Ion:188 Resp: 172157

Ion Ratio Lower Upper

188 100

94 11.0 7.5 11.3




80 10.6 8.6 13.0

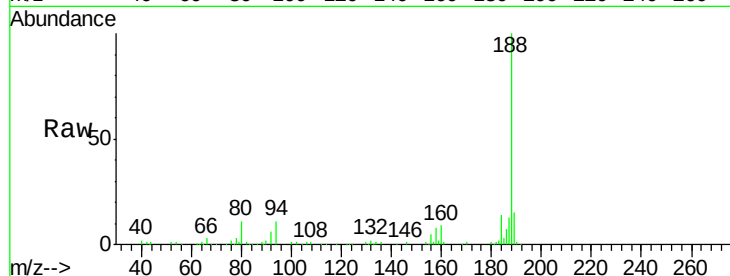

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

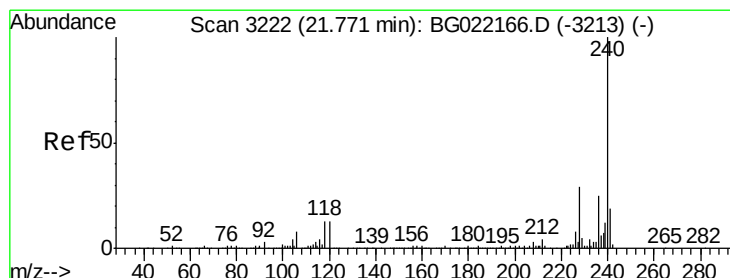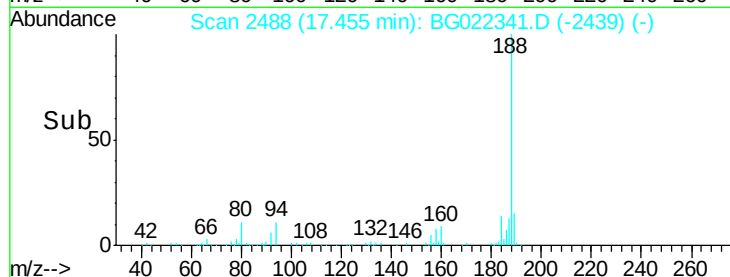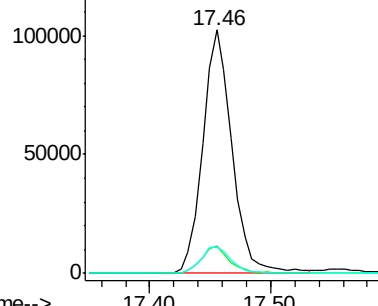

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.73 min Scan# 3215

Delta R.T. -0.01 min

Lab File: BG022341.D

Acq: 14 Jun 2016 19:05


Tgt Ion:240 Resp: 164785

Ion Ratio Lower Upper

240 100

120 12.9 8.4 12.6#



236 26.6 19.6 29.4

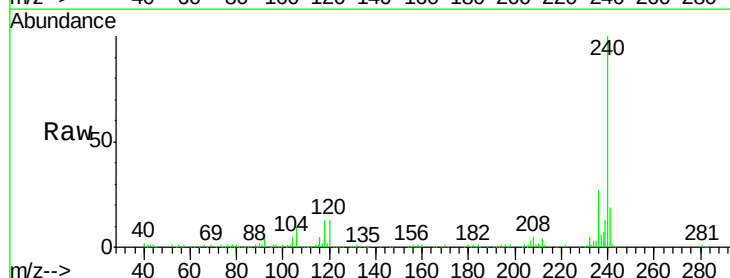


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

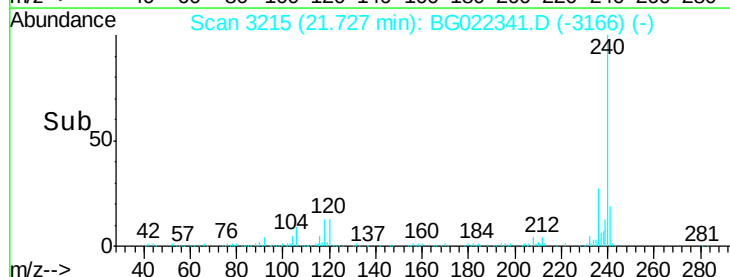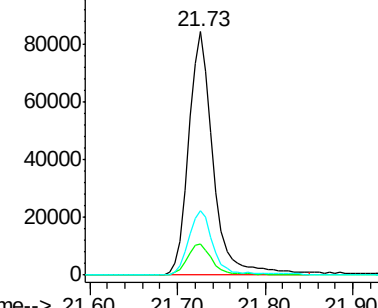

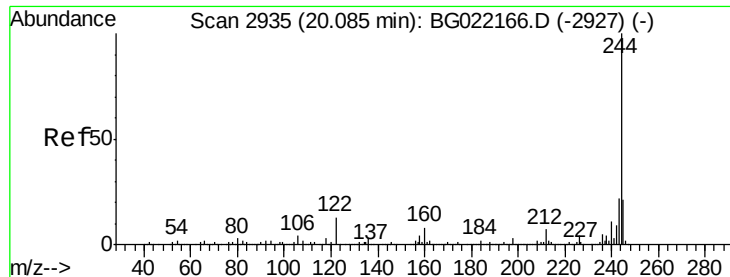

#78

Terphenyl-d14

Concen: 92.12 ng

RT: 20.05 min Scan# 2930

Delta R.T. -0.01 min

Lab File: BG022341.D

Acq: 14 Jun 2016 19:05

Instrument :

BNA_G

ClientSampled :

W-47


Tgt Ion:244 Resp: 639366

Ion Ratio Lower Upper

244 100

212 7.6 6.5 9.7




122 13.7 8.6 12.8#

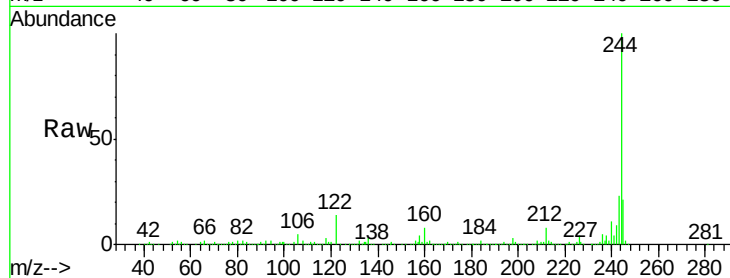

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

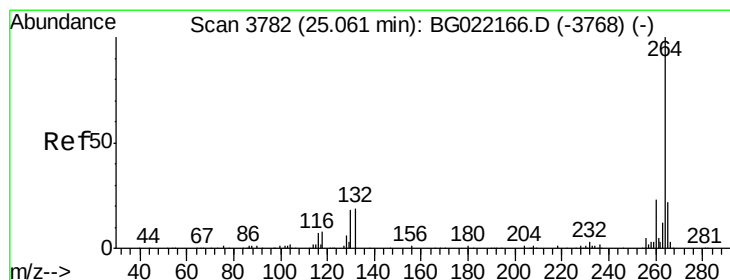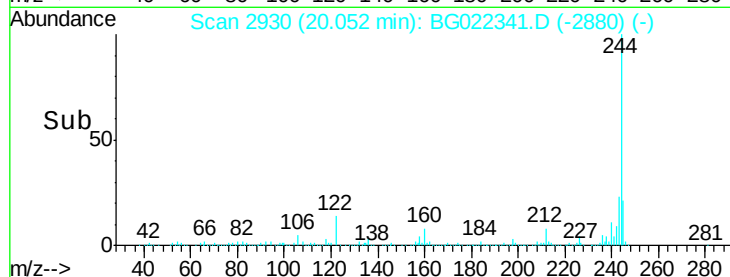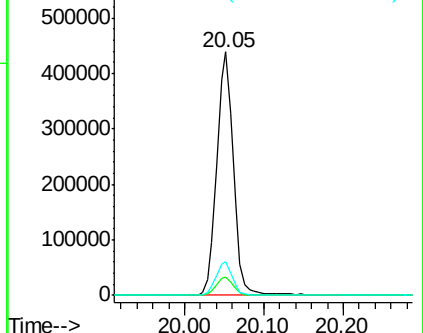

#86

Perylene-d12

Concen: 20.00 ng

RT: 24.99 min Scan# 3771

Delta R.T. -0.02 min

Lab File: BG022341.D

Acq: 14 Jun 2016 19:05


Tgt Ion:264 Resp: 149886

Ion Ratio Lower Upper

264 100

260 22.8 20.2 30.4

265 22.0 17.8 26.8

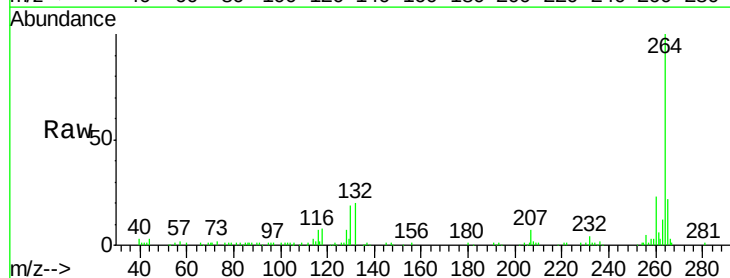

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

