
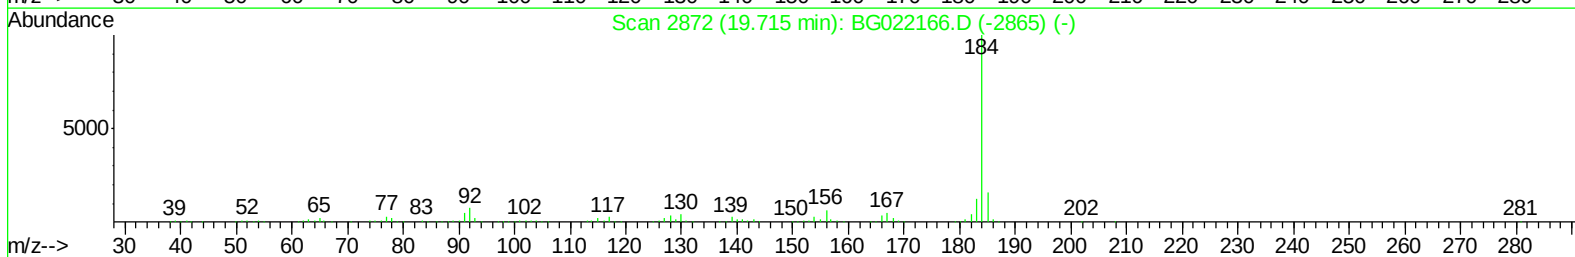
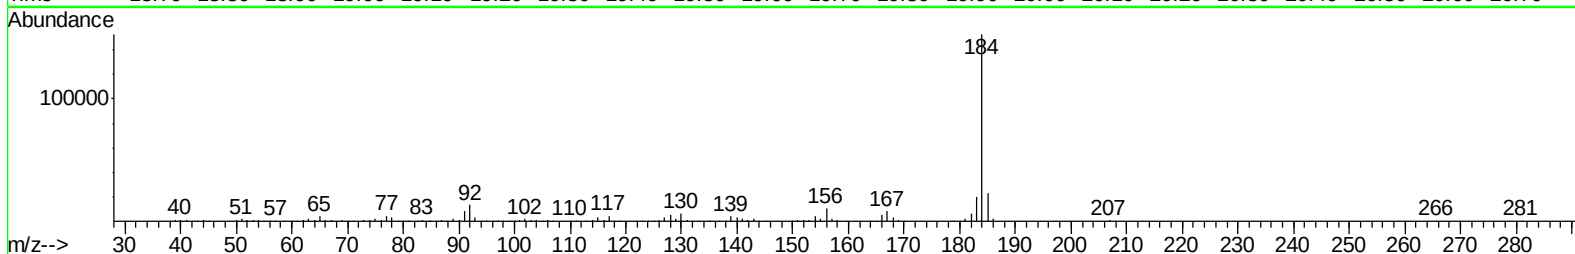


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061416\
Data File : BG022333.D
Acq On : 14 Jun 2016 12:13
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 07:09:50 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 17:40:23 2016
Response via : Initial Calibration

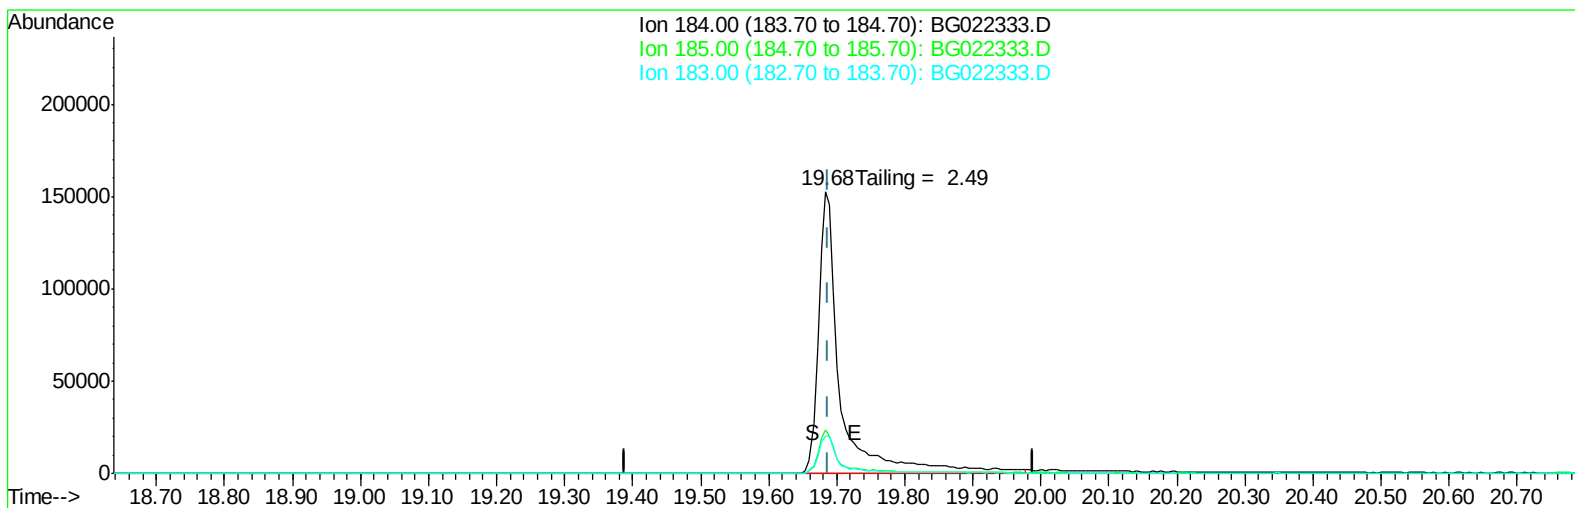

TIC: BG022333.D

(76) Benzidine




19.683min (-0.006) 237129.06ng m

response 347255

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	15.28
183.00	12.80	13.31
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061416\
Data File : BG022333.D
Acq On : 14 Jun 2016 12:13
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 07:09:50 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 17:40:23 2016
Response via : Initial Calibration

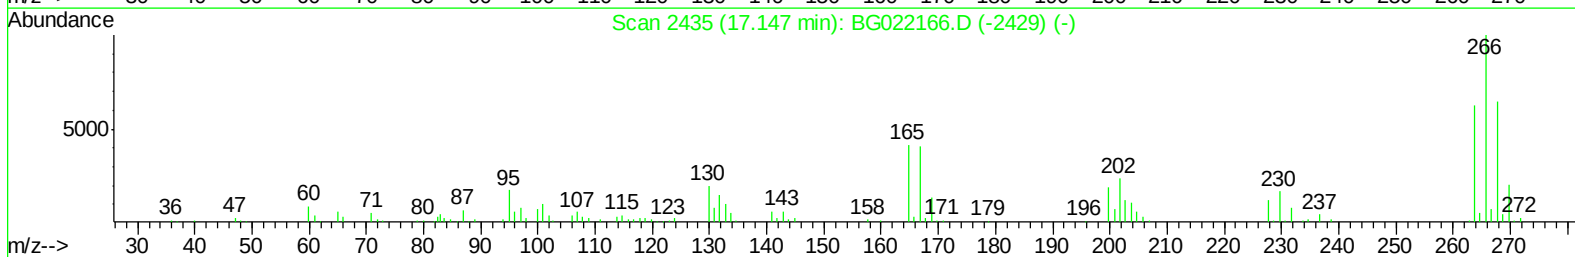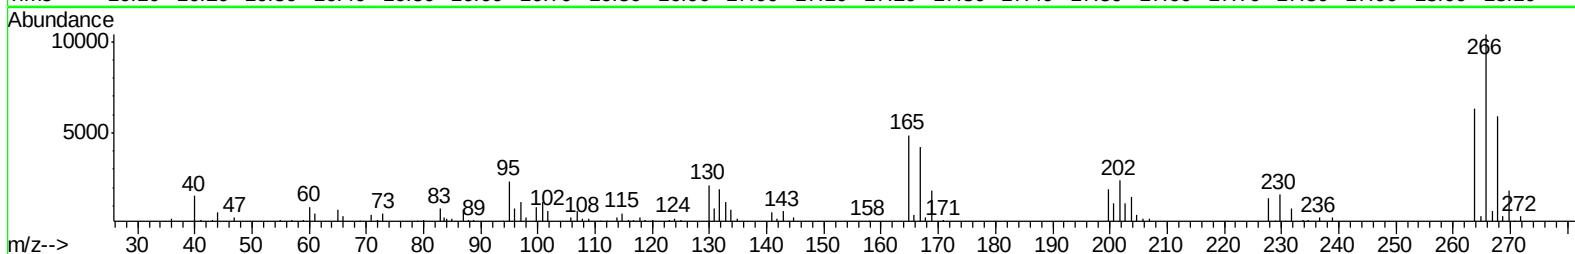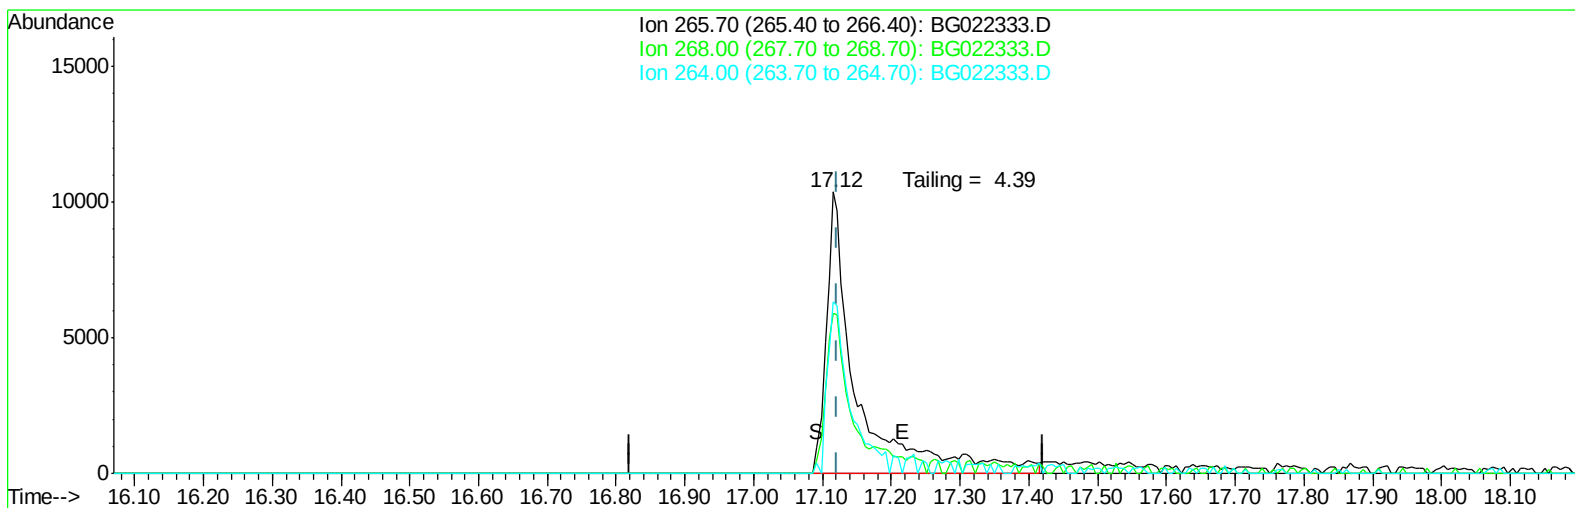

TIC: BG022333.D

(69) Pentachlorophenol (C)

17.116min (-0.006) 0.00ng

response 24359

Ion	Exp%	Act%
265.70	100	100
268.00	68.10	60.72
264.00	67.20	60.76
0.00	0.00	0.00