

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061416\
 Data File : BG022337.D
 Acq On : 14 Jun 2016 16:26
 Operator : UM/SJ
 Sample : H3427-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 W-19

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.617	466	473	486	rBV	120056	240549	11.04%	2.910%
2	7.239	739	749	760	rBV	83099	170463	7.82%	2.062%
3	7.603	804	811	828	rBV	275374	537483	24.67%	6.503%
4	8.073	882	891	903	rBV	67846	136649	6.27%	1.653%
5	8.396	939	946	956	rVB	244134	470094	21.57%	5.688%
6	9.248	1084	1091	1103	rBV	187039	393971	18.08%	4.767%
7	10.893	1363	1371	1384	rBV	103780	245561	11.27%	2.971%
8	13.332	1778	1786	1801	rBV	704106	1193292	54.76%	14.438%
9	14.712	2013	2021	2029	rBV2	201370	350663	16.09%	4.243%
10	16.199	2267	2274	2289	rBV	576958	958062	43.97%	11.592%
11	17.456	2481	2488	2497	rBV2	284999	477915	21.93%	5.782%
12	20.053	2923	2930	2947	rBV	1464640	2179010	100.00%	26.364%
13	21.728	3208	3215	3228	rBV	257353	489893	22.48%	5.927%
14	25.000	3761	3772	3784	rVB2	128315	421515	19.34%	5.100%


Sum of corrected areas: 8265120

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061416\
Data File : BG022337.D
Acq On : 14 Jun 2016 16:26
Operator : UM/SJ
Sample : H3427-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
W-19

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

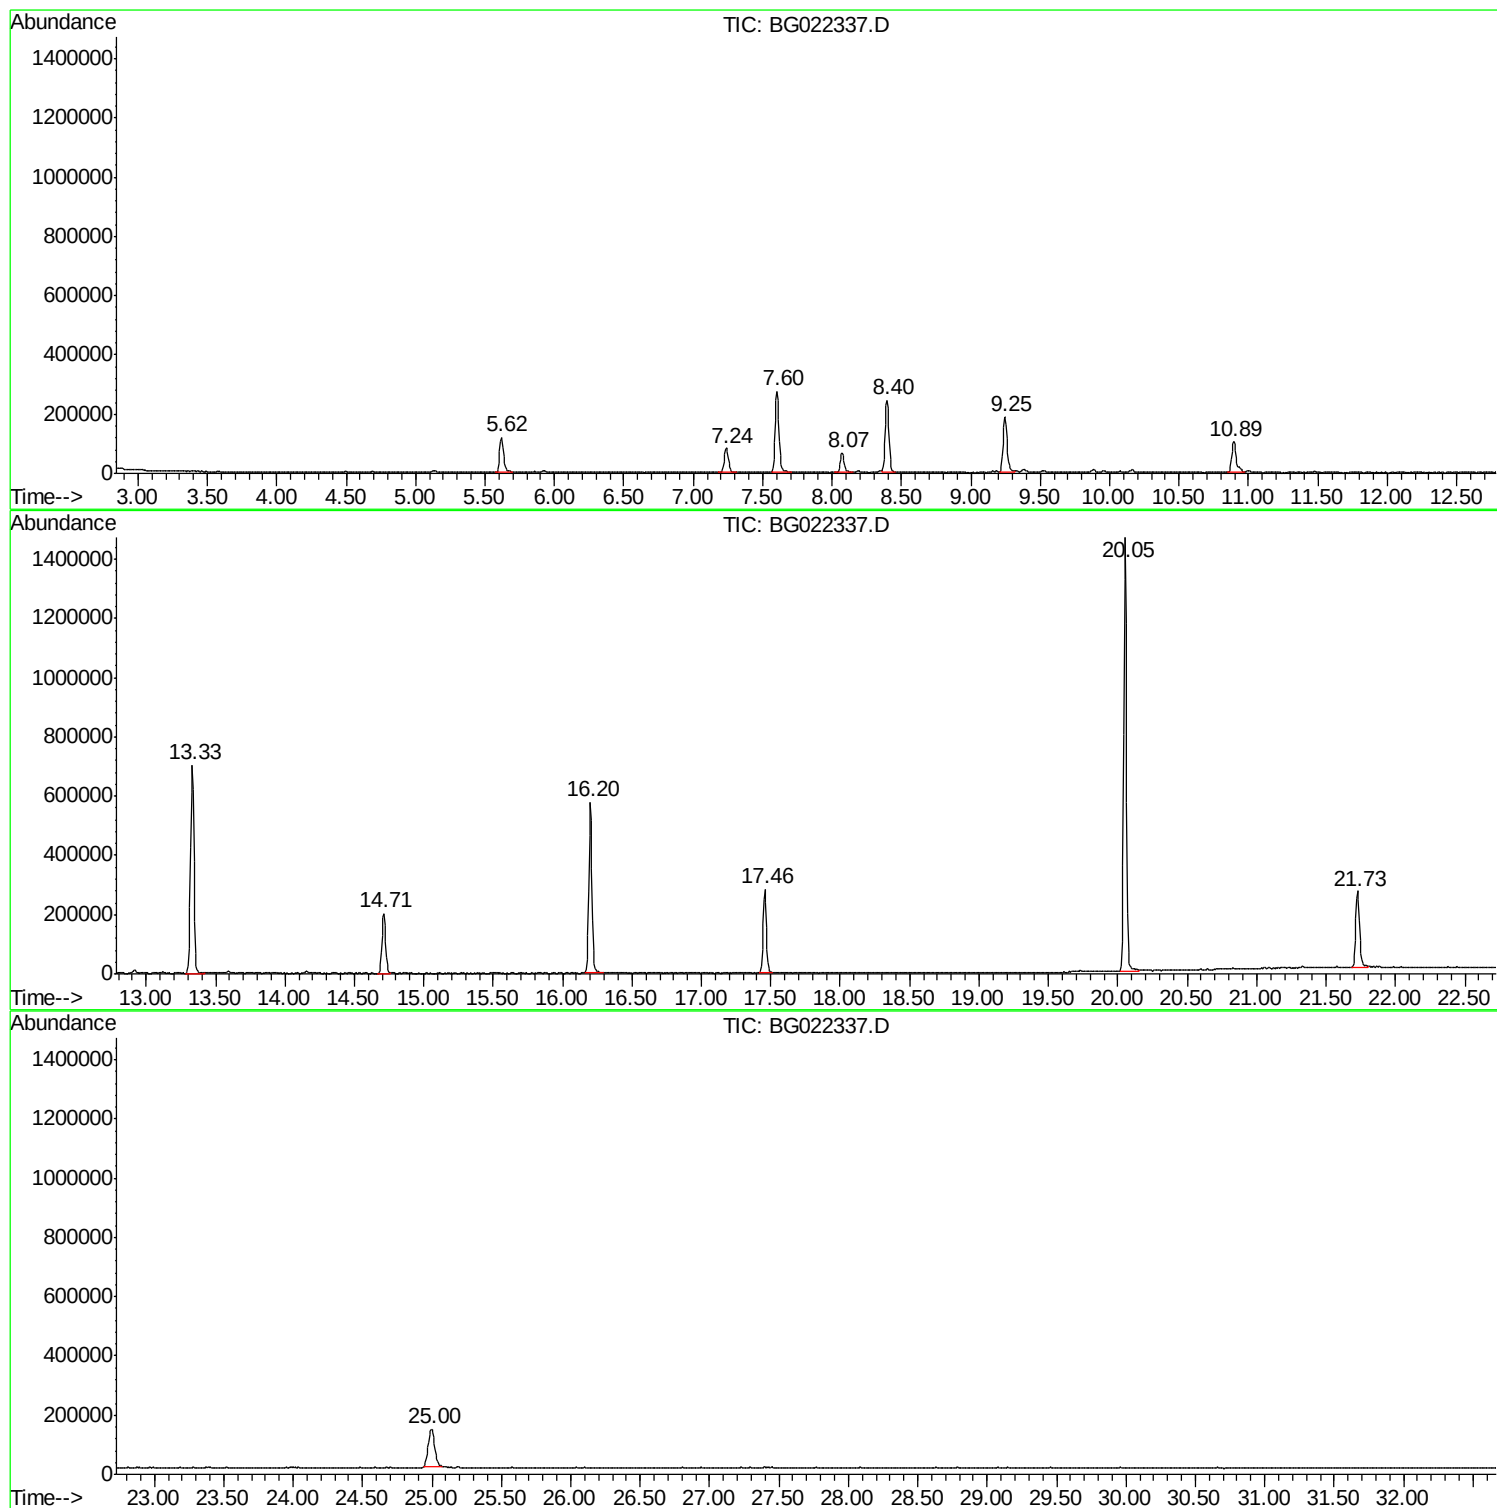

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061416\
Data File : BG022337.D
Acq On : 14 Jun 2016 16:26
Operator : UM/SJ
Sample : H3427-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
W-19










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.60 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.60	78.67 ng	537483	1,4-Dichlorobenzene-d4	8.07

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		Amphetaminil	250	C17H18N2	017590-01-1	12
4		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
5		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9

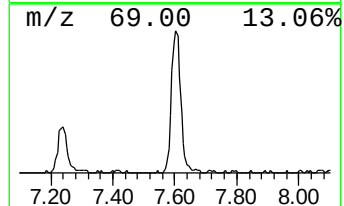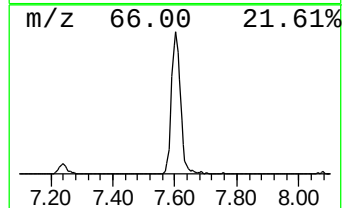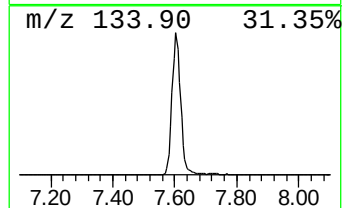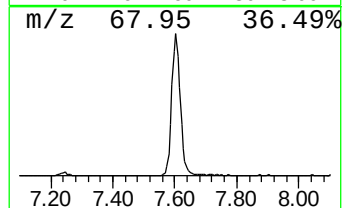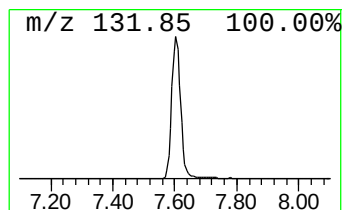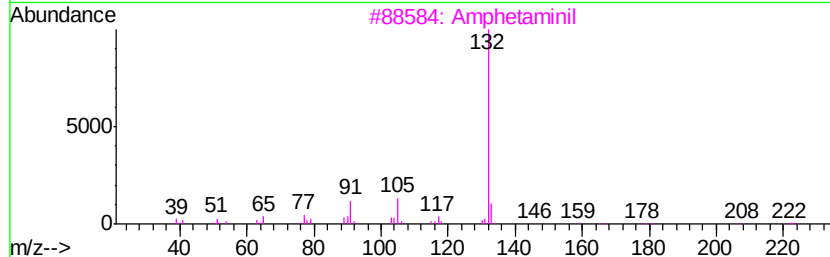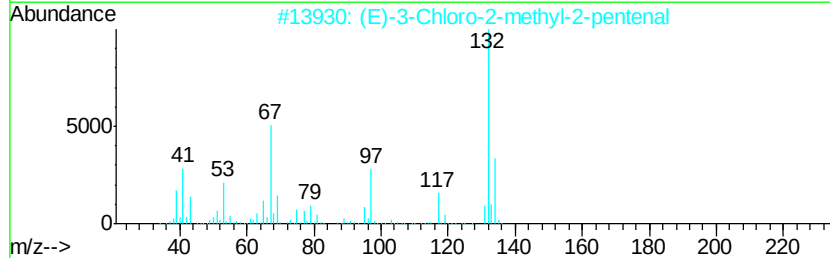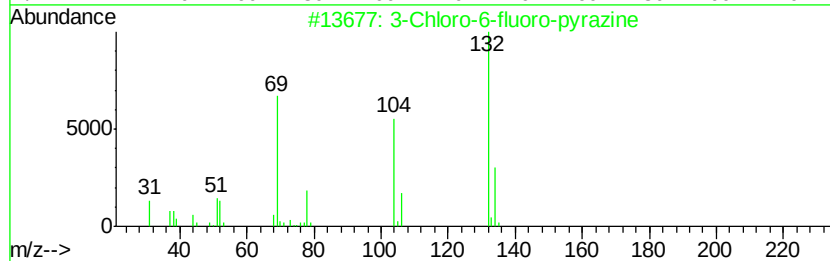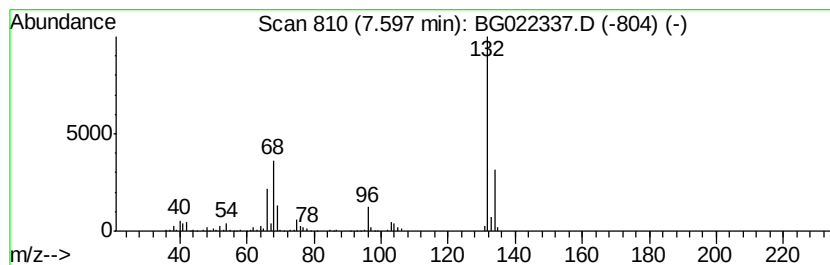

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061416\
Data File : BG022337.D
Acq On : 14 Jun 2016 16:26
Operator : UM/SJ
Sample : H3427-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
W-19

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.60	7.60	78.7	ng	537483	1	8.07	136649	20.0