

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061416\
 Data File : BG022340.D
 Acq On : 14 Jun 2016 18:25
 Operator : UM/SJ
 Sample : H3427-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 W-42

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.618	467	473	488	rBV	134490	265084	12.17%	3.217%
2	7.234	742	748	763	rBV	92235	190187	8.73%	2.308%
3	7.604	803	811	828	rBV	282745	554898	25.47%	6.735%
4	8.074	883	891	899	rBV	61502	122785	5.64%	1.490%
5	8.397	937	946	959	rBV	241360	472584	21.69%	5.736%
6	9.243	1082	1090	1108	rBV	179249	387828	17.80%	4.707%
7	10.894	1362	1371	1385	rBV	99123	209221	9.60%	2.539%
8	13.332	1778	1786	1799	rBV	678197	1177094	54.03%	14.287%
9	14.713	2013	2021	2033	rBV2	193362	343910	15.79%	4.174%
10	16.200	2267	2274	2291	rBV	545458	943937	43.33%	11.457%
11	17.457	2481	2488	2502	rBV	270912	470796	21.61%	5.714%
12	20.054	2923	2930	2942	rBV	1527485	2178609	100.00%	26.443%
13	21.728	3208	3215	3226	rBV2	253091	483569	22.20%	5.869%
14	24.995	3760	3771	3785	rBV2	135910	438481	20.13%	5.322%


Sum of corrected areas: 8238983

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061416\
Data File : BG022340.D
Acq On : 14 Jun 2016 18:25
Operator : UM/SJ
Sample : H3427-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
W-42

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

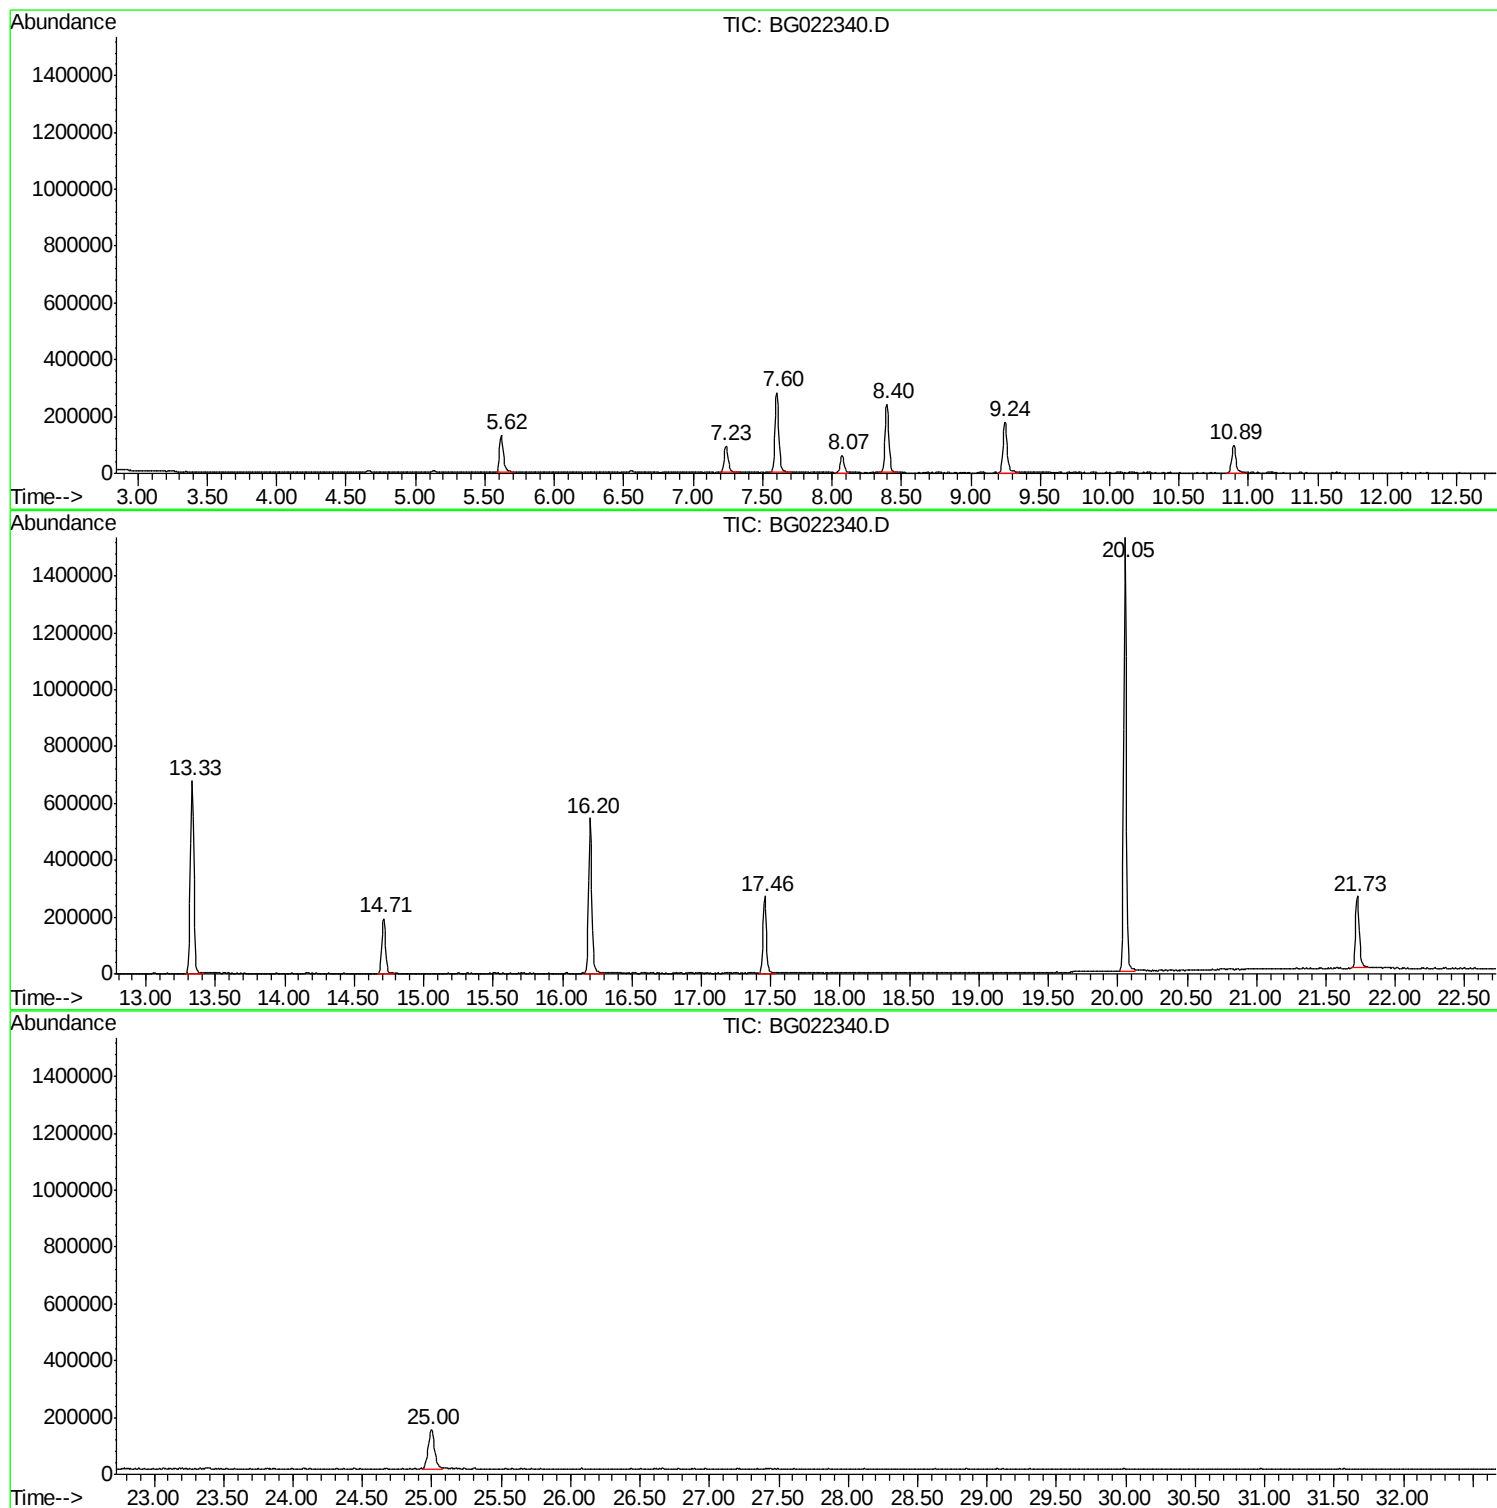

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061416\
Data File : BG022340.D
Acq On : 14 Jun 2016 18:25
Operator : UM/SJ
Sample : H3427-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
W-42










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.60 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.60	90.39 ng	554898	1,4-Dichlorobenzene-d4	8.07

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	12
4		1-Isoquinolinemethanol, .alpha.-...	191	C12H17NO	114608-92-3	10
5		Amphetaminil	250	C17H18N2	017590-01-1	10

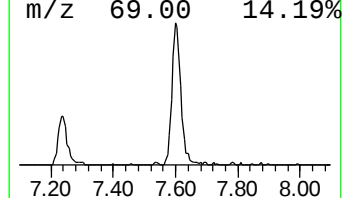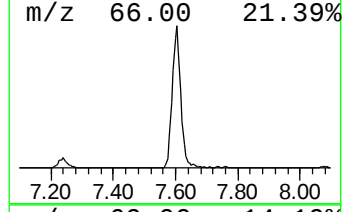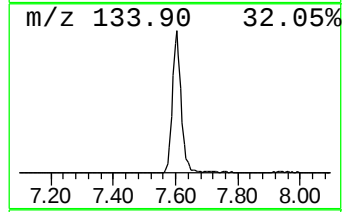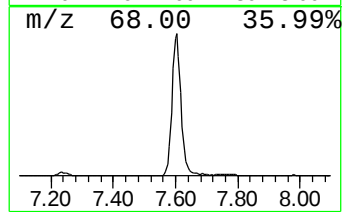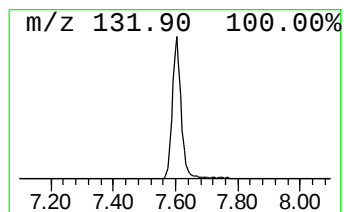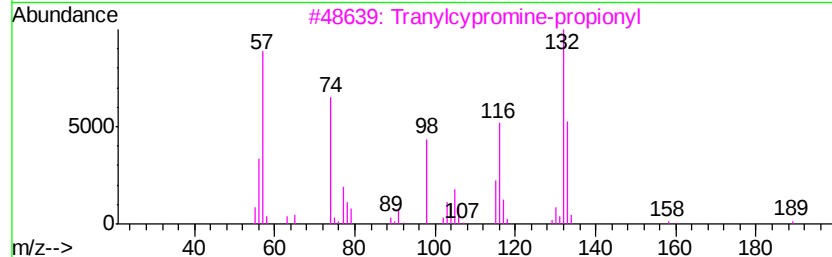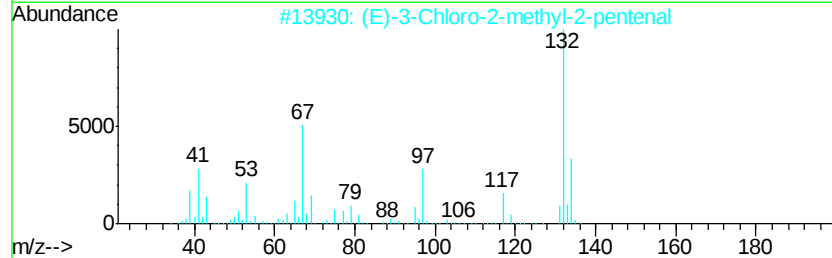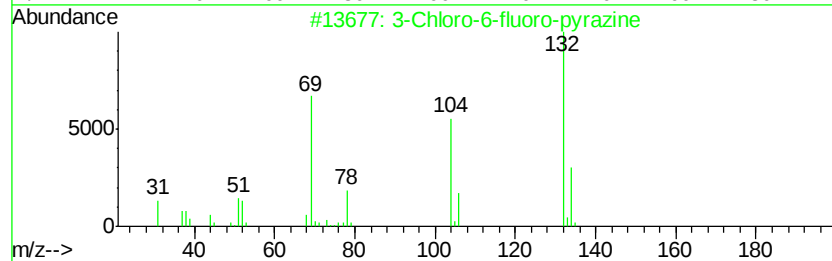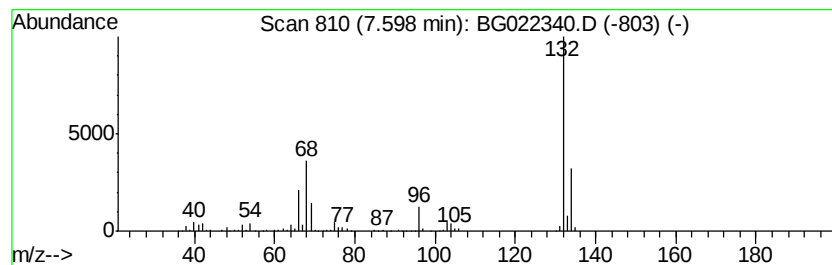

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061416\
Data File : BG022340.D
Acq On : 14 Jun 2016 18:25
Operator : UM/SJ
Sample : H3427-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
W-42

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.60	7.60	90.4	ng	554898	1	8.07	122785	20.0