

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061417\
 Data File : BG027447.D
 Acq On : 15 Jun 2017 11:37
 Operator : SJ/MA
 Sample : I3660-05
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jun 15 14:29:38 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG061417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 14 19:09:08 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.52	152	36211	20.00	ng	0.00
21) Naphthalene-d8	11.34	136	166695	20.00	ng	0.00
38) Acenaphthene-d10	15.11	164	113447	20.00	ng	0.00
63) Phenanthrene-d10	17.86	188	323350	20.00	ng	0.00
75) Chrysene-d12	22.23	240	364148	20.00	ng	0.00
86) Perylene-d12	25.88	264	259008	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	6.11	112	367122	143.28	ng	0.00
7) Phenol-d6	7.66	99	498643	126.63	ng	0.00
23) Nitrobenzene-d5	9.68	82	328616	100.51	ng	0.00
41) 2,4,6-Tribromophenol	16.59	330	299969	176.18	ng	0.00
44) 2-Fluorobiphenyl	13.73	172	758105	96.54	ng	0.00
78) Terphenyl-d14	20.44	244	1568836	110.42	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061417\
Data File : BG027447.D
Acq On : 15 Jun 2017 11:37
Operator : SJ/MA
Sample : I3660-05
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jun 15 14:29:38 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG061417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 14 19:09:08 2017
Response via : Initial Calibration

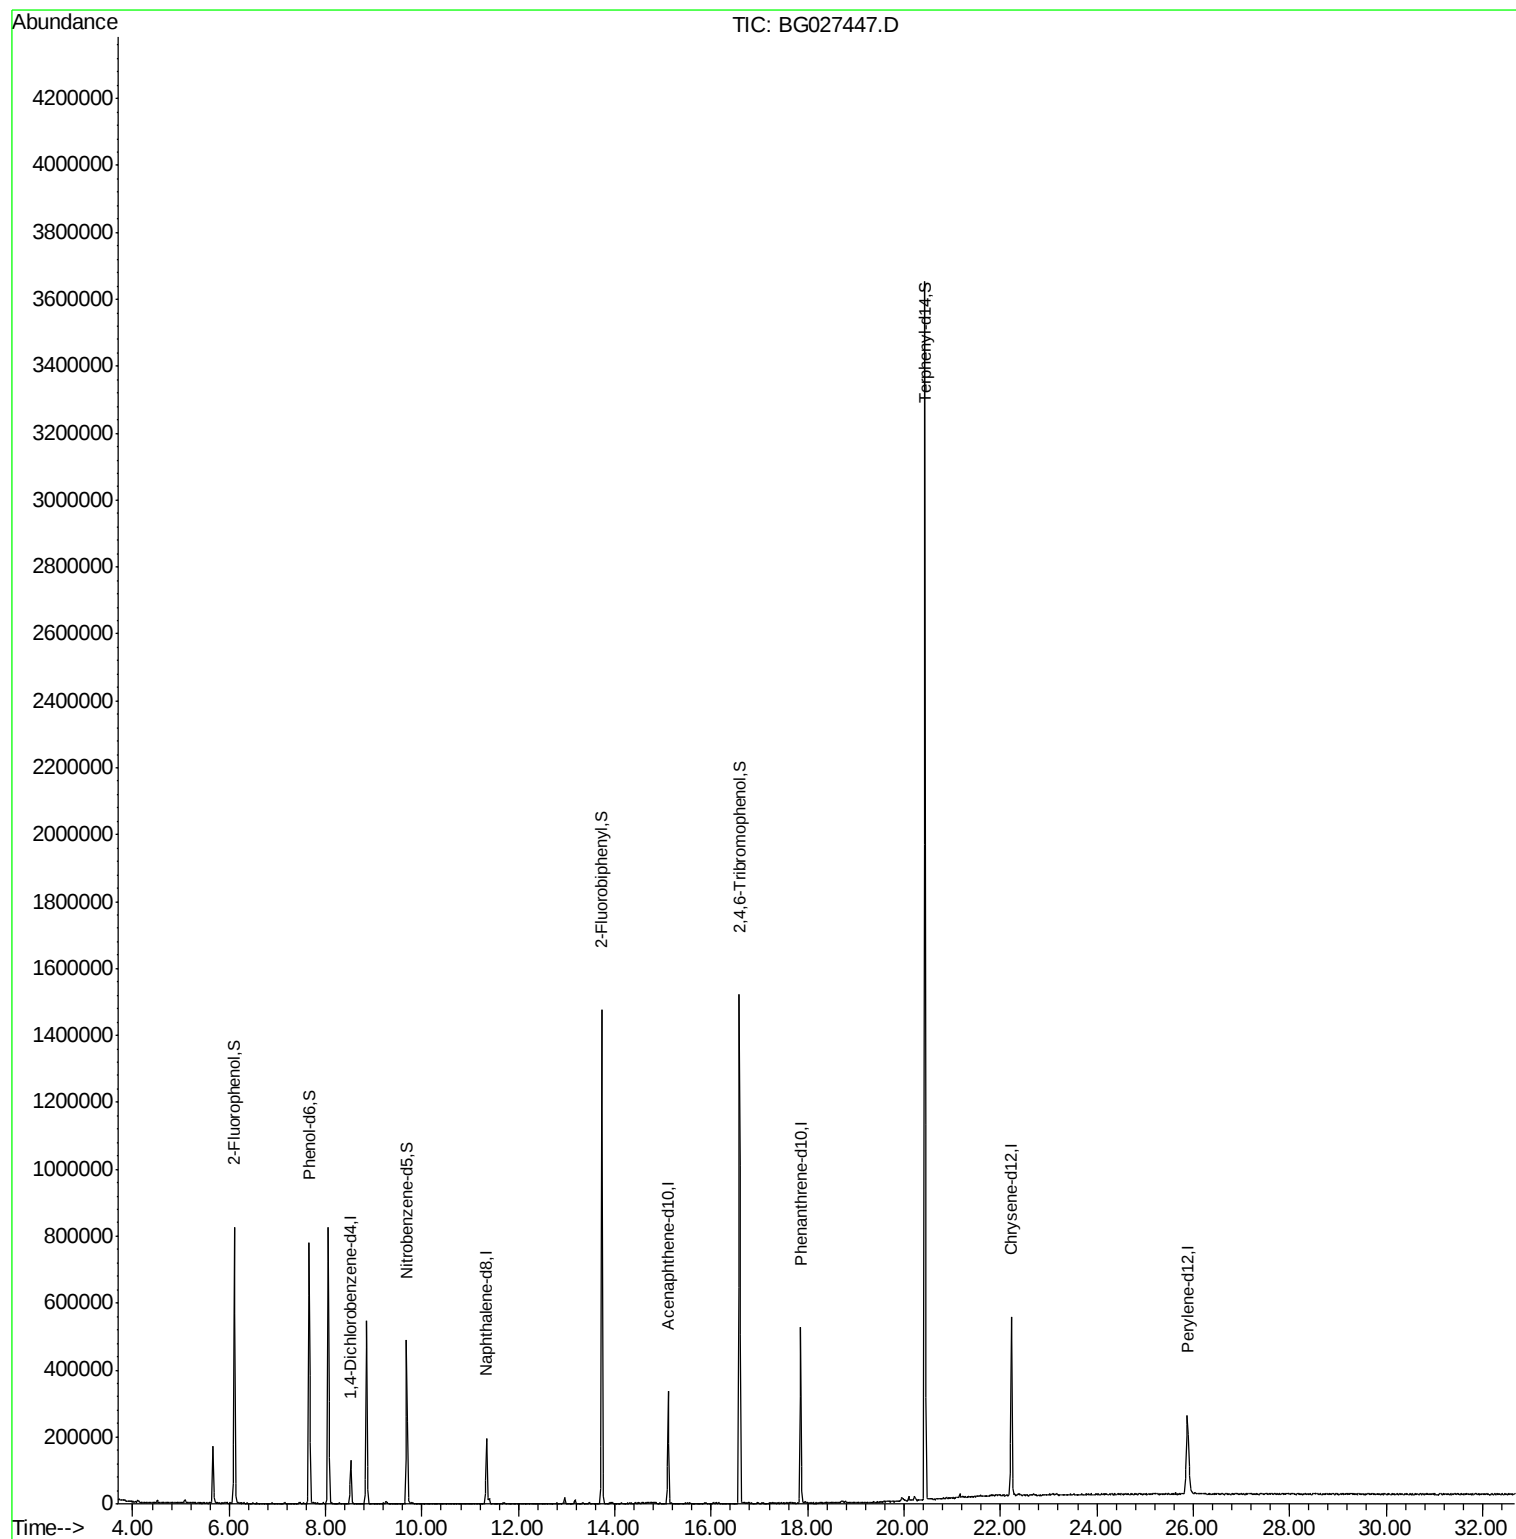




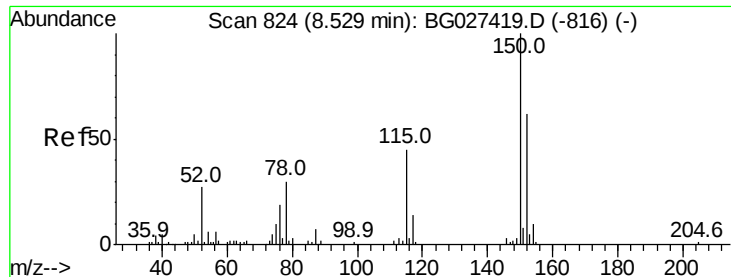


#1

1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.52 min Scan# 822
Delta R.T. -0.01 min
Lab File: BG027447.D
Acq: 15 Jun 2017 11:37

Instrument :
BNA_G
ClientSampleId :




Tot Ion:152 Resp: 36211
Ion Ratio Lower Upper
152 100
150 149.9 114.0 171.0
115 67.8 48.1 72.1

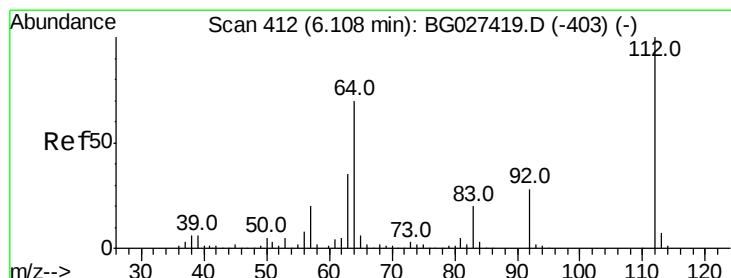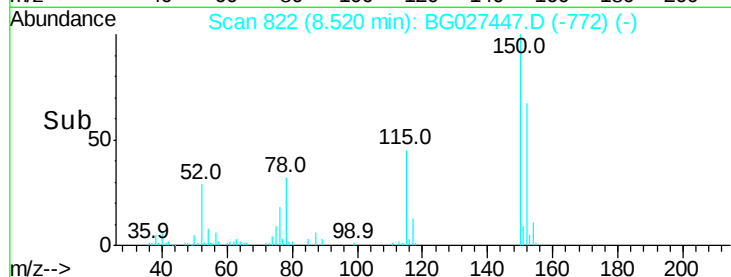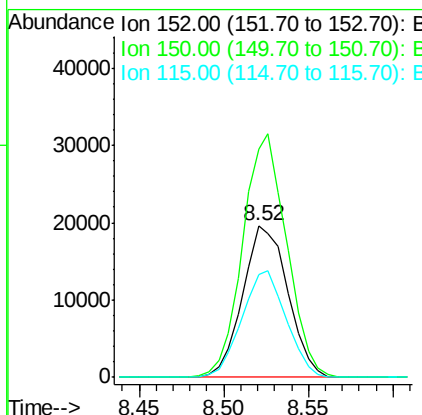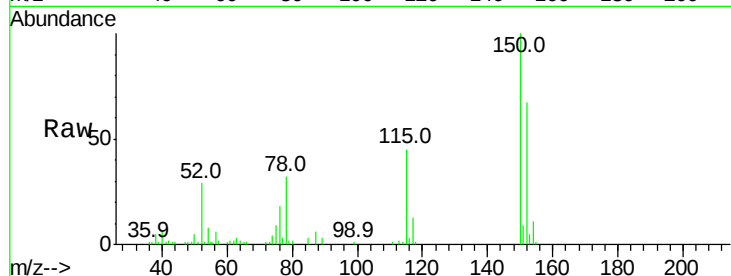


#5

2-Fluorophenol
Concen: 143.28 ng
RT: 6.11 min Scan# 411
Delta R.T. -0.00 min
Lab File: BG027447.D
Acq: 15 Jun 2017 11:37

Tgt Ion:112 Resp: 367122
Ion Ratio Lower Upper
112 100
64 73.6 61.8 92.6
63 37.5 37.2 55.8

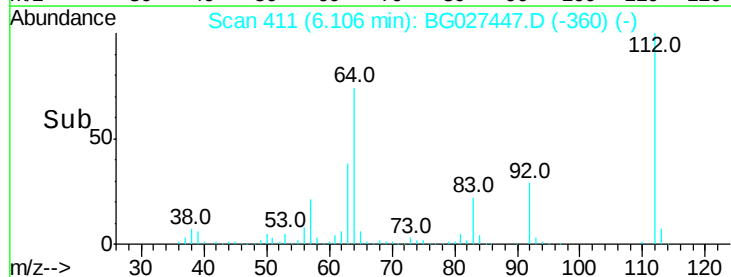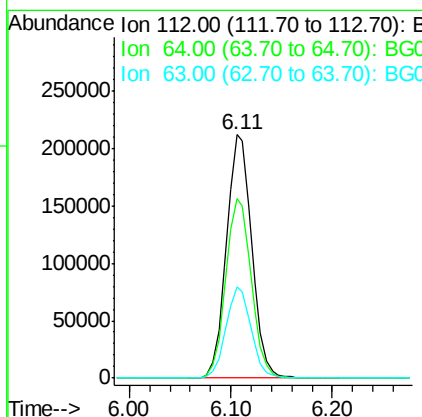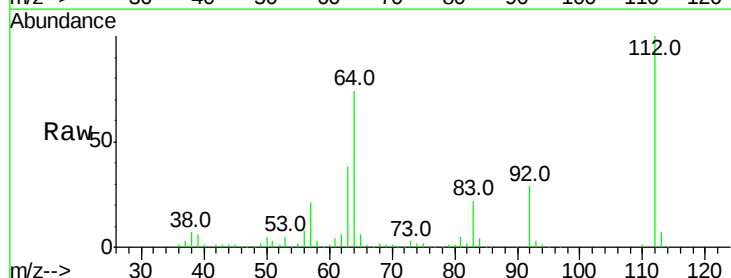

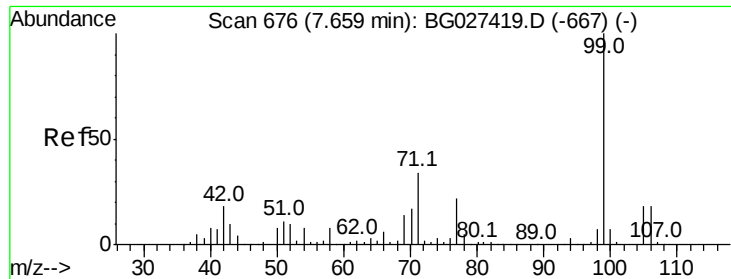

#7

Phenol-d6

Concen: 126.63 ng

RT: 7.66 min Scan# 676

Delta R.T. 0.00 min

Lab File: BG027447.D

Acq: 15 Jun 2017 11:37

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 498643

Ion Ratio Lower Upper




99 100

42 17.9 20.5 30.7#

71 33.8 37.6 56.4#

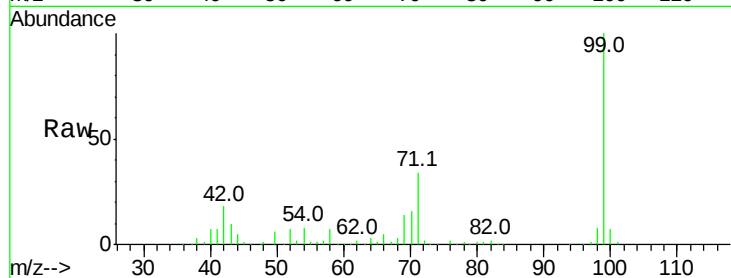

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

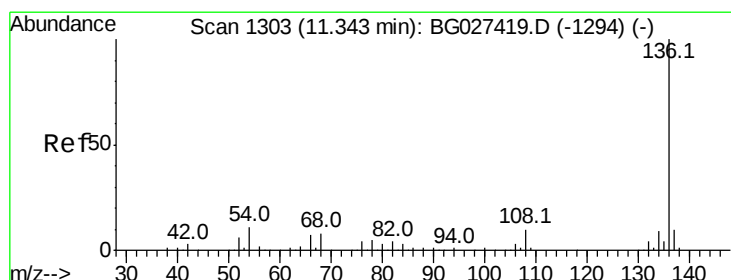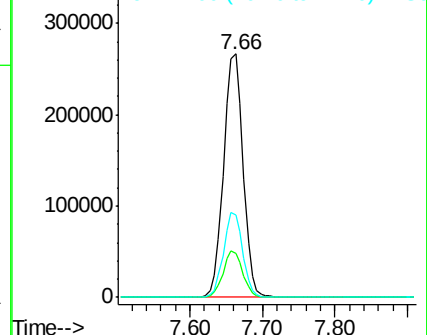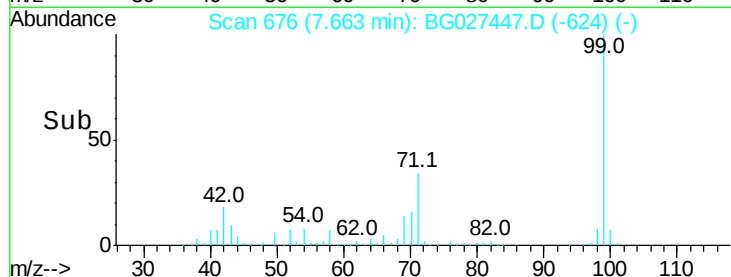

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 11.34 min Scan# 1302

Delta R.T. -0.00 min

Lab File: BG027447.D

Acq: 15 Jun 2017 11:37

Tgt Ion:136 Resp: 166695


Ion Ratio Lower Upper

136 100



137 11.0 8.9 13.3


54 12.3 9.3 13.9

68 8.5 5.1 7.7#

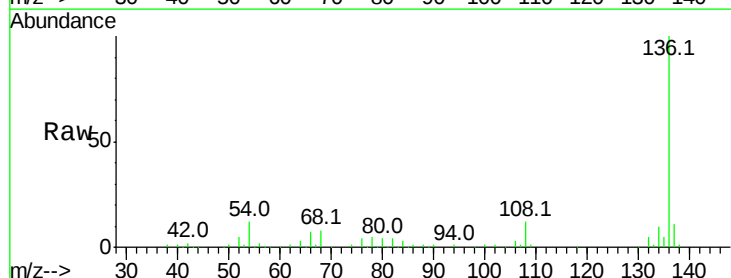

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

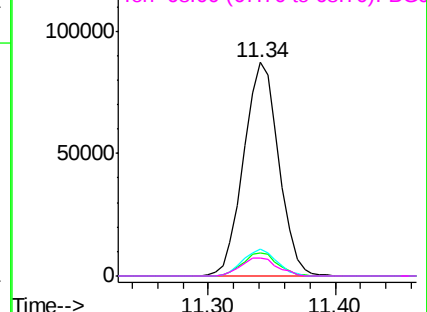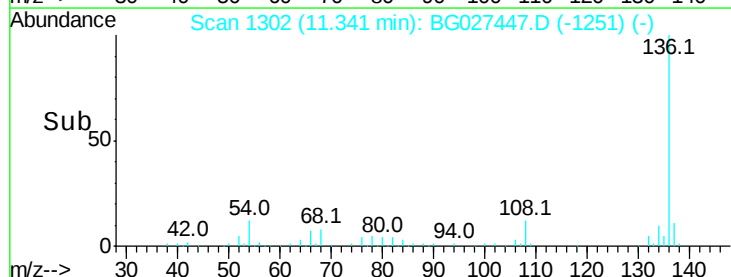


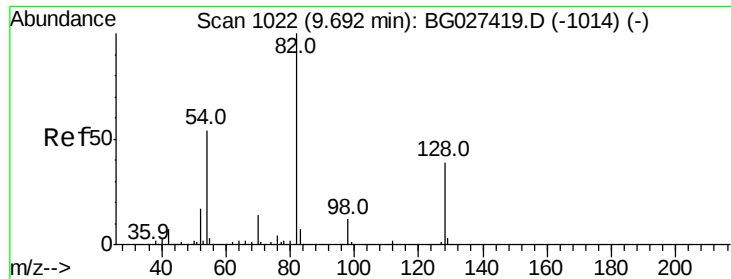




#23
 Nitrobenzene-d5
 Concen: 100.51 ng
 RT: 9.68 min Scan# 1020
 Delta R.T. -0.01 min
 Lab File: BG027447.D
 Acq: 15 Jun 2017 11:37

Instrument :
 BNA_G
 ClientSampled :

Tot Ion: 82 Resp: 328616
 Ion Ratio Lower Upper
 82 100
 128 36.8 26.4 39.6
 54 53.3 49.4 74.2

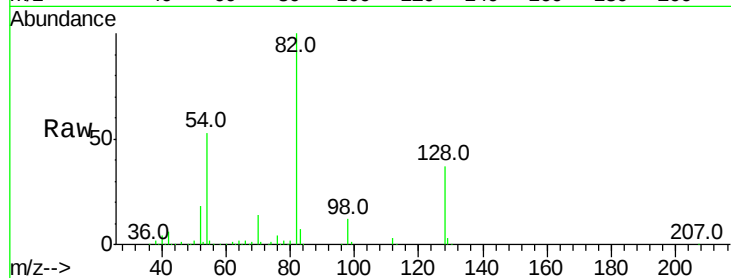


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

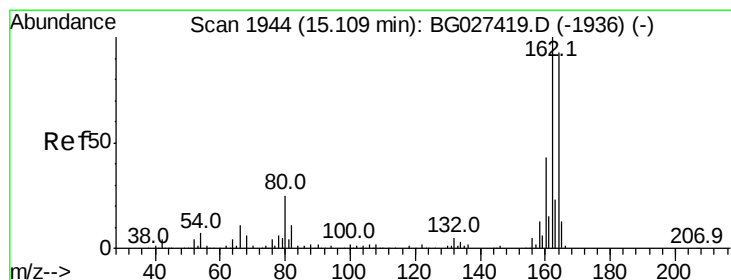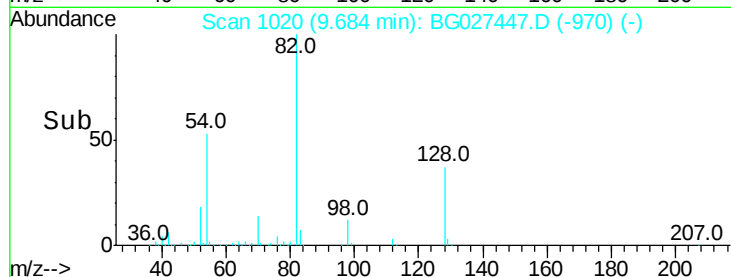
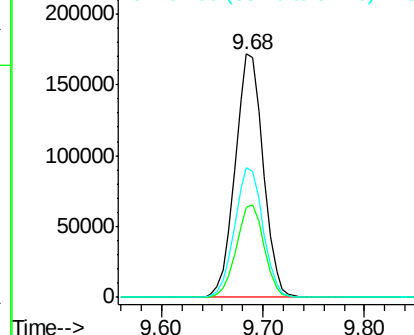



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 15.11 min Scan# 1943
 Delta R.T. -0.00 min
 Lab File: BG027447.D
 Acq: 15 Jun 2017 11:37

Tgt Ion:164 Resp: 113447
 Ion Ratio Lower Upper
 164 100
 162 100.4 85.1 127.7
 160 44.5 34.7 52.1

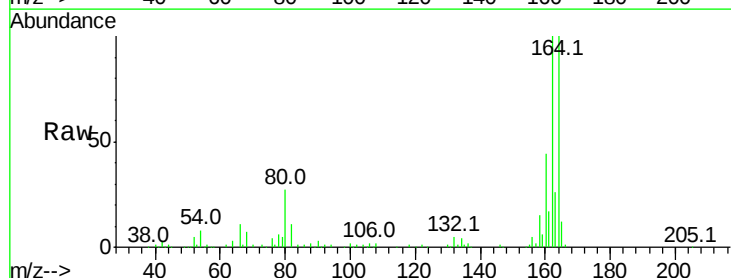

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC



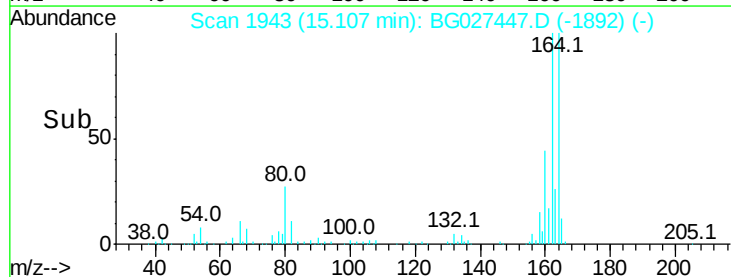
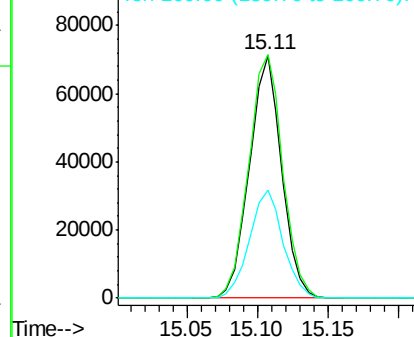


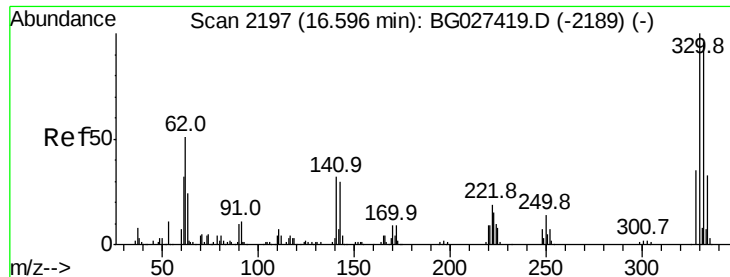

#41
 2,4,6-Tribromophenol
 Concen: 176.18 ng
 RT: 16.59 min Scan# 2196
 Delta R.T. -0.00 min
 Lab File: BG027447.D
 Acq: 15 Jun 2017 11:37




Instrument :
 BNA_G
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
330	100		
332	97.6	77.3	115.9
141	34.2	32.1	48.1

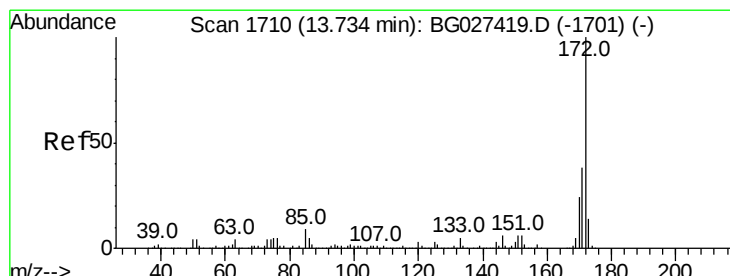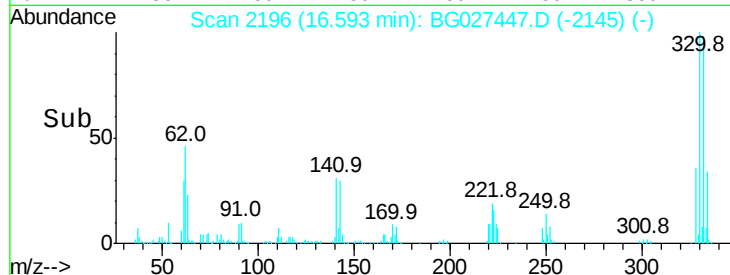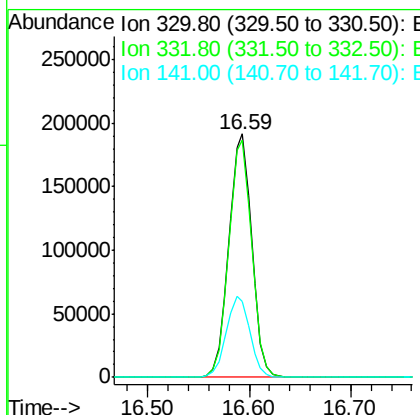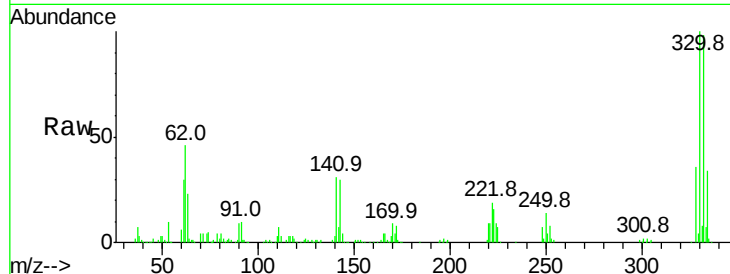

#44
 2-Fluorobiphenyl
 Concen: 96.54 ng
 RT: 13.73 min Scan# 1709
 Delta R.T. -0.00 min
 Lab File: BG027447.D
 Acq: 15 Jun 2017 11:37

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.7	32.2	48.2
170	24.5	21.8	32.6

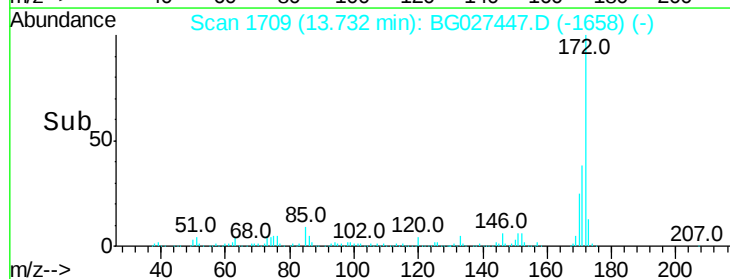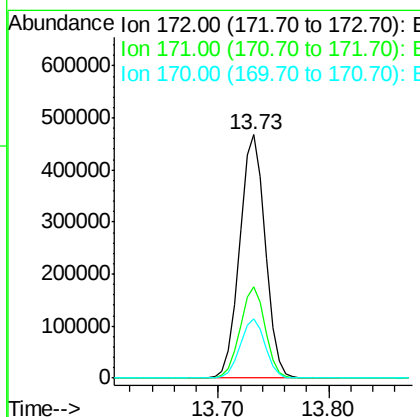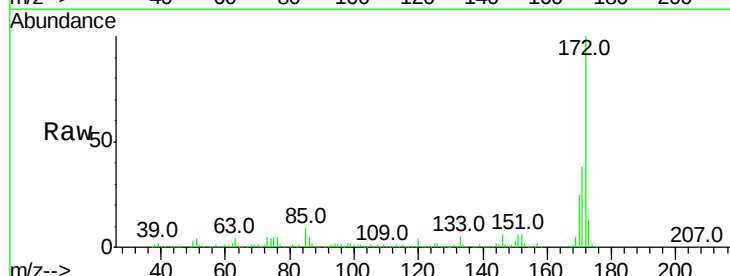


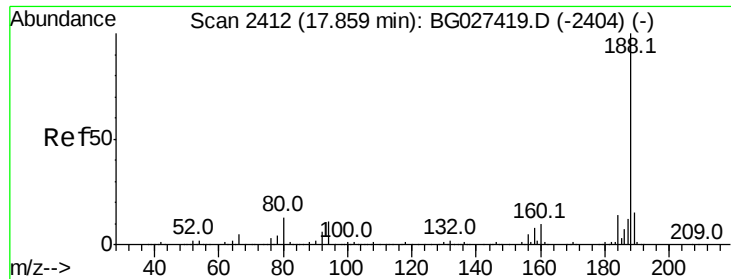




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.86 min Scan# 2411
Delta R.T. -0.00 min
Lab File: BG027447.D
Acq: 15 Jun 2017 11:37

Instrument :
BNA_G
ClientSampleId :

Tot Ion:188 Resp: 323350
Ion Ratio Lower Upper
188 100
94 11.1 5.8 8.8#
80 14.3 7.5 11.3#

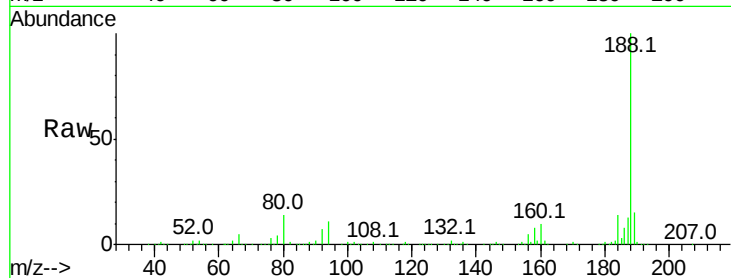


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

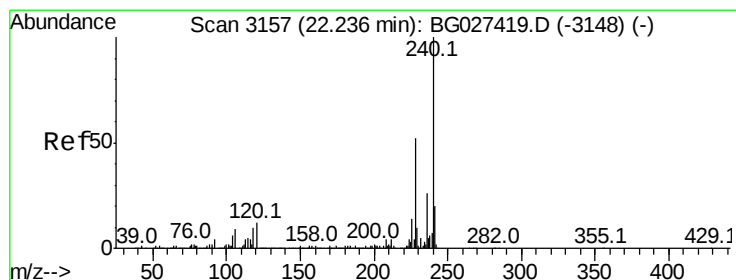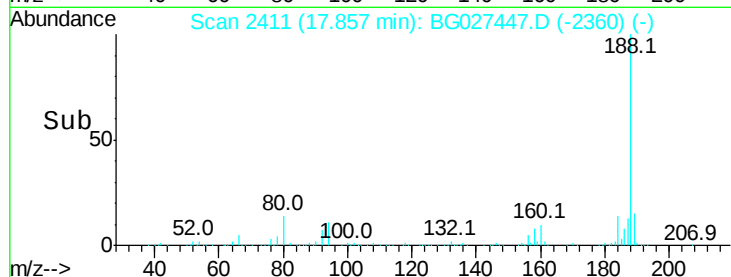
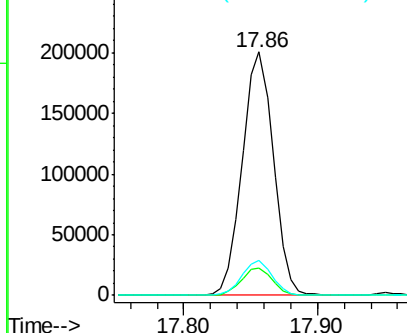



#75
Chrysene-d12
Concen: 20.00 ng
RT: 22.23 min Scan# 3155
Delta R.T. -0.01 min
Lab File: BG027447.D
Acq: 15 Jun 2017 11:37

Tgt Ion:240 Resp: 364148
Ion Ratio Lower Upper
240 100
120 12.2 5.7 8.5#
236 25.2 22.2 33.4

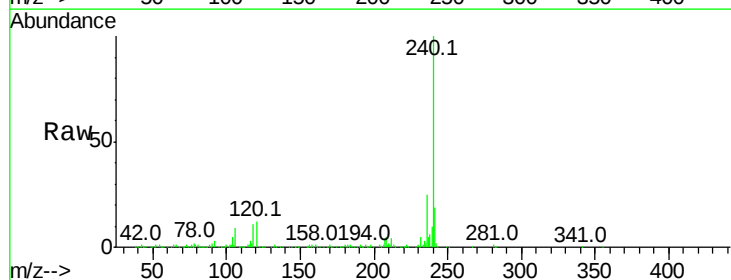

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

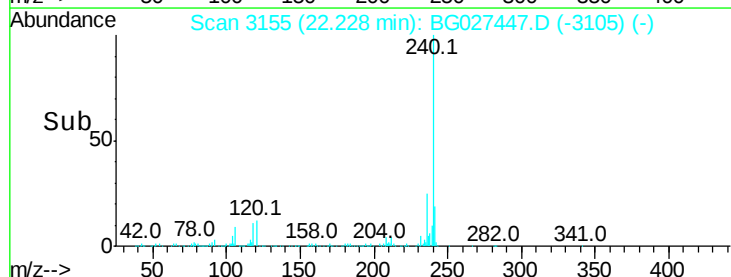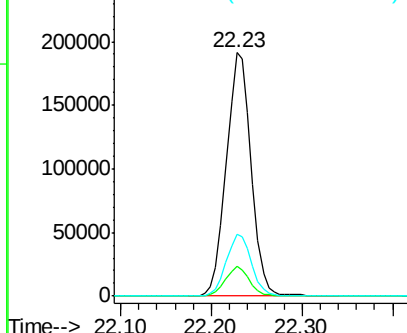

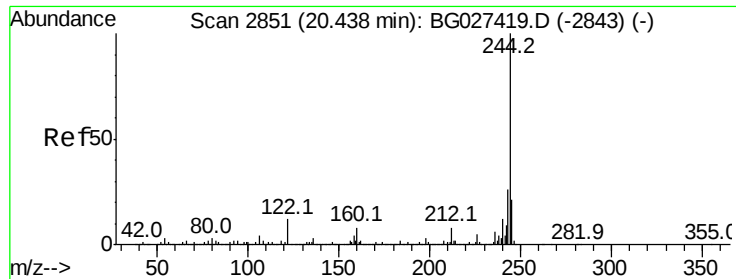

#78

Terphenyl-d14

Concen: 110.42 ng

RT: 20.44 min Scan# 2850

Delta R.T. -0.00 min

Lab File: BG027447.D

Acq: 15 Jun 2017 11:37


Instrument :

BNA_G

ClientSampled :

Tot Ion:244 Resp: 1568836




Ion	Ratio	Lower	Upper
244	100		
212	8.0	10.0	15.0#
122	11.9	8.6	12.8

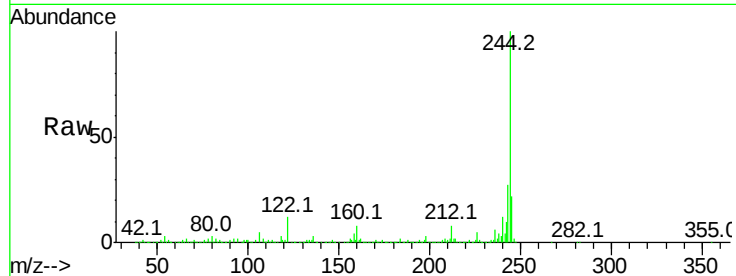

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

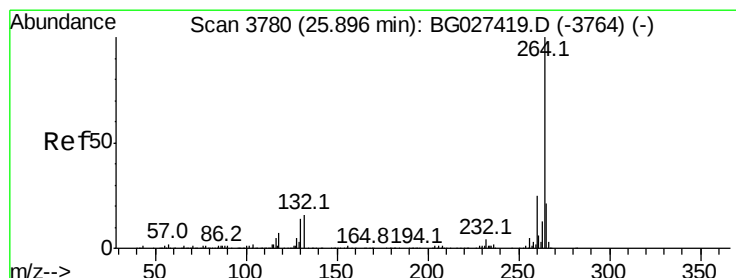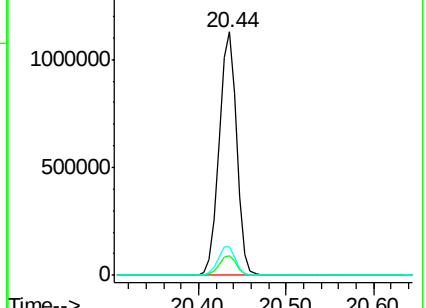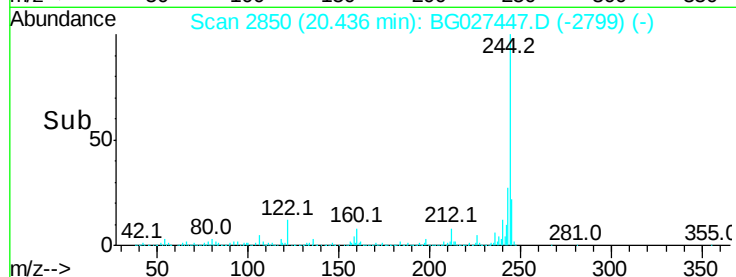

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.88 min Scan# 3776


Delta R.T. -0.02 min

Lab File: BG027447.D

Acq: 15 Jun 2017 11:37

Tgt Ion:264 Resp: 259008

Ion	Ratio	Lower	Upper
264	100		
260	24.2	21.8	32.8
265	20.6	18.2	27.4

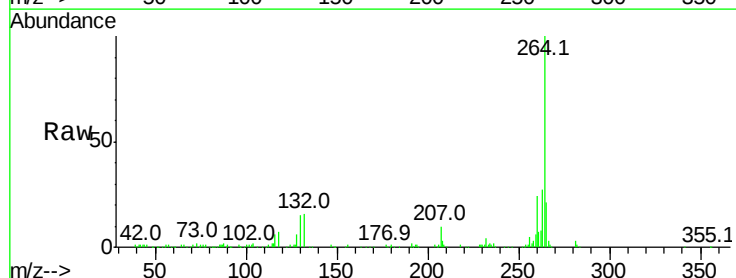

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

