
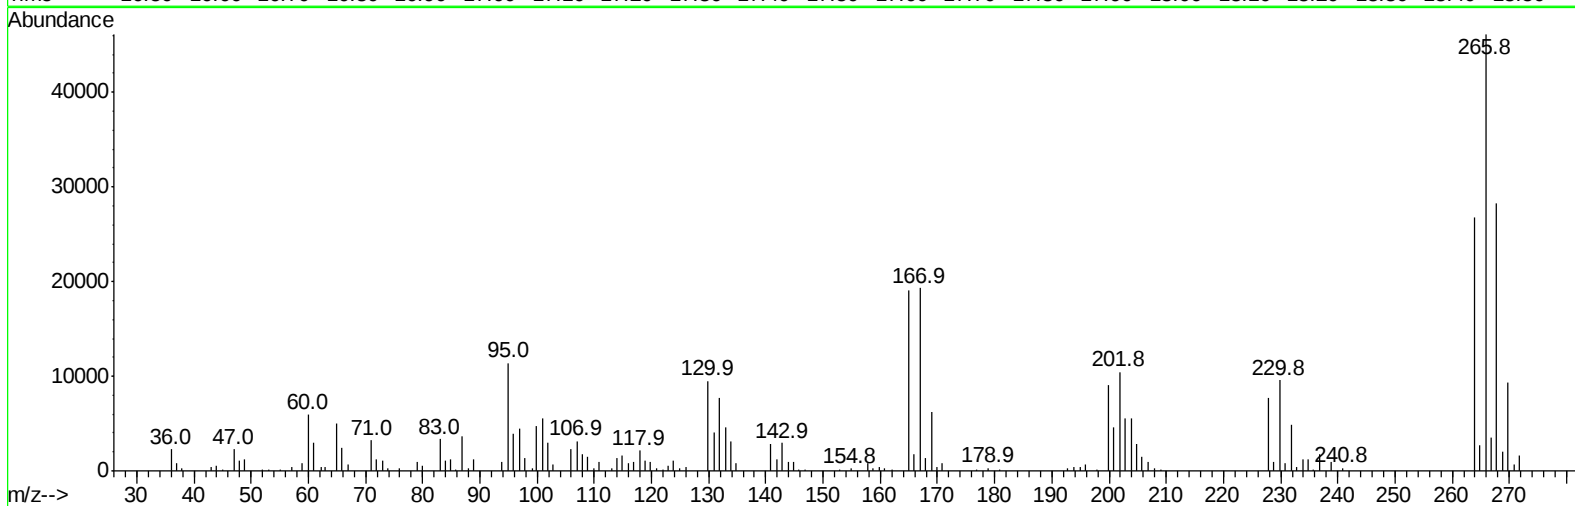


Data Path : Z:\HPCHEM1\BNA G\DATA\BG061417\  
Data File : BG027433.D  
Acq On : 15 Jun 2017 2:06  
Operator : SJ/MA  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 07:23:51 2017  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG061417.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jun 14 19:09:08 2017  
Response via : Initial Calibration

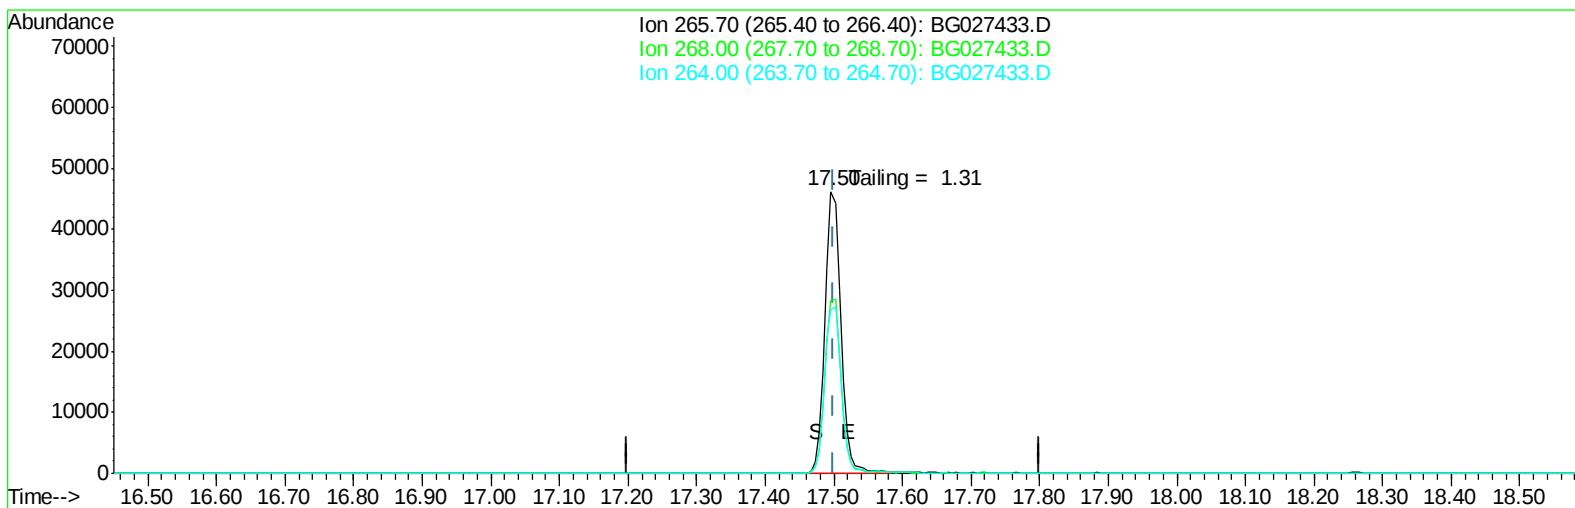

TIC: BG027433.D

(69) Pentachlorophenol (C)



17.496min (-0.004) 0.00ng

response 74027

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 60.70 | 61.20 |
| 264.00 | 62.60 | 58.07 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061417\  
Data File : BG027433.D  
Acq On : 15 Jun 2017 2:06  
Operator : SJ/MA  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 07:23:51 2017  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG061417.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jun 14 19:09:08 2017  
Response via : Initial Calibration

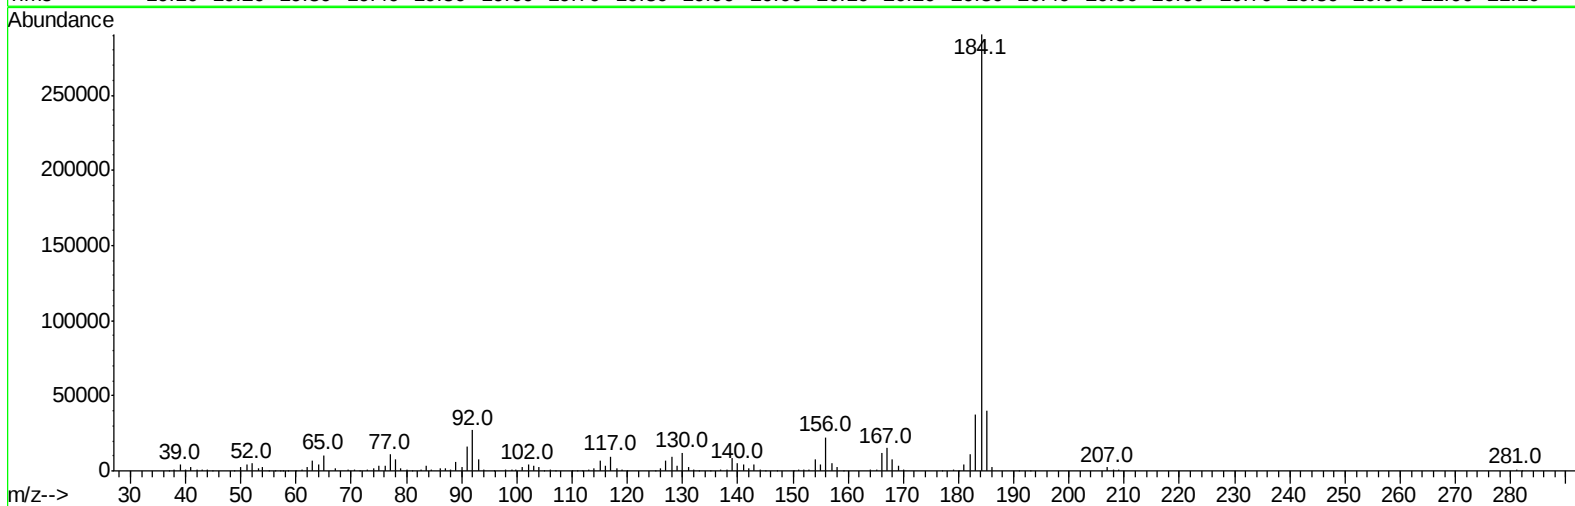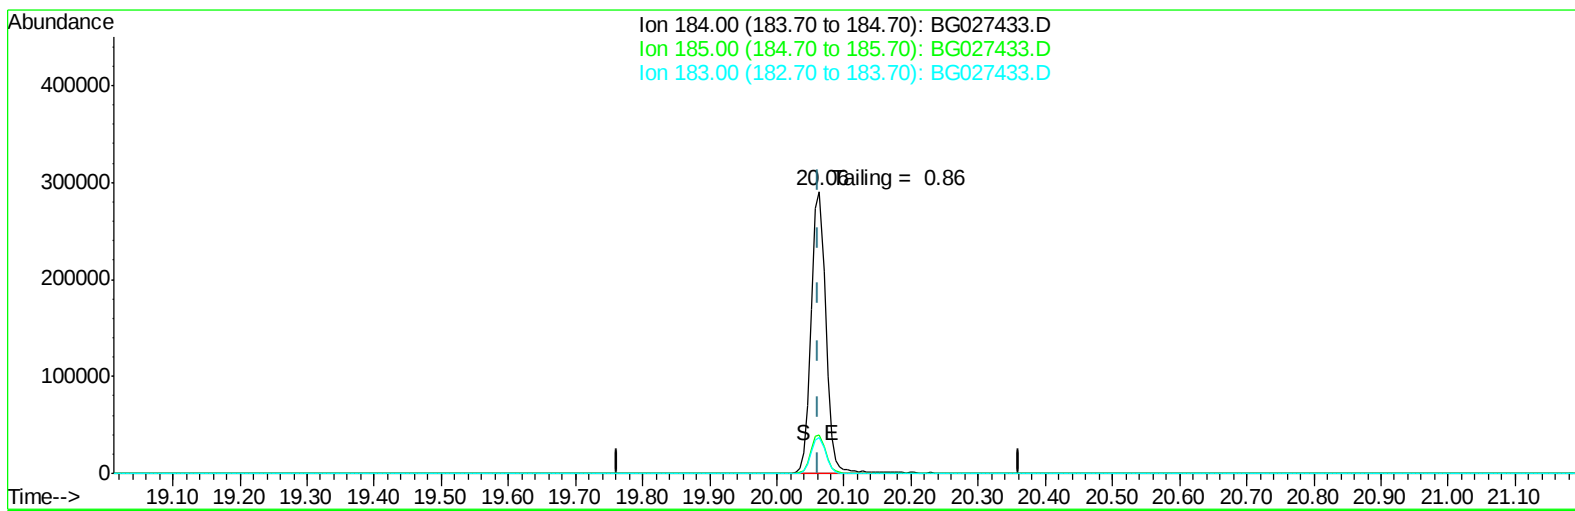

TIC: BG027433.D

(76) Benzidine

20.064min (+0.002) 0.00ng

response 430782

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.30 | 13.73 |
| 183.00 | 13.80 | 12.94 |
| 0.00   | 0.00  | 0.00  |